

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

11/7/2022 14:46

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.738	0.0	0.072	
ICB1	0.992	0.0	0.001	
CCV1	246.196	0.0	0.183	
CCB1	0.772	0.0	0.001	
PB148813BL	0.412	0.0	0.001	
PB148813BS	98.174	0.0	0.073	
LOWPB148813	10.176	0.0	0.008	102% (PO-110)
HIGHPB148813	494.543	0.0	0.367	99% (PO-110)
N5460-01	1.203	0.0	0.001	
N5460-01DUP	0.844	0.0	0.001	12
N5460-01MS	36.324	0.0	0.027	
N5460-01MSD	35.993	0.0	0.027	11/7/22
N5481-01	0.927	0.0	0.001	
CCV2	254.482	0.0	0.189	
CCB2	0.583	0.0	0.001	
PB148814BL	0.643	0.0	0.001	
PB148814BS	96.440	0.0	0.072	
N5431-01	0.867	0.0	0.001	
N5431-02	0.916	0.0	0.001	
N5431-03	0.669	0.0	0.001	
N5431-04	0.752	0.0	0.001	
N5431-04DUP	0.751	0.0	0.001	
N5431-04MS	36.337	0.0	0.027	
N5431-04MSD	35.228	0.0	0.027	
N5431-05	0.763	0.0	0.001	
CCV3	245.681	0.0	0.183	
CCB3	0.703	0.0	0.001	
N5431-06	3.350	0.0	0.003	
N5431-07	0.827	0.0	0.001	
N5431-08	0.957	0.0	0.001	
CCV4	247.557	0.0	0.184	
CCB4	0.884	0.0	0.001	

N 32
Mean 60.990
SD 114.4633
CV% 187.68

Aquakem v. 7.2AQ1

Results from time period:

Mon Nov 07 13:46:31 2022

Mon Nov 07 14:38:27 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time
0.OPPBCN	A	Total CN	P	0.6824	µg/l	11/7/2022 10:00:38
5.OPPBCN	A	Total CN	P	4.594	µg/l	11/7/2022 10:00:39
10PPBCN	A	Total CN	P	9.6093	µg/l	11/7/2022 10:00:40
50PPBCN	A	Total CN	P	49.1775	µg/l	11/7/2022 10:00:41
100PPBCN	A	Total CN	P	100.4695	µg/l	11/7/2022 10:00:42
250PPBCN	A	Total CN	P	250.934	µg/l	11/7/2022 10:00:43
500PPBCN	A	Total CN	P	499.5332	µg/l	11/7/2022 10:00:44
ICV1	S	Total CN	P	96.7379	µg/l	11/7/2022 13:46:32
ICB1	S	Total CN	P	0.992	µg/l	11/7/2022 13:46:33
CCV1	S	Total CN	P	246.1965	µg/l	11/7/2022 13:46:36
CCB1	S	Total CN	P	0.7717	µg/l	11/7/2022 13:46:38
PB148813BL	S	Total CN	P	0.4115	µg/l	11/7/2022 13:46:39
PB148813BS	S	Total CN	P	98.174	µg/l	11/7/2022 13:46:41
LOWPB148813	S	Total CN	P	10.1755	µg/l	11/7/2022 13:54:07
HIGHPB148813	S	Total CN	P	494.5433	µg/l	11/7/2022 13:54:09
N5460-01	S	Total CN	P	1.2027	µg/l	11/7/2022 13:54:10
N5460-01DUP	S	Total CN	P	0.8444	µg/l	11/7/2022 13:54:11
N5460-01MS	S	Total CN	P	36.3244	µg/l	11/7/2022 13:54:14
N5460-01MSD	S	Total CN	P	35.9931	µg/l	11/7/2022 13:54:15
N5481-01	S	Total CN	P	0.9265	µg/l	11/7/2022 13:54:16
CCV2	S	Total CN	P	254.4823	µg/l	11/7/2022 13:57:29
CCB2	S	Total CN	P	0.5833	µg/l	11/7/2022 13:57:30
PB148814BL	S	Total CN	P	0.6427	µg/l	11/7/2022 14:31:40
PB148814BS	S	Total CN	P	96.4396	µg/l	11/7/2022 14:31:41
N5431-01	S	Total CN	P	0.8666	µg/l	11/7/2022 14:31:42
N5431-02	S	Total CN	P	0.9158	µg/l	11/7/2022 14:31:43
N5431-03	S	Total CN	P	0.6688	µg/l	11/7/2022 14:31:44
N5431-04	S	Total CN	P	0.7521	µg/l	11/7/2022 14:31:45
N5431-04DUP	S	Total CN	P	0.7505	µg/l	11/7/2022 14:31:46
N5431-04MS	S	Total CN	P	36.3372	µg/l	11/7/2022 14:31:49
N5431-04MSD	S	Total CN	P	35.2281	µg/l	11/7/2022 14:31:50
N5431-05	S	Total CN	P	0.7634	µg/l	11/7/2022 14:38:19
CCV3	S	Total CN	P	245.6812	µg/l	11/7/2022 14:38:20
CCB3	S	Total CN	P	0.703	µg/l	11/7/2022 14:38:21
N5431-06	S	Total CN	P	3.3503	µg/l	11/7/2022 14:38:22
N5431-07	S	Total CN	P	0.8273	µg/l	11/7/2022 14:38:23
N5431-08	S	Total CN	P	0.9572	µg/l	11/7/2022 14:38:24
CCV4	S	Total CN	P	247.5567	µg/l	11/7/2022 14:38:25
CCB4	S	Total CN	P	0.8836	µg/l	11/7/2022 14:38:26

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

11/7/2022 10:02


Test Total CN

Accepted 11/7/2022 10:02

Factor 1350
Bias 0

Coeff. of det. 0.999987

Errors

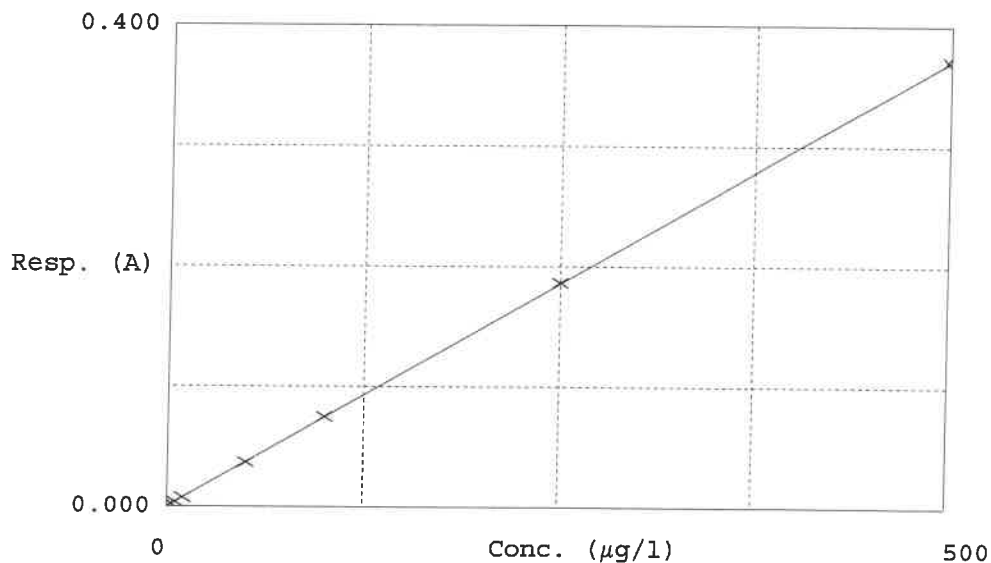

	Calibrator	Response	Calc. con.	Conc.	^{Re} Errors
1	0.0PPBCN	0.001	0.6824	0.0000	-
2	5.0PPBCN	0.004	4.5940	5.0000	-8.1
3	10PPBCN	0.008	9.6093	10.0000	-3.9
4	50PPBCN	0.037	49.1775	50.0000	-1.6
5	100PPBCN	0.075	100.4695	100.0000	0.5
6	250PPBCN	0.186	250.9340	250.0000	0.4
7	500PPBCN	0.371	499.5332	500.0000	-0.1

12
11/07/22