

LB177823

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

11/9/2022 15:51

Reviewed by : 12

Instrument ID : Konelab

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.055	0.0	0.110	
ICB1	0.005	0.0	0.007	
CCV1	1.059	0.0	0.110	
CCB1	0.004	0.0	0.007	
PB148934BL	0.004	0.0	0.007	
PB148934BS	1.066	0.0	0.111	
N4955-12	0.023	0.0	0.009	
N5534-01	0.048	0.0	0.011	
N5534-01DUP	0.049	0.0	0.011	
N5534-01MS	1.107	0.0	0.115	
N5534-01MSD	1.099	0.0	0.114	
CCV2	1.062	0.0	0.110	
CCB2	0.003	0.0	0.007	

N 13
Mean 0.506
SD 0.5479
CV% 108.17

Aquakem v. 7.2AQ1

Results from time period:

Wed Nov 09 14:37:08 2022

Wed Nov 09 15:49:43 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0031	mg/l	11/9/2022 14:37:08	
0.05PPM	A	Phenolics-	P	0.0547	mg/l	11/9/2022 14:37:09	
0.1PPM	A	Phenolics-	P	0.1033	mg/l	11/9/2022 14:37:10	
0.25PPM	A	Phenolics-	P	0.2561	mg/l	11/9/2022 14:37:11	
0.50PPM	A	Phenolics-	P	0.4974	mg/l	11/9/2022 14:37:12	
1.0PPM	A	Phenolics-	P	0.9715	mg/l	11/9/2022 14:37:13	
2.0PPM	A	Phenolics-	P	2.0139	mg/l	11/9/2022 14:37:14	
ICV1	S	Phenolics-	P	1.055	mg/l	11/9/2022 15:46:55	
ICB1	S	Phenolics-	P	0.0049	mg/l	11/9/2022 15:46:56	
CCV1	S	Phenolics-	P	1.0592	mg/l	11/9/2022 15:46:57	
CCB1	S	Phenolics-	P	0.0041	mg/l	11/9/2022 15:46:58	
PB148934BL	S	Phenolics-	P	0.0042	mg/l	11/9/2022 15:46:59	
PB148934BS	S	Phenolics-	P	1.0657	mg/l	11/9/2022 15:47:00	
N4955-12	S	Phenolics-	P	0.0228	mg/l	11/9/2022 15:47:01	
N5534-01	S	Phenolics-	P	0.0483	mg/l	11/9/2022 15:47:02	
N5534-01DUP	S	Phenolics-	P	0.049	mg/l	11/9/2022 15:47:03	
N5534-01MS	S	Phenolics-	P	1.1067	mg/l	11/9/2022 15:47:04	
N5534-01MSD	S	Phenolics-	P	1.0988	mg/l	11/9/2022 15:47:05	
CCV2	S	Phenolics-	P	1.0621	mg/l	11/9/2022 15:47:06	
CCB2	S	Phenolics-	P	0.0031	mg/l	11/9/2022 15:49:43	

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

11/9/2022 14:41

Reviewed by : 12

Instrument ID : Konelab


Test Phenolics-

Accepted 11/9/2022 14:41

Factor 10.25
Bias 0.007

Coeff. of det. 0.999653

Errors

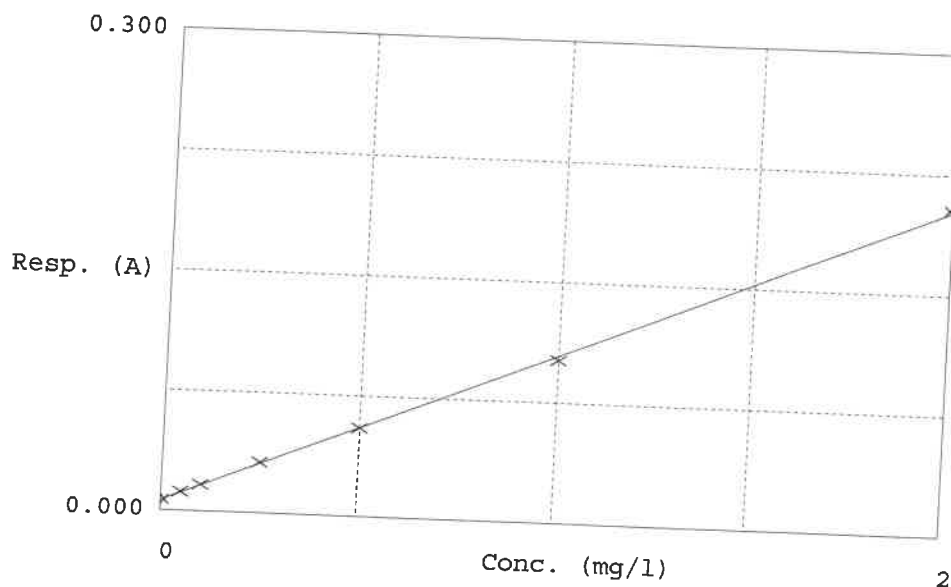

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.007	0.0031	0.0000	
2	Phenol-2	0.012	0.0547	0.0500	
3	Phenol-2	0.017	0.1033	0.1000	9.4
4	Phenol-2	0.032	0.2561	0.2500	3.3
5	Phenol-2	0.055	0.4974	0.5000	2.4
6	Phenol-2	0.101	0.9715	1.0000	-0.5
7	Phenol-2	0.203	2.0139	2.0000	-2.9
					0.7

12
11/9/22