

LB122825

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092Reviewed by : 12 Instrument ID : Konelab

11/9/2022 16:26

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.060	0.0	0.110	
ICB1	0.038	0.0	0.010	
CCV1	1.064	0.0	0.110	
CCB1	0.005	0.0	0.007	
PB148935BL	0.004	0.0	0.007	
PB148935BS	1.057	0.0	0.110	
N4955-03	0.024	0.0	0.009	
PB148937BL	0.004	0.0	0.007	
PB148937BS	1.060	0.0	0.110	
N4955-09	0.024	0.0	0.009	
CCV2	1.064	0.0	0.110	
CCB2	0.001	0.0	0.007	

N	12
Mean	0.450
SD	0.5391
CV%	119.67

Aquakem v. 7.2AQ1

Results from time period:

Wed Nov 09 16:15:16 2022

Wed Nov 09 16:25:29 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0031	mg/l	11/9/2022 14:37:08	
0.05PPM	A	Phenolics-	P	0.0547	mg/l	11/9/2022 14:37:09	
0.1PPM	A	Phenolics-	P	0.1033	mg/l	11/9/2022 14:37:10	
0.25PPM	A	Phenolics-	P	0.2561	mg/l	11/9/2022 14:37:11	
0.50PPM	A	Phenolics-	P	0.4974	mg/l	11/9/2022 14:37:12	
1.0PPM	A	Phenolics-	P	0.9715	mg/l	11/9/2022 14:37:13	
2.0PPM	A	Phenolics-	P	2.0139	mg/l	11/9/2022 14:37:14	
ICV1	S	Phenolics-	P	1.0605	mg/l	11/9/2022 16:15:17	
ICB1	S	Phenolics-	P	0.0379	mg/l	11/9/2022 16:15:18	
CCV1	S	Phenolics-	P	1.0638	mg/l	11/9/2022 16:15:20	
CCB1	S	Phenolics-	P	0.0054	mg/l	11/9/2022 16:15:22	
PB148935BL	S	Phenolics-	P	0.0039	mg/l	11/9/2022 16:15:25	
PB148935BS	S	Phenolics-	P	1.0569	mg/l	11/9/2022 16:15:26	
N4955-03	S	Phenolics-	P	0.0239	mg/l	11/9/2022 16:25:19	
PB148937BL	S	Phenolics-	P	0.0043	mg/l	11/9/2022 16:25:20	
PB148937BS	S	Phenolics-	P	1.06	mg/l	11/9/2022 16:25:22	
N4955-09	S	Phenolics-	P	0.0235	mg/l	11/9/2022 16:25:25	
CCV2	S	Phenolics-	P	1.0639	mg/l	11/9/2022 16:25:26	
CCB2	S	Phenolics-	P	0.0014	mg/l	11/9/2022 16:25:28	

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

11/9/2022 14:41


Test Phenolics-

Accepted 11/9/2022 14:41

Factor 10.25
Bias 0.007

Coeff. of det. 0.999653

Errors

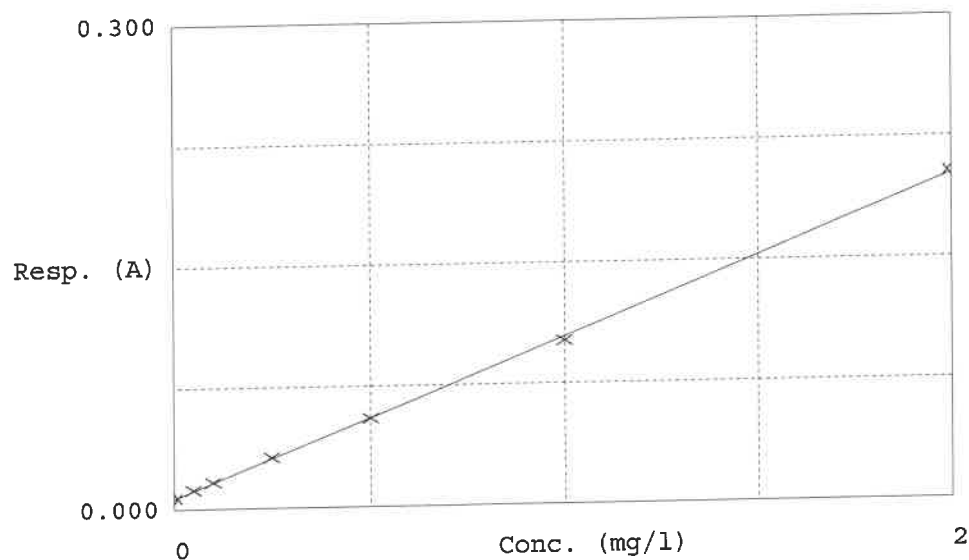

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.007	0.0031	0.0000	
2	Phenol-2	0.012	0.0547	0.0500	9.4
3	Phenol-2	0.017	0.1033	0.1000	3.3
4	Phenol-2	0.032	0.2561	0.2500	2.4
5	Phenol-2	0.055	0.4974	0.5000	-0.5
6	Phenol-2	0.101	0.9715	1.0000	-2.9
7	Phenol-2	0.203	2.0139	2.0000	0.7

12
11/9/22