


LB122866

7470A

INSTRUMENT ID: CV1

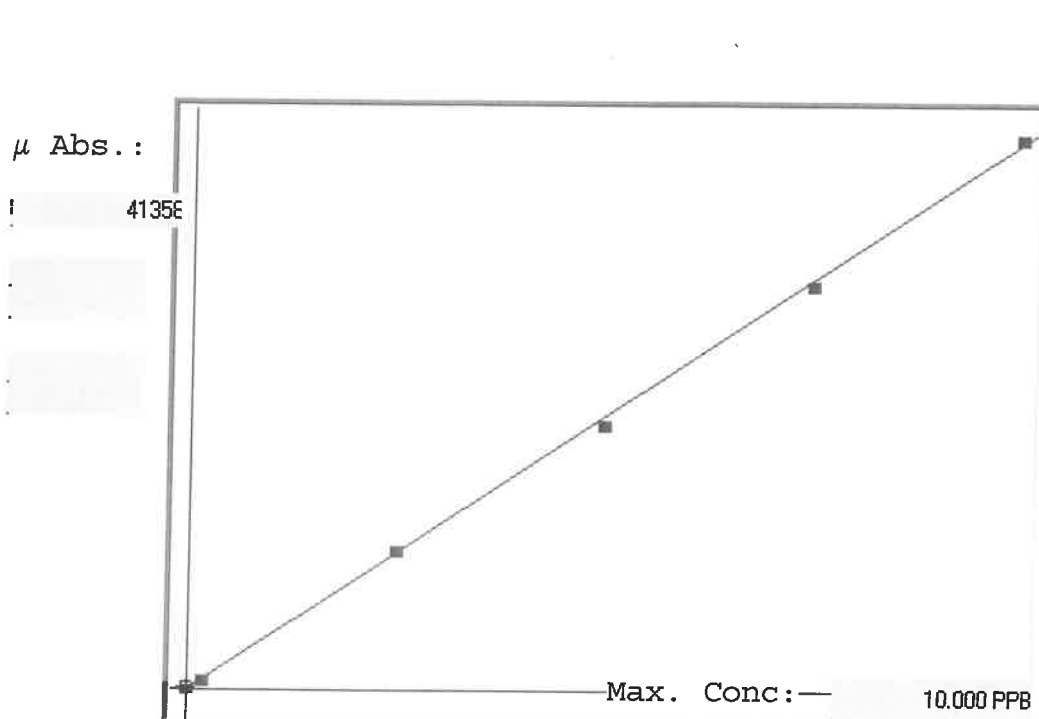

Linear

A= 0.0000e+000

B= 2.4398e-004

C= 4.6378e-003

Rho= 0.9998005

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.048	0.048	179	0.000	179					
0.2	0.200	0.189	-0.011	756	0.0 %	756					-6
2.5	2.500	2.554	0.054	10449	0.0 %	10449					2
5.0	5.000	4.887	-0.113	20012	0.0 %	20012					-2
7.5	7.500	7.426	-0.074	30419	0.0 %	30419					-1
10.0	10.000	10.095	0.095	41358	0.0 %	41358					1

LB122866 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 13 Nov 2022 14:44:41

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	179	-	0.0000	7470A	PPB	13 Nov 2022 14:52:10	S	Std
0.2 - 1	50.2	756	-	0.2000	7470A	PPB	13 Nov 2022 14:54:28	S	Std
2.5 - 1	52.5	10449	-	2.5000	7470A	PPB	13 Nov 2022 14:56:45	S	Std
5.0 - 1	55	20012	-	5.0000	7470A	PPB	13 Nov 2022 14:59:02	S	Std
7.5 - 1	57.5	30419	-	7.5000	7470A	PPB	13 Nov 2022 15:01:18	S	Std
10.0 - 1	510	41358	-	10.0000	7470A	PPB	13 Nov 2022 15:03:34	S	Std
ICV19 - 1	ICV19	17032	4.1601	-	7470A	PPB	13 Nov 2022 15:06:21	U	SMPL
ICB19 - 1	ICB19	70	0.0217	-	7470A	PPB	13 Nov 2022 15:08:36	U	SMPL
CCV15 - 1	CCV15	21059	5.1426	-	7470A	PPB	13 Nov 2022 15:10:51	U	SMPL
CCB15 - 1	CCB15	-97	-0.0190	-	7470A	PPB	13 Nov 2022 15:13:06	U	SMPL
CRA - 1	CRA	720	0.1803	-	7470A	PPB	13 Nov 2022 15:18:09	U	SMPL
HighStd - 1	HighStd	41504	10.1308	-	7470A	PPB	13 Nov 2022 15:20:24	U	SMPL
ChkStd - 1	ChkStd	28686	7.0035	-	7470A	PPB	13 Nov 2022 15:22:39	U	SMPL
PB148993BL - 1	PBW	11	0.0073	-	7470A	PPB	13 Nov 2022 15:24:55	U	SMPL
PB148993BS - 1	LCSW	15782	3.8551	-	7470A	PPB	13 Nov 2022 15:27:11	U	SMPL
N5530-02 - 1	WC-13	0	0.0046	-	7470A	PPB	13 Nov 2022 15:29:28	U	SMPL
N5530-04 - 1	WC-12	-10	0.0022	-	7470A	PPB	13 Nov 2022 15:31:44	U	SMPL
N5530-06 - 1	WC-11	-13	0.0015	-	7470A	PPB	13 Nov 2022 15:34:01	U	SMPL
N5530-08 - 1	WC-10	-35	-0.0039	-	7470A	PPB	13 Nov 2022 15:36:18	U	SMPL
N5530-10 - 1	WC-09	-20	-0.0002	-	7470A	PPB	13 Nov 2022 15:38:33	U	SMPL
CCV16 - 1	CCV16	20762	5.0702	-	7470A	PPB	13 Nov 2022 15:40:49	U	SMPL
CCB16 - 1	CCB16	-69	-0.0122	-	7470A	PPB	13 Nov 2022 15:43:04	U	SMPL
N5531-03 - 1	WC-08	35	0.0132	-	7470A	PPB	13 Nov 2022 15:45:20	U	SMPL
N5531-05 - 1	WC-07	78	0.0237	-	7470A	PPB	13 Nov 2022 15:47:35	U	SMPL
N5531-07 - 1	WC-34	-9	0.0024	-	7470A	PPB	13 Nov 2022 15:49:50	U	SMPL
N5531-09 - 1	WC-33	-13	0.0015	-	7470A	PPB	13 Nov 2022 15:52:06	U	SMPL
N5531-11 - 1	WC-30	-18	0.0002	-	7470A	PPB	13 Nov 2022 15:54:21	U	SMPL
N5531-14 - 1	WC-28	29	0.0117	-	7470A	PPB	13 Nov 2022 15:56:37	U	SMPL
N5531-16 - 1	WC-27	-20	-0.0002	-	7470A	PPB	13 Nov 2022 15:58:54	U	SMPL
N5531-18 - 1	WC-26	11	0.0073	-	7470A	PPB	13 Nov 2022 16:01:11	U	SMPL
N5553-01 - 1	COMP-1	28	0.0115	-	7470A	PPB	13 Nov 2022 16:03:28	U	SMPL
N5553-02 - 1	8258	-3	0.0039	-	7470A	PPB	13 Nov 2022 16:05:43	U	SMPL
CCV17 - 1	CCV17	20816	5.0833	-	7470A	PPB	13 Nov 2022 16:07:59	U	SMPL
CCB17 - 1	CCB17	-8	0.0027	-	7470A	PPB	13 Nov 2022 16:10:14	U	SMPL
N5561-02 - 1	WC-25	92	0.0271	-	7470A	PPB	13 Nov 2022 16:12:30	U	SMPL
N5561-04 - 1	WC-06	102	0.0295	-	7470A	PPB	13 Nov 2022 16:14:45	U	SMPL
N5561-06 - 1	WC-05	82	0.0246	-	7470A	PPB	13 Nov 2022 16:17:00	U	SMPL
N5561-06DUP - 1	WC-05DUP	57	0.0185	-	7470A	PPB	13 Nov 2022 16:19:16	U	SMPL
N5561-06MS - 1	WC-05MS	16709	4.0813	-	7470A	PPB	13 Nov 2022 16:21:31	U	SMPL
N5561-06MSD - 1	WC-05MSD	18836	4.6002	-	7470A	PPB	13 Nov 2022 16:23:48	U	SMPL
PB148995BL - 1	PBW	50	0.0168	-	7470A	PPB	13 Nov 2022 16:26:04	U	SMPL
PB148995BS - 1	LCSW	15996	3.9073	-	7470A	PPB	13 Nov 2022 16:28:21	U	SMPL
N5360-07 - 1	SPLP-LEACHATE-AMENDED-COMP-11	80	0.0242	-	7470A	PPB	13 Nov 2022 16:30:38	U	SMPL
N5360-07DUP - 1	SPLP-LEACHATE-AMENDED-COMP-11DUP	110	0.0315	-	7470A	PPB	13 Nov 2022 16:32:54	U	SMPL
CCV18 - 1	CCV18	20985	5.1246	-	7470A	PPB	13 Nov 2022 16:35:09	U	SMPL
CCB18 - 1	CCB18	-30	-0.0027	-	7470A	PPB	13 Nov 2022 16:37:25	U	SMPL
N5360-07MS - 1	SPLP-LEACHATE-AMENDED-COMP-11MS	15391	3.7597	-	7470A	PPB	13 Nov 2022 16:39:40	U	SMPL
N5360-07MSD - 1	SPLP-LEACHATE-AMENDED-COMP-11MSD	16153	3.9457	-	7470A	PPB	13 Nov 2022 16:41:56	U	SMPL
N5360-08 - 1	SPLP-LEACHATE-AMENDED-COMP-12	187	0.0503	-	7470A	PPB	13 Nov 2022 16:44:11	U	SMPL
N5360-09 - 1	SPLP-LEACHATE-AMENDED-COMP-13	101	0.0293	-	7470A	PPB	13 Nov 2022 16:46:26	U	SMPL
PB149015BL - 1	PBW	9	0.0068	-	7470A	PPB	13 Nov 2022 16:48:42	U	SMPL
PB149015BS - 1	LCSW	15045	3.6753	-	7470A	PPB	13 Nov 2022 16:50:58	U	SMPL
N5532-02 - 1	B-3(OW)	-61	-0.0102	-	7470A	PPB	13 Nov 2022 16:53:15	U	SMPL
N5532-04 - 1	DUP-06	84	0.0251	-	7470A	PPB	13 Nov 2022 16:55:31	U	SMPL
N5551-04 - 1	MW-12I	195	0.0522	-	7470A	PPB	13 Nov 2022 16:57:48	U	SMPL
N5551-04DUP - 1	MW-12IDUP	154	0.0422	-	7470A	PPB	13 Nov 2022 17:00:04	U	SMPL
CCV19 - 1	CCV19	20565	5.0221	-	7470A	PPB	13 Nov 2022 17:02:19	U	SMPL
CCB19 - 1	CCB19	-63	-0.0107	-	7470A	PPB	13 Nov 2022 17:04:35	U	SMPL
N5551-07 - 1	N5551-04MS	14782	3.6112	-	7470A	PPB	13 Nov 2022 17:06:50	U	SMPL
N5551-08 - 1	N5551-04MSD	14694	3.5897	-	7470A	PPB	13 Nov 2022 17:09:06	U	SMPL
N5551-14 - 1	MW-8I	676	0.1696	-	7470A	PPB	13 Nov 2022 17:11:22	U	SMPL
N5551-16 - 1	MW-21	460	0.1169	-	7470A	PPB	13 Nov 2022 17:13:38	U	SMPL
N5572-03 - 1	31914	148	0.0407	-	7470A	PPB	13 Nov 2022 17:15:53	U	SMPL
N5582-07 - 1	CLI-0659	221	0.0586	-	7470A	PPB	13 Nov 2022 17:18:10	U	SMPL
N5587-20 - 1	FB-02-20221110	39	0.0142	-	7470A	PPB	13 Nov 2022 17:20:26	U	SMPL
PB148976TB - 1	PB148976TB	-44	-0.0061	-	7470A	PPB	13 Nov 2022 17:22:43	U	SMPL
PB148995TB - 1	PB148995TB	-1	0.0044	-	7470A	PPB	13 Nov 2022 17:25:00	U	SMPL
CCV20 - 1	CCV20	20480	5.0014	-	7470A	PPB	13 Nov 2022 17:27:15	U	SMPL
CCB20 - 1	CCB20	-35	-0.0039	-	7470A	PPB	13 Nov 2022 17:29:30	U	SMPL
N5561-06LX5 - 1		10	0.0071	-	7470A	PPB	13 Nov 2022 17:31:46	U	SMPL
N5561-06A - 1		16918	4.1323	-	7470A	PPB	13 Nov 2022 17:34:02	U	SMPL
N5360-07LX5 - 1		-60	-0.0100	-	7470A	PPB	13 Nov 2022 17:36:18	U	SMPL
N5360-07A - 1		17004	4.1533	-	7470A	PPB	13 Nov 2022 17:38:34	U	SMPL
N5551-04LX5 - 1		-50	-0.0076	-	7470A	PPB	13 Nov 2022 17:40:50	U	SMPL
N5551-04A - 1		16953	4.1408	-	7470A	PPB	13 Nov 2022 17:43:07	U	SMPL
CCV21 - 1	CCV21	20435	4.9904	-	7470A	PPB	13 Nov 2022 17:45:23	U	SMPL
CCB21 - 1	CCB21	-35	-0.0039	-	7470A	PPB	13 Nov 2022 17:47:40	U	SMPL