

L B122808

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

11/15/2022 12:58

Reviewed by : <u>12</u>	Instrument ID : Konelab
-------------------------	-------------------------

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	93.416	0.0	0.069	
ICB1	1.254	0.0	0.001	
CCV1	244.143	0.0	0.180	
CCB1	1.093	0.0	0.001	
PB149068BL	1.138	0.0	0.001	
PB149068BS	95.913	0.0	0.071	
MIDPB149068	236.476	0.0	0.175	
N5609-01	1.552	0.0	0.002	
N5609-01DUP	1.476	0.0	0.001	
N5609-01MS	35.129	0.0	0.026	
N5609-01MSD	35.982	0.0	0.027	
CCV2	242.812	0.0	0.179	
CCB2	1.215	0.0	0.001	

95% / (90 - 110)
11/15/22

N	13
Mean	76.277
SD	99.7133
CV%	130.73

Aquakem v. 7.2AQ1

Results from time period:

Tue Nov 15 12:49:56 2022

Tue Nov 15 12:57:41 2022

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.95	µg/l	11/15/2022 11:14:22	
5.OPPBCN	A	Total CN	P	5.506	µg/l	11/15/2022 11:14:23	
10PPBCN	A	Total CN	P	10.3104	µg/l	11/15/2022 11:14:24	
50PPBCN	A	Total CN	P	47.8442	µg/l	11/15/2022 11:14:25	
100PPBCN	A	Total CN	P	98.444	µg/l	11/15/2022 11:14:26	
250PPBCN	A	Total CN	P	252.8597	µg/l	11/15/2022 11:14:27	
500PPBCN	A	Total CN	P	499.0857	µg/l	11/15/2022 11:14:28	
ICV1	S	Total CN	P	93.4159	µg/l	11/15/2022 12:49:57	
ICB1	S	Total CN	P	1.2541	µg/l	11/15/2022 12:49:58	
CCV1	S	Total CN	P	244.1427	µg/l	11/15/2022 12:50:01	
CCB1	S	Total CN	P	1.0928	µg/l	11/15/2022 12:50:03	
PB149068BL	S	Total CN	P	1.1381	µg/l	11/15/2022 12:50:05	
PB149068BS	S	Total CN	P	95.9125	µg/l	11/15/2022 12:50:06	
MIDPB149068	S	Total CN	P	236.4763	µg/l	11/15/2022 12:57:32	
N5609-01	S	Total CN	P	1.5522	µg/l	11/15/2022 12:57:34	
N5609-01DUP	S	Total CN	P	1.4764	µg/l	11/15/2022 12:57:35	
N5609-01MS	S	Total CN	P	35.1289	µg/l	11/15/2022 12:57:36	
N5609-01MSD	S	Total CN	P	35.9825	µg/l	11/15/2022 12:57:37	
CCV2	S	Total CN	P	242.8123	µg/l	11/15/2022 12:57:40	
CCB2	S	Total CN	P	1.2152	µg/l	11/15/2022 12:57:41	

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

11/15/2022 11:16


Test Total CN

Accepted 11/15/2022 11:16

Factor 1357
Bias 0

Coeff. of det. 0.999916

Errors

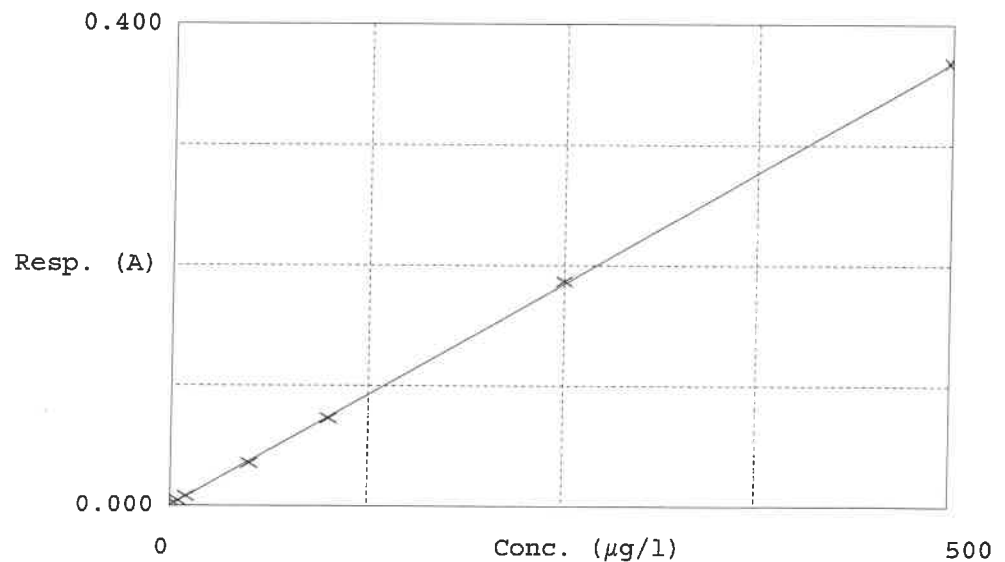

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.9500	0.0000	-
2	5.0PPBCN	0.004	5.5060	5.0000	10.1
3	10PPBCN	0.008	10.3104	10.0000	3.1
4	50PPBCN	0.036	47.8442	50.0000	-4.3
5	100PPBCN	0.073	98.4440	100.0000	-1.6
6	250PPBCN	0.187	252.8597	250.0000	1.1
7	500PPBCN	0.368	499.0857	500.0000	-0.2

12
11/15/22