

LB122901

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

11/15/2022 16:06

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.083	0.0	0.110	
ICB1	-0.005	0.0	0.008	
CCV1	1.094	0.0	0.111	
CCB1	-0.006	0.0	0.008	
PB149086BL	-0.006	0.0	0.008	
PB149086BS	1.093	0.0	0.111	
N5564-01	0.209	0.0	0.028	
N5564-01DUP	0.206	0.0	0.028	
N5564-01MS	1.355	0.0	0.135	
N5564-01MSD	1.363	0.0	0.136	
N5564-02	0.318	0.0	0.038	
CCV2	1.008	0.0	0.103	
CCB2	-0.001	0.0	0.008	
IDOC-01	1.012	0.0	0.103	
IDOC-02	1.002	0.0	0.102	
IDOC-03	1.007	0.0	0.102	
IDOC-04	1.007	0.0	0.103	
IDOC-05	1.009	0.0	0.103	
IDOC-06	1.006	0.0	0.102	
IDOC-07	1.006	0.0	0.102	
IDOC-08	1.000	0.0	0.102	
CCV3	1.007	0.0	0.103	
CCB3	-0.002	0.0	0.008	

N	23
Mean	0.729
SD	0.4933
CV%	67.67

Aquakem v. 7.2AQ1

Results from time period:

Tue Nov 15 14:35:58 2022

Tue Nov 15 16:00:13 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time
0.00PPM	A	Phenolics-	P	-0.0044	mg/l	11/15/2022 14:35:58
0.05PPM	A	Phenolics-	P	0.0568	mg/l	11/15/2022 14:35:59
0.1PPM	A	Phenolics-	P	0.1008	mg/l	11/15/2022 14:36:00
0.25PPM	A	Phenolics-	P	0.2495	mg/l	11/15/2022 14:36:01
0.50PPM	A	Phenolics-	P	0.5023	mg/l	11/15/2022 14:36:02
1.0PPM	A	Phenolics-	P	0.9914	mg/l	11/15/2022 14:36:03
2.0PPM	A	Phenolics-	P	2.0036	mg/l	11/15/2022 14:36:04
ICV1	S	Phenolics-	P	1.0834	mg/l	11/15/2022 15:12:37
ICB1	S	Phenolics-	P	-0.0047	mg/l	11/15/2022 15:12:39
CCV1	S	Phenolics-	P	1.0938	mg/l	11/15/2022 15:12:41
CCB1	S	Phenolics-	P	-0.0056	mg/l	11/15/2022 15:12:44
PB149086BL	S	Phenolics-	P	-0.0061	mg/l	11/15/2022 15:12:45
PB149086BS	S	Phenolics-	P	1.0928	mg/l	11/15/2022 15:12:48
N5564-01	S	Phenolics-	P	0.2088	mg/l	11/15/2022 15:22:39
N5564-01DUP	S	Phenolics-	P	0.2058	mg/l	11/15/2022 15:22:40
N5564-01MS	S	Phenolics-	P	1.3553	mg/l	11/15/2022 15:22:41
N5564-01MSD	S	Phenolics-	P	1.3632	mg/l	11/15/2022 15:22:42
N5564-02	S	Phenolics-	P	0.3179	mg/l	11/15/2022 15:22:43
CCV2	S	Phenolics-	P	1.0078	mg/l	11/15/2022 15:57:25
CCB2	S	Phenolics-	P	-0.0005	mg/l	11/15/2022 15:57:26
IDOC-01	S	Phenolics-	P	1.0118	mg/l	11/15/2022 15:57:27
IDOC-02	S	Phenolics-	P	1.0021	mg/l	11/15/2022 15:57:28
IDOC-03	S	Phenolics-	P	1.0067	mg/l	11/15/2022 15:57:29
IDOC-04	S	Phenolics-	P	1.0071	mg/l	11/15/2022 15:57:30
IDOC-05	S	Phenolics-	P	1.0093	mg/l	11/15/2022 15:57:31
IDOC-06	S	Phenolics-	P	1.0058	mg/l	11/15/2022 15:57:32
IDOC-07	S	Phenolics-	P	1.0062	mg/l	11/15/2022 15:57:33
IDOC-08	S	Phenolics-	P	1.0005	mg/l	11/15/2022 15:57:34
CCV3	S	Phenolics-	P	1.0072	mg/l	11/15/2022 15:57:35
CCB3	S	Phenolics-	P	-0.0018	mg/l	11/15/2022 15:57:36

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

11/15/2022 14:36

Test Phenolics-

Accepted

11/15/2022 14:36

Factor

10.71


Bias

0.008

Coeff. of det.

0.999949

Errors

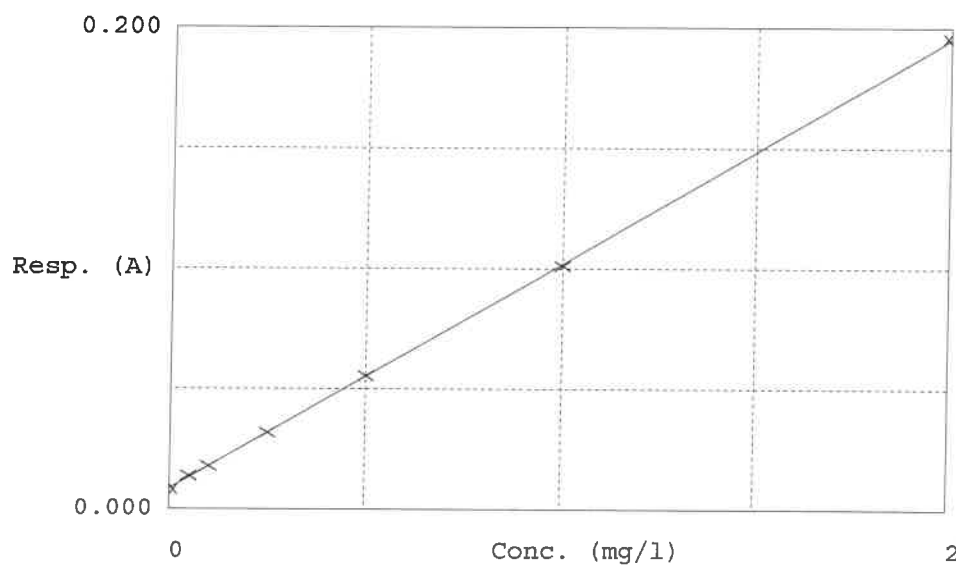

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.008	-0.0044	0.0000	-
2	Phenol-2	0.014	0.0568	0.0500	13.6
3	Phenol-2	0.018	0.1008	0.1000	0.8
4	Phenol-2	0.032	0.2495	0.2500	-0.2
5	Phenol-2	0.055	0.5023	0.5000	0.5
6	Phenol-2	0.101	0.9914	1.0000	-0.9
7	Phenol-2	0.196	2.0036	2.0000	0.2

12

11/15/22