


LB122905

7470A

INSTRUMENT ID: CV2

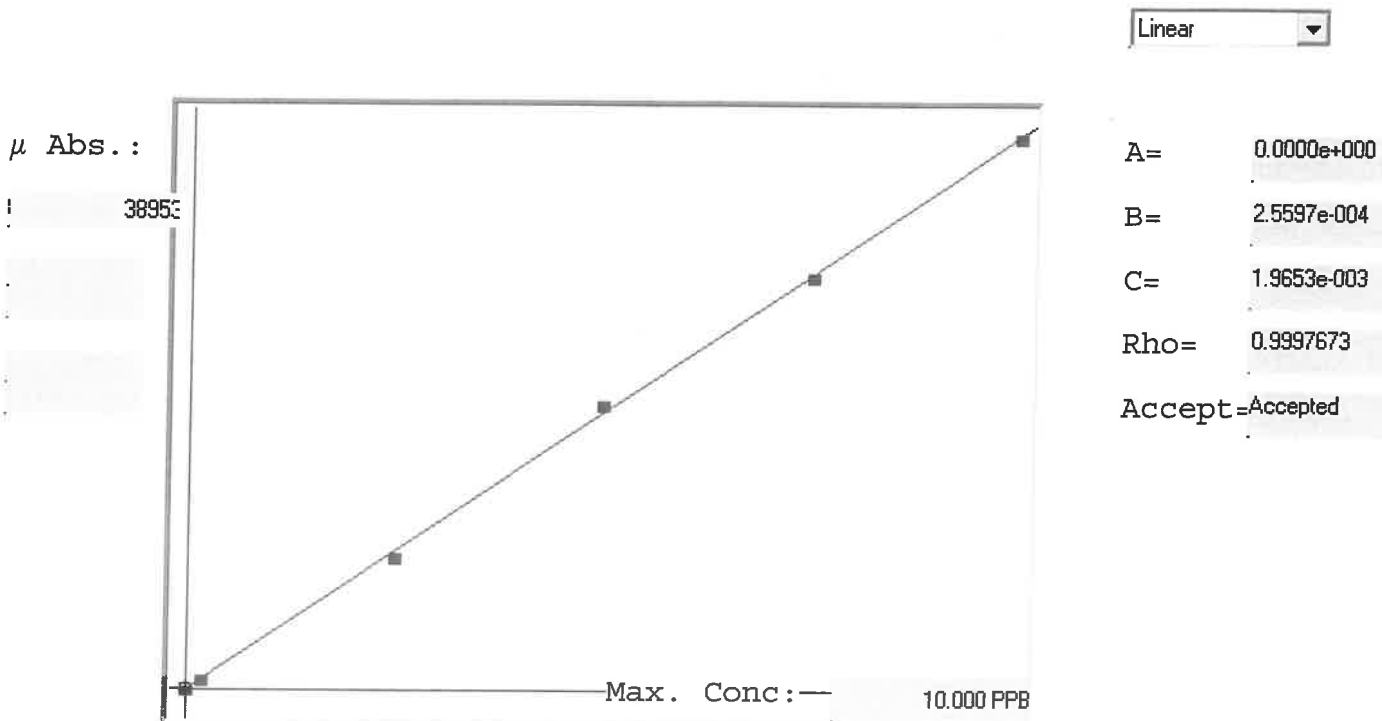

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	9/0/0
0.0	0.000	0.015	0.015	50	0.000	50					-
0.2	0.200	0.190	-0.010	736	0.0 %	736					-5
2.5	2.500	2.405	-0.095	9389	0.0 %	9389					-4
5.0	5.000	5.161	0.161	20156	0.0 %	20156					3
7.5	7.500	7.456	-0.044	29119	0.0 %	29119					-1
10.0	10.000	9.973	-0.027	38953	0.0 %	38953					0

LB122905 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 16 Nov 2022 08:18:21

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	50	-	0.0000	7470A	PPB	16 Nov 2022 08:32:13	S	Std
0.2 - 1	50.2	736	-	0.2000	7470A	PPB	16 Nov 2022 08:34:30	S	Std
2.5 - 1	52.5	9389	-	2.5000	7470A	PPB	16 Nov 2022 08:36:47	S	Std
5.0 - 1	55	20156	-	5.0000	7470A	PPB	16 Nov 2022 08:39:04	S	Std
7.5 - 1	57.5	29119	-	7.5000	7470A	PPB	16 Nov 2022 08:41:20	S	Std
10.0 - 1	510	38953	-	10.0000	7470A	PPB	16 Nov 2022 08:43:36	S	Std
ICV23 - 1	ICV23	14773	3.7834	-	7470A	PPB	16 Nov 2022 08:46:17	U	SMPL
ICB23 - 1	ICB23	122	0.0332	-	7470A	PPB	16 Nov 2022 08:48:31	U	SMPL
CCV36 - 1	CCV36	19839	5.0802	-	7470A	PPB	16 Nov 2022 08:50:46	U	SMPL
CCB36 - 1	CCB36	-38	-0.0078	-	7470A	PPB	16 Nov 2022 08:53:02	U	SMPL
CRA - 1	CRA	665	0.1722	-	7470A	PPB	16 Nov 2022 08:55:17	U	SMPL
HighStd - 1	HighStd	38305	9.8069	-	7470A	PPB	16 Nov 2022 08:57:32	U	SMPL
ChkStd - 1	ChkStd	25334	6.4867	-	7470A	PPB	16 Nov 2022 08:59:47	U	SMPL
PB149079BL - 1	PBW	-35	-0.0070	-	7470A	PPB	16 Nov 2022 09:02:03	U	SMPL
PB149079BS - 1	LCSW	16762	4.2925	-	7470A	PPB	16 Nov 2022 09:04:19	U	SMPL
N5550-01 - 1	D2781	-12	-0.0011	-	7470A	PPB	16 Nov 2022 09:06:35	U	SMPL
N5550-01DUP - 1	D2781DUP	1	0.0022	-	7470A	PPB	16 Nov 2022 09:08:51	U	SMPL
N5550-01MS - 1	D2781MS	14282	3.6577	-	7470A	PPB	16 Nov 2022 09:11:08	U	SMPL
N5550-01MSD - 1	D2781MSD	15926	4.0785	-	7470A	PPB	16 Nov 2022 09:13:25	U	SMPL
PB149080BL - 1	PBW	-75	-0.0172	-	7470A	PPB	16 Nov 2022 09:15:40	U	SMPL
CCV37 - 1	CCV37	18442	4.7226	-	7470A	PPB	16 Nov 2022 09:17:55	U	SMPL
CCB37 - 1	CCB37	-75	-0.0172	-	7470A	PPB	16 Nov 2022 09:20:11	U	SMPL
PB149080BS - 1	LCSW	17430	4.4635	-	7470A	PPB	16 Nov 2022 09:22:26	U	SMPL
N5598-02 - 1	FRAC-TANK-0760533	-44	-0.0093	-	7470A	PPB	16 Nov 2022 09:24:41	U	SMPL
N5598-13 - 1	FRAC-TANK-SLURRY-0760533	10	0.0045	-	7470A	PPB	16 Nov 2022 09:26:57	U	SMPL
N5607-02 - 1	WC-01	23	0.0079	-	7470A	PPB	16 Nov 2022 09:29:13	U	SMPL
N5607-04 - 1	WC-36	0	0.0020	-	7470A	PPB	16 Nov 2022 09:31:29	U	SMPL
N5607-06 - 1	WC-37	0	0.0020	-	7470A	PPB	16 Nov 2022 09:33:44	U	SMPL
N5607-08 - 1	WC-38	-1	0.0017	-	7470A	PPB	16 Nov 2022 09:36:01	U	SMPL
N5607-10 - 1	WC-39	31	0.0099	-	7470A	PPB	16 Nov 2022 09:38:18	U	SMPL
N5607-12 - 1	WC-40	-3	0.0012	-	7470A	PPB	16 Nov 2022 09:40:38	U	SMPL
N5613-02 - 1	WC-COMP-1	50	0.0148	-	7470A	PPB	16 Nov 2022 09:42:55	U	SMPL
CCV38 - 1	CCV38	18705	4.7899	-	7470A	PPB	16 Nov 2022 09:45:11	U	SMPL
CCB38 - 1	CCB38	-67	-0.0152	-	7470A	PPB	16 Nov 2022 09:47:26	U	SMPL
N5617-03 - 1	D2784	46	0.0137	-	7470A	PPB	16 Nov 2022 09:49:42	U	SMPL
N5617-03DUP - 1	D2784DUP	64	0.0183	-	7470A	PPB	16 Nov 2022 09:51:57	U	SMPL
N5617-03MS - 1	D2784MS	16250	4.1615	-	7470A	PPB	16 Nov 2022 09:54:13	U	SMPL
N5617-03MSD - 1	D2784MSD	16049	4.1100	-	7470A	PPB	16 Nov 2022 09:56:29	U	SMPL
PB149081BL - 1	PBW	-7	0.0002	-	7470A	PPB	16 Nov 2022 09:58:44	U	SMPL
PB149081BS - 1	LCSW	14967	3.8331	-	7470A	PPB	16 Nov 2022 10:01:01	U	SMPL
N5605-01 - 1	C10HPT-1	47	0.0140	-	7470A	PPB	16 Nov 2022 10:03:17	U	SMPL
N5605-02 - 1	C10HPT-2	165	0.0442	-	7470A	PPB	16 Nov 2022 10:05:34	U	SMPL
N5605-03 - 1	C10HPT-3	128	0.0347	-	7470A	PPB	16 Nov 2022 10:07:51	U	SMPL
N5605-03DUP - 1	C10HPT-3DUP	143	0.0386	-	7470A	PPB	16 Nov 2022 10:10:06	U	SMPL
CCV39 - 1	CCV39	17864	4.5746	-	7470A	PPB	16 Nov 2022 10:12:22	U	SMPL
CCB39 - 1	CCB39	-10	-0.0006	-	7470A	PPB	16 Nov 2022 10:14:37	U	SMPL
N5605-03MS - 1	C10HPT-3MS	15581	3.9902	-	7470A	PPB	16 Nov 2022 10:16:53	U	SMPL
N5605-03MSD - 1	C10HPT-3MSD	14828	3.7975	-	7470A	PPB	16 Nov 2022 10:19:08	U	SMPL
PB149038TB - 1	PB149038TB	59	0.0171	-	7470A	PPB	16 Nov 2022 10:21:24	U	SMPL
PB149052TB - 1	PB149052TB	144	0.0358	-	7470A	PPB	16 Nov 2022 10:23:39	U	SMPL
N5550-01LX5 - 1		29	0.0094	-	7470A	PPB	16 Nov 2022 10:25:55	U	SMPL
N5550-01A - 1		15976	4.0913	-	7470A	PPB	16 Nov 2022 10:28:11	U	SMPL
N5617-03LX5 - 1		-68	-0.0154	-	7470A	PPB	16 Nov 2022 10:30:27	U	SMPL
N5617-03A - 1		15027	3.8484	-	7470A	PPB	16 Nov 2022 10:32:44	U	SMPL
N5605-03LX5 - 1		8	0.0040	-	7470A	PPB	16 Nov 2022 10:35:01	U	SMPL
N5605-03A - 1		15624	4.0012	-	7470A	PPB	16 Nov 2022 10:37:17	U	SMPL
CCV40 - 1	CCV40	18375	4.7054	-	7470A	PPB	16 Nov 2022 10:39:33	U	SMPL
CCB40 - 1	CCB40	-6	0.0004	-	7470A	PPB	16 Nov 2022 10:41:48	U	SMPL