

LB 123035

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

11/25/2022 16:36

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.718	0.0	0.067	
ICB1	1.961	0.0	0.001	
CCV1	251.427	0.0	0.176	
CCB1	1.835	0.0	0.001	
PB149297BL	1.806	0.0	0.001	
PB149297BS	96.987	0.0	0.068	
LOWPB149297	10.257	0.0	0.007	
HIGHPB149297	509.096	0.0	0.357	
N5752-25	1.890	0.0	0.001	
N5752-25DUP	1.637	0.0	0.001	
PB149296BL	1.588	0.0	0.001	
PB149296BS	93.174	0.0	0.065	
CCV2	242.542	0.0	0.170	
CCB2	1.657	0.0	0.001	
N5753-01	5.399	0.0	0.004	
N5753-01DUP	5.173	0.0	0.004	
N5753-01MS	38.369	0.0	0.027	
N5753-01MSD	38.588	0.0	0.027	
N5766-01	2.441	0.0	0.002	
N5766-02	1.760	0.0	0.001	
N5766-03	3.867	0.0	0.003	
N5766-04	2.348	0.0	0.002	
N5766-05	3.045	0.0	0.002	
N5772-01	1.783	0.0	0.001	
CCV3	249.406	0.0	0.175	
CCB3	2.038	0.0	0.001	
N5722-02	1.388	0.0	0.001	
N5772-03	2.256	0.0	0.002	
N5772-04	2.593	0.0	0.002	
N5752-25MS	33.800	0.0	0.024	
N5752-25MSD	33.891	0.0	0.024	
CCV4	256.727	0.0	0.180	
CCB4	1.670	0.0	0.001	

102.9% (PO-110)
102.9% (PO-710)

12
11/25/22

N 33
Mean 60.549
SD 114.7138
CV% 189.46

Aquakem v. 7.2AQ1

Results from time period:

Fri Nov 25 15:53:53 2022

Fri Nov 25 16:35:07 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	1.7489	µg/l	11/25/2022 14:44:59	
5.0PPBCN	A	Total CN	P	5.6172	µg/l	11/25/2022 14:45:00	
10PPBCN	A	Total CN	P	9.6845	µg/l	11/25/2022 14:45:01	
50PPBCN	A	Total CN	P	47.4478	µg/l	11/25/2022 14:45:02	
100PPBCN	A	Total CN	P	97.55	µg/l	11/25/2022 14:45:03	
250PPBCN	A	Total CN	P	254.4126	µg/l	11/25/2022 14:45:04	
500PPBCN	A	Total CN	P	498.5391	µg/l	11/25/2022 14:45:05	
ICV1	S	Total CN	P	95.7179	µg/l	11/25/2022 15:53:54	
ICB1	S	Total CN	P	1.961	µg/l	11/25/2022 15:53:55	
CCV1	S	Total CN	P	251.4268	µg/l	11/25/2022 15:53:58	
CCB1	S	Total CN	P	1.835	µg/l	11/25/2022 15:53:59	
PB149297BL	S	Total CN	P	1.806	µg/l	11/25/2022 15:54:01	
PB149297BS	S	Total CN	P	96.9871	µg/l	11/25/2022 15:54:03	
LOWPB149297	S	Total CN	P	10.2572	µg/l	11/25/2022 16:01:30	
HIGHPB149297	S	Total CN	P	509.0957	µg/l	11/25/2022 16:01:31	
N5752-25	S	Total CN	P	1.89	µg/l	11/25/2022 16:01:32	
N5752-25DUP	S	Total CN	P	1.637	µg/l	11/25/2022 16:01:33	
PB149296BL	S	Total CN	P	1.5875	µg/l	11/25/2022 16:01:38	
PB149296BS	S	Total CN	P	93.1738	µg/l	11/25/2022 16:09:00	
CCV2	S	Total CN	P	242.5423	µg/l	11/25/2022 16:09:01	
CCB2	S	Total CN	P	1.6573	µg/l	11/25/2022 16:09:02	
N5753-01	S	Total CN	P	5.3994	µg/l	11/25/2022 16:09:03	
N5753-01DUP	S	Total CN	P	5.1733	µg/l	11/25/2022 16:09:04	
N5753-01MS	S	Total CN	P	38.3691	µg/l	11/25/2022 16:09:05	
N5753-01MSD	S	Total CN	P	38.5882	µg/l	11/25/2022 16:09:06	
N5766-01	S	Total CN	P	2.4411	µg/l	11/25/2022 16:09:09	
N5766-02	S	Total CN	P	1.7601	µg/l	11/25/2022 16:09:10	
N5766-03	S	Total CN	P	3.8672	µg/l	11/25/2022 16:16:35	
N5766-04	S	Total CN	P	2.3479	µg/l	11/25/2022 16:16:36	
N5766-05	S	Total CN	P	3.0451	µg/l	11/25/2022 16:16:37	
N5772-01	S	Total CN	P	1.7828	µg/l	11/25/2022 16:16:38	
CCV3	S	Total CN	P	249.4064	µg/l	11/25/2022 16:16:39	
CCB3	S	Total CN	P	2.0379	µg/l	11/25/2022 16:16:40	
N5722-02	S	Total CN	P	1.3876	µg/l	11/25/2022 16:16:41	
N5772-03	S	Total CN	P	2.2556	µg/l	11/25/2022 16:16:42	
N5772-04	S	Total CN	P	2.593	µg/l	11/25/2022 16:16:43	
N5752-25MS	S	Total CN	P	33.8001	µg/l	11/25/2022 16:35:01	
N5752-25MSD	S	Total CN	P	33.8912	µg/l	11/25/2022 16:35:04	
CCV4	S	Total CN	P	256.7265	µg/l	11/25/2022 16:35:05	
CCB4	S	Total CN	P	1.67	µg/l	11/25/2022 16:35:07	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

11/25/2022 14:45

Reviewed by : 12

Instrument ID : Konelab


Test Total CN

Accepted 11/25/2022 14:45

Factor 1426
Bias 0

Coeff. of det. 0.999817

Errors

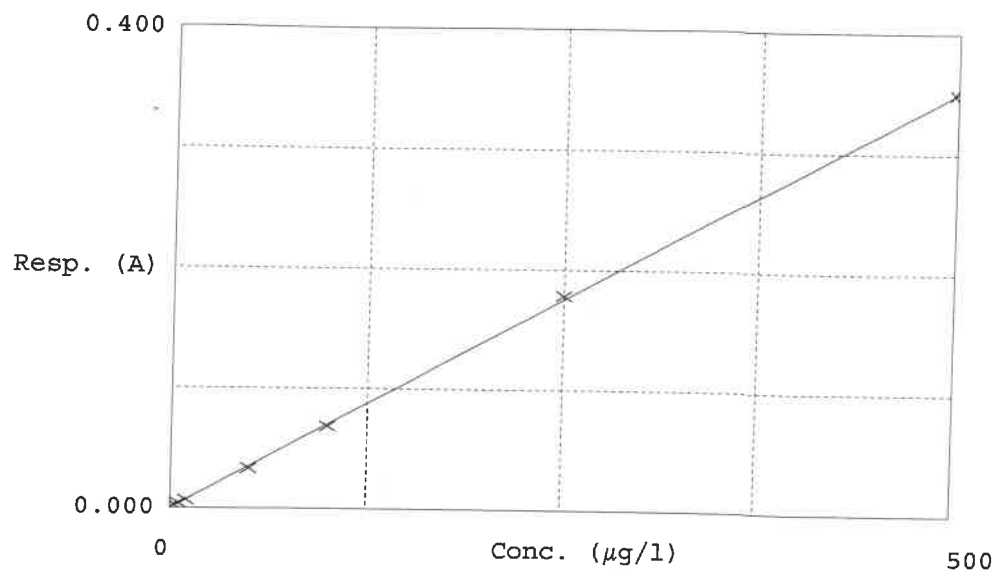

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	1.7489	0.0000	
2	5.0PPBCN	0.004	5.6172	5.0000	12.3
3	10PPBCN	0.007	9.6845	10.0000	-3.2
4	50PPBCN	0.033	47.4478	50.0000	-5.1
5	100PPBCN	0.068	97.5500	100.0000	-2.5
6	250PPBCN	0.178	254.4126	250.0000	1.8
7	500PPBCN	0.350	498.5391	500.0000	-0.9

12
11/25/22