

L B123041

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

11/28/2022 13:13

Test: CNEPA-NEW

Sample Id	Result	Dil. 1 +	Response	Errors
ICV001 ICV001	92.361	0.0	0.090	
ICB001 ICB001	1.567	0.0	0.008	
CCV001 CCV001	245.263	0.0	0.227	
CCB001 CCB001	1.325	0.0	0.008	
PB149311BL PBW311	2.038	0.0	0.008	
N5717-01 MA0B23	1.892	0.0	0.008	
N5717-02 MA0B23D	1.802	0.0	0.008	
N5717-03 MA0B23S	92.839	0.0	0.090	
N5717-04 MA0B24	2.244	0.0	0.009	
CCV002 CCV002	242.746	0.0	0.225	
CCB002 CCB002	1.703	0.0	0.008	

N	11
Mean	62.344
SD	96.6945
CV%	155.10

Aquakem v. 7.2AQ1

Results from time period:

Mon Nov 28 11:57:20 2022

Mon Nov 28 12:51:46 2022

Sample Id	Sam/Ctr	Test short	Test ty	Result	Result unit	Result date and time	Stat
S0.0	A	CNEPA-NE\ P		1.5538	µg/l	11/28/2022 12:15:25	
S5.0	A	CNEPA-NE\ P		5.2041	µg/l	11/28/2022 12:15:26	
S10.0	A	CNEPA-NE\ P		9.0796	µg/l	11/28/2022 12:15:27	
S100.0	A	CNEPA-NE\ P		96.4279	µg/l	11/28/2022 12:15:28	
S250.0	A	CNEPA-NE\ P		254.0075	µg/l	11/28/2022 12:15:29	
S500.0	A	CNEPA-NE\ P		498.727	µg/l	11/28/2022 12:15:30	
ICV001 ICV001	S	CNEPA-NE\ P		92.3613	µg/l	11/28/2022 12:39:52	
ICB001 ICB001	S	CNEPA-NE\ P		1.5666	µg/l	11/28/2022 12:39:54	
CCV001 CCV001	S	CNEPA-NE\ P		245.2628	µg/l	11/28/2022 12:39:55	
CCB001 CCB001	S	CNEPA-NE\ P		1.3253	µg/l	11/28/2022 12:39:58	
PB149311BL PBW311	S	CNEPA-NE\ P		2.0378	µg/l	11/28/2022 12:39:59	
N5717-01 MA0B23	S	CNEPA-NE\ P		1.8924	µg/l	11/28/2022 12:47:24	
N5717-02 MA0B23D	S	CNEPA-NE\ P		1.802	µg/l	11/28/2022 12:47:25	
N5717-03 MA0B23S	S	CNEPA-NE\ P		92.8386	µg/l	11/28/2022 12:47:30	
N5717-04 MA0B24	S	CNEPA-NE\ P		2.2437	µg/l	11/28/2022 12:47:31	
CCV002 CCV002	S	CNEPA-NE\ P		242.7462	µg/l	11/28/2022 12:47:33	
CCB002 CCB002	S	CNEPA-NE\ P		1.7025	µg/l	11/28/2022 12:51:43	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

11/28/2022 12:15

Test CNEPA-NEW

Accepted

11/28/2022 12:15

~~Factor~~ Slope

~~1111~~ 0.000900

Bias Y. Intercept


0.007

12 11/29/22

Coeff. of det.

0.999830

Errors

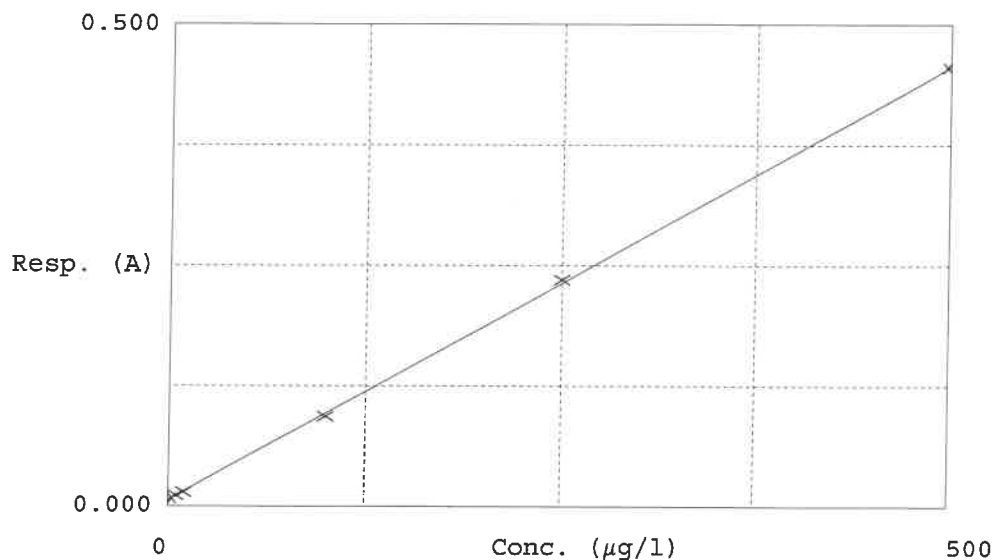

	Calibrator	Response	Calc. con.	Conc.	Re Errors
1	0.0PPBCN 50.0	0.008	1.5538	0.0000	—
2	5.0PPBCN 55.0	0.011	5.2041	5.0000	4.1
3	10PPBCN 510.0	0.015	9.0796	10.0000	-9.2
4	100PPBCN 5100.0	0.093	96.4279	100.0000	-3.6
5	250PPBCN 5250.0	0.235	254.0075	250.0000	1.6
6	500PPBCN 5500.0	0.455	498.7270	500.0000	-0.3

11/28/22