

Clear table

| Instrument ID: IC-2 |                      |                       |                       |                       | Analyst :             | IZ                     | Method: 300.0 / 9056A |              |                |                          |         |
|---------------------|----------------------|-----------------------|-----------------------|-----------------------|-----------------------|------------------------|-----------------------|--------------|----------------|--------------------------|---------|
| ident               | concentra<br>tion F- | concentratio<br>n CL- | concentrati<br>on NO2 | concentrati<br>on BR- | concentrati<br>on NO3 | concentrati<br>on HPO4 | concentrati<br>on SO4 | file name    | date time      | Initial wt/<br>Final Vol | Analyst |
| STD1                | 0.0000               | 0.0000                | 0.0000                | 0.0000                | 0.0000                | 0.0000                 | 0.0000                | _2022-11-17_ | 11/17/22 11:09 |                          | IZ/MA   |
| STD2                | 0.4740               | 0.6670                | 0.6970                | 2.2420                | 0.5680                | 1.1120                 | 3.3950                | _2022-11-17_ | 11/17/22 11:40 |                          | IZ/MA   |
| STD3                | 0.7820               | 1.2000                | 1.2010                | 4.0470                | 1.0040                | 1.9330                 | 6.0320                | _2022-11-17_ | 11/17/22 12:10 |                          | IZ/MA   |
| STD4                | 0.9960               | 1.4670                | 1.4680                | 4.8950                | 1.2220                | 2.4470                 | 7.2720                | _2022-11-17_ | 11/17/22 12:41 |                          | IZ/MA   |
| STD5                | 1.8820               | 2.9690                | 2.9160                | 9.7890                | 2.4520                | 5.0120                 | 14.7020               | _2022-11-17_ | 11/17/22 12:41 |                          | IZ/MA   |
| STD6                | 3.9100               | 5.9260                | 5.9450                | 19.7890               | 4.9360                | 9.9460                 | 29.9000               | _2022-11-17_ | 11/17/22 13:11 |                          | IZ/MA   |
| STD7                | 5.1030               | 7.5700                | 7.5720                | 25.2390               | 6.3170                | 12.5480                | 37.6980               | _2022-11-17_ | 11/17/22 13:42 |                          | IZ/MA   |
| ICV                 | 1.9060               | 3.0640                | 3.0810                | 10.2210               | 2.5420                | 4.8410                 | 15.6160               | _2022-11-17_ | 11/17/22 14:13 |                          | IZ/MA   |
| ICB                 | 0.0000               | 0.0000                | 0.0000                | 0.0000                | 0.0000                | 0.0000                 | 0.0000                | _2022-11-17_ | 11/17/22 15:33 |                          | IZ/MA   |
| CCV                 | 2.0250               | 2.8180                | 2.8140                | 9.2320                | 2.3130                | 5.0230                 | 13.9950               | _2022-12-06_ | 11/17/22 16:06 |                          | IZ/MA   |
| CCB                 | 0.0000               | 0.0000                | 0.0000                | 0.0000                | 0.0000                | 0.0000                 | 0.0000                | _2022-12-06_ | 12/6/22 10:30  |                          | IZ/MA   |
| LB123150BLW         | 1.8640               | 2.9020                | 2.7790                | 9.4330                | 2.3840                | 4.7830                 | 14.5670               | _2022-12-06_ | 12/6/22 11:04  |                          | IZ/MA   |
| LB123150BSW         | 0.0000               | 221.0510              | 0.0000                | 0.0000                | 1.8300                | 0.4920                 | 33.7770               | _2022-12-06_ | 12/6/22 11:36  |                          | IZ/MA   |
| N5841-01            | 0.0000               | 306.0130              | 0.0000                | 0.0000                | 3.2820                | 0.0000                 | 36.2350               | _2022-12-06_ | 12/6/22 12:07  |                          | IZ/MA   |
| N5841-03            | 0.5620               | 289.0130              | 0.0000                | 0.0000                | 0.0000                | 0.0000                 | 47.5050               | _2022-12-06_ | 12/6/22 13:21  |                          | IZ/MA   |
| N5841-05            | 0.0000               | 148.3760              | 0.2560                | 0.0000                | 1.1090                | 0.0000                 | 31.1390               | _2022-12-06_ | 12/6/22 13:53  |                          | IZ/MA   |
| N5841-07            | 0.3160               | 20.7650               | 0.0000                | 0.0000                | 0.0000                | 0.0000                 | 10.5260               | _2022-12-06_ | 12/6/22 14:25  |                          | IZ/MA   |
| N5841-09            | 0.0000               | 204.5350              | 0.0000                | 0.0000                | 0.6720                | 0.0000                 | 18.9000               | _2022-12-06_ | 12/6/22 15:18  |                          | IZ/MA   |
| N5841-11            | 0.0000               | 196.7730              | 0.0000                | 0.0000                | 2.5920                | 0.0000                 | 42.9570               | _2022-12-06_ | 12/6/22 15:50  |                          | IZ/MA   |
| N5841-13            | 0.0000               | 16.6820               | 0.0000                | 0.0000                | 0.9710                | 0.0000                 | 19.8880               | _2022-12-06_ | 12/6/22 16:22  |                          | IZ/MA   |
| N5841-15            | 0.2890               | 2.8650                | 2.9220                | 9.4720                | 2.3710                | 5.6380                 | 14.1000               | _2022-12-06_ | 12/6/22 16:53  |                          | IZ/MA   |
| CCV                 | 1.9160               | 0.0000                | 0.0000                | 0.0000                | 0.0000                | 0.0000                 | 0.0000                | _2022-12-06_ | 12/6/22 17:25  |                          | IZ/MA   |
| CCB                 | 0.0000               | 200.1470              | 0.0000                | 0.0000                | 0.7900                | 0.0000                 | 24.2640               | _2022-12-06_ | 12/6/22 17:57  |                          | IZ/MA   |
| N5841-17            | 0.6000               | 200.0860              | 0.0000                | 0.0000                | 0.8100                | 0.0000                 | 23.7810               | _2022-12-06_ | 12/6/22 18:28  |                          | IZ/MA   |
| N5841-19            | 0.3790               | 0.2480                | 0.0000                | 0.0000                | 0.1640                | 0.0000                 | 0.0000                | _2022-12-06_ | 12/6/22 19:00  |                          | IZ/MA   |
| N5861-01            | 0.0000               | 2.9780                | 2.9780                | 9.6260                | 2.4720                | 5.5800                 | 14.4410               | _2022-12-06_ | 12/6/22 20:03  |                          | IZ/MA   |
| N5861-01MS          | 1.9600               | 3.0760                | 3.0370                | 9.8790                | 2.5580                | 5.7750                 | 14.8600               | _2022-12-06_ | 12/6/22 20:35  |                          | IZ/MA   |
| N5861-01MSD         | 2.0500               | 0.7460                | 0.0000                | 0.0000                | 0.5170                | 0.0000                 | 1.5560                | _2022-12-06_ | 12/6/22 21:07  |                          | IZ/MA   |
| N5869-01            | 0.0000               | 0.2230                | 0.0000                | 0.0000                | 0.2170                | 0.0000                 | 0.8400                | _2022-12-06_ | 12/6/22 21:38  |                          | IZ/MA   |
| N5853-01            | 0.0000               | 686.1970              | 0.0000                | 0.0000                | 0.2920                | 0.0000                 | 29.6530               | _2022-12-06_ | 12/6/22 22:10  |                          | IZ/MA   |
| N5865-03            | 0.3300               | 491.5740              | 0.0000                | 0.0000                | 0.0000                | 0.0000                 | 21.7870               | _2022-12-06_ | 12/6/22 22:42  |                          | IZ/MA   |
| N5865-05            | 0.3780               | 115.1970              | 0.0000                | 0.0000                | 0.0000                | 0.0000                 | 17.9090               | _2022-12-06_ | 12/6/22 23:13  |                          | IZ/MA   |
| N5865-07            | 0.4520               | 2.9210                | 2.9710                | 9.5540                | 0.3130                | 0.0000                 | 14.0950               | _2022-12-06_ | 12/6/22 23:45  |                          | IZ/MA   |
| CCV                 | 1.9750               |                       |                       |                       | 2.4000                | 6.2260                 |                       | _2022-12-07_ | 12/7/22 0:17   |                          | IZ/MA   |




Clear table

| Instrument ID: IC-2   |                      |                       |                        |                        |                        |                         |                        |             |                |                          |         |
|-----------------------|----------------------|-----------------------|------------------------|------------------------|------------------------|-------------------------|------------------------|-------------|----------------|--------------------------|---------|
| Analyst : IZ          |                      |                       |                        |                        |                        |                         |                        |             |                |                          |         |
| Method: 300.0 / 9056A |                      |                       |                        |                        |                        |                         |                        |             |                |                          |         |
| ident                 | concentra<br>tion F- | concentratio<br>n CL- | concentratio<br>on NO2 | concentratio<br>on BR- | concentratio<br>on NO3 | concentratio<br>on HPO4 | concentratio<br>on SO4 | file name   | date time      | Initial wt/<br>Final Vol | Analyst |
| STD1                  | 0.0000               | 0.0000                | 0.0000                 | 0.0000                 | 0.0000                 | 0.0000                  | 0.0000                 | 2022-11-17_ | 11/17/22 11:09 |                          | IZ/MA   |
| STD2                  | 0.4740               | 0.6670                | 0.6970                 | 2.2420                 | 0.5680                 | 1.1120                  | 3.3950                 | 2022-11-17_ | 11/17/22 11:40 |                          | IZ/MA   |
| STD3                  | 0.7820               | 1.2000                | 1.2010                 | 4.0470                 | 1.0040                 | 1.9330                  | 6.0320                 | 2022-11-17_ | 11/17/22 12:10 |                          | IZ/MA   |
| STD4                  | 0.9960               | 1.4670                | 1.4680                 | 4.8950                 | 1.2220                 | 2.4470                  | 7.2720                 | 2022-11-17_ | 11/17/22 12:41 |                          | IZ/MA   |
| STD5                  | 1.8820               | 2.9690                | 2.9160                 | 9.7890                 | 2.4520                 | 5.0120                  | 14.7020                | 2022-11-17_ | 11/17/22 13:11 |                          | IZ/MA   |
| STD6                  | 3.9100               | 5.9260                | 5.9450                 | 19.7890                | 4.9360                 | 9.9460                  | 29.9000                | 2022-11-17_ | 11/17/22 13:42 |                          | IZ/MA   |
| STD7                  | 5.1030               | 7.5700                | 7.5720                 | 25.2390                | 6.3170                 | 12.5480                 | 37.6980                | 2022-11-17_ | 11/17/22 14:13 |                          | IZ/MA   |
| ident                 | True<br>Value F-     | True Value<br>CL-     | True Value<br>NO2      | True Value<br>BR-      | True Value<br>NO3      | True Value<br>HPO4      | True Value<br>SO4      |             |                |                          |         |
| STD1                  | 0.0000               | 0.0000                | 0.0000                 | 0.0000                 | 0.0000                 | 0.0000                  | 0.0000                 |             |                |                          |         |
| STD2                  | 0.4000               | 0.6000                | 0.6000                 | 2.0000                 | 0.5000                 | 1.0000                  | 3.0000                 |             |                |                          |         |
| STD3                  | 0.8000               | 1.2000                | 1.2000                 | 4.0000                 | 1.0000                 | 2.0000                  | 6.0000                 |             |                |                          |         |
| STD4                  | 1.0000               | 1.5000                | 1.5000                 | 5.0000                 | 1.2500                 | 2.5000                  | 7.5000                 |             |                |                          |         |
| STD5                  | 2.0000               | 3.0000                | 3.0000                 | 10.0000                | 2.5000                 | 5.0000                  | 15.0000                |             |                |                          |         |
| STD6                  | 4.0000               | 6.0000                | 6.0000                 | 20.0000                | 5.0000                 | 10.0000                 | 30.0000                |             |                |                          |         |
| STD7                  | 5.0000               | 7.5000                | 7.5000                 | 25.0000                | 6.2500                 | 12.5000                 | 37.0000                |             |                |                          |         |
| ident                 | Relative<br>Error F- | Relative<br>Error CL- | Relative<br>Error NO2  | Relative<br>Error BR-  | Relative<br>Error NO3  | Relative<br>Error HPO4  | Relative<br>Error SO4  |             |                |                          |         |
| STD1                  |                      | 11.1667               | 16.1667                | 12.1000                | 13.6000                | 11.2000                 | 13.1667                |             |                |                          |         |
| STD2                  | 18.5000              | 0.0000                | 0.0833                 | 1.1750                 | 0.4000                 | -3.3500                 | 0.5333                 |             |                |                          |         |
| STD3                  | -2.2500              | -2.2000               | -2.1333                | -2.1000                | -2.2400                | -2.1200                 | -3.0400                |             |                |                          |         |
| STD4                  | -0.4000              | -1.0333               | -2.8000                | -2.1100                | -1.9200                | 0.2400                  | -1.9867                |             |                |                          |         |
| STD5                  | -5.9000              | -1.2333               | -0.9167                | -1.0550                | -1.2800                | -0.5400                 | -0.3333                |             |                |                          |         |
| STD6                  | -2.2500              | 0.9333                | 0.9600                 | 0.9560                 | 1.0720                 | 0.3840                  | 1.8865                 |             |                |                          |         |
| STD7                  | 2.0600               |                       |                        |                        |                        |                         |                        |             |                |                          |         |

# CALIBRATION OF COMPONENT F-

Method: AnionsIC2-111722.mtw  
 Equation:  $Q = 0.0713424 \cdot A + 3.87962$   
 RSD: 5.032 %  
 Correlation coefficient: 0.998619

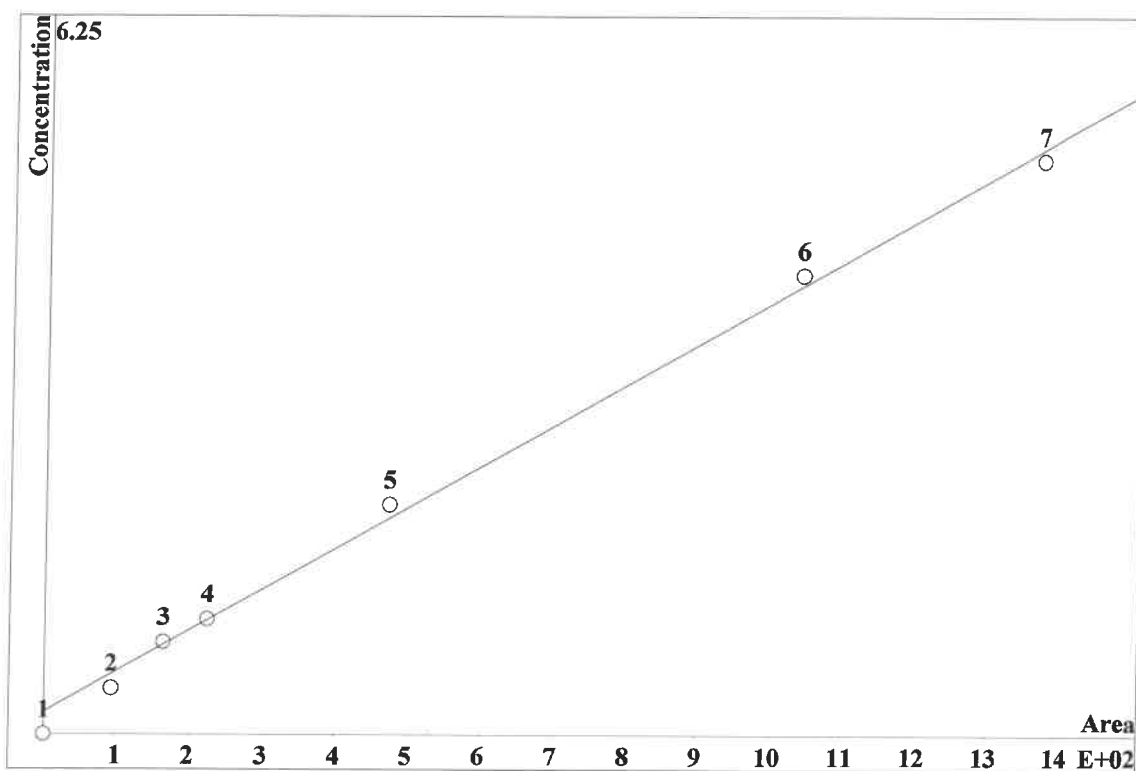


K3 = 0      K2 = 0      K1 = 0.0713424      K0 = 3.87962  
 Base: Area  
 Ref.channel: ch1  
 ISTD:  
 Formula: Linear  
 Weight: 1

| Level | Height | Area  | Conc. | Vol/Dil | Retention | Used | File |
|-------|--------|-------|-------|---------|-----------|------|------|
| 1     | 0      | 0     | 0     | 0       | 0         |      | 0    |
| 2     | 1.905  | 93.38 | 0.4   | 20      | 5.877     |      |      |
| 3     | 4.035  | 164.9 | 0.8   | 20      | 5.877     |      |      |
| 4     | 5.668  | 224.7 | 1     | 20      | 5.877     |      |      |
| 5     | 12.14  | 473.2 | 2     | 20      | 5.877     |      |      |
| 6     | 27.79  | 1042  | 4     | 20      | 5.877     |      |      |
| 7     | 37.65  | 1376  | 5     | 20      | 5.877     |      |      |

## CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-111722.mtw  
 Equation:  $Q = 0.123976 \cdot A + 2.60209$   
 RSD: 1.971 %  
 Correlation coefficient: 0.999788

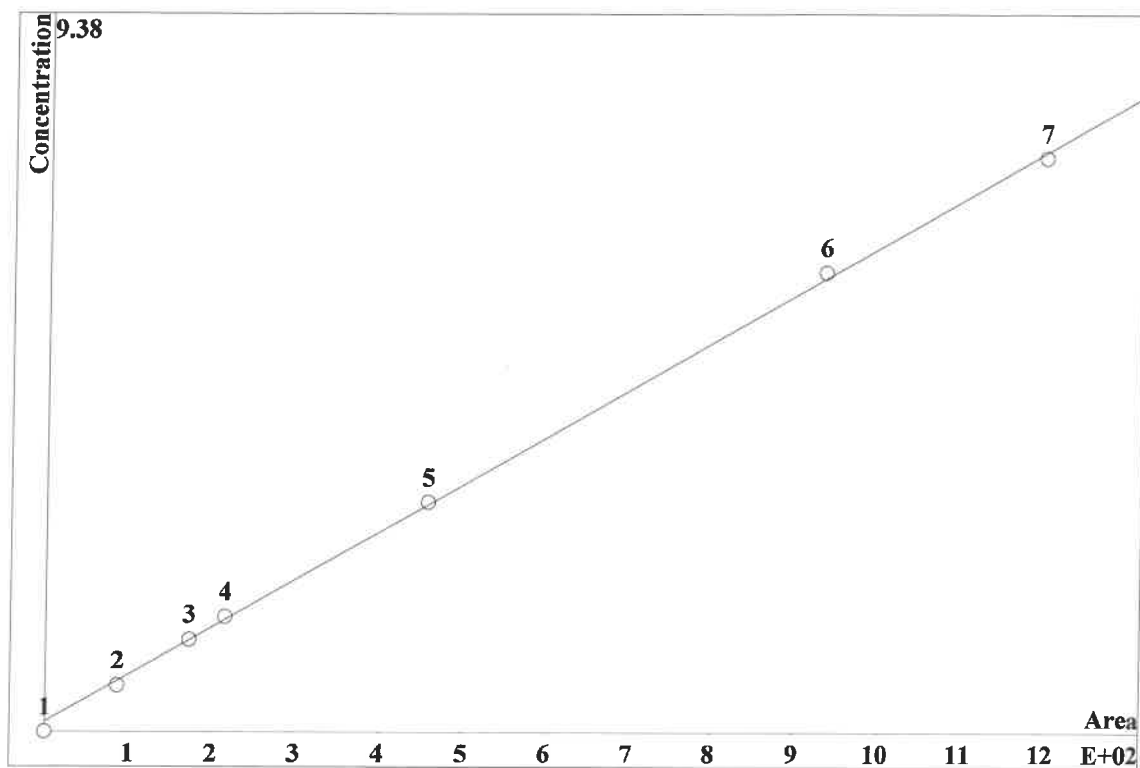


K3 = 0      K2 = 0      K1 = 0.123976      K0 = 2.60209  
 Base: Area  
 Ref.channel: chl  
 ISTD:  
 Formula: Linear  
 Weight: 1

| Level | Height | Area  | Conc. | Vol/Dil | Retention | Used | File |
|-------|--------|-------|-------|---------|-----------|------|------|
| 1     | 0      | 0     | 0     | 0       | 0         |      | 0    |
| 2     | 5.363  | 86.66 | 0.6   | 20      | 9.035     |      |      |
| 3     | 10.6   | 172.6 | 1.2   | 20      | 9.035     |      |      |
| 4     | 13.2   | 215.7 | 1.5   | 20      | 9.035     |      |      |
| 5     | 28.36  | 458   | 3     | 20      | 9.035     |      |      |
| 6     | 58.28  | 935.1 | 6     | 20      | 9.035     |      |      |
| 7     | 74.06  | 1200  | 7.5   | 20      | 9.035     |      |      |

8

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-111722.mtw  
 Equation:  $Q = 0.0550348 \cdot A + 4.49555$   
 RSD: 2.433 %  
 Correlation coefficient: 0.999677

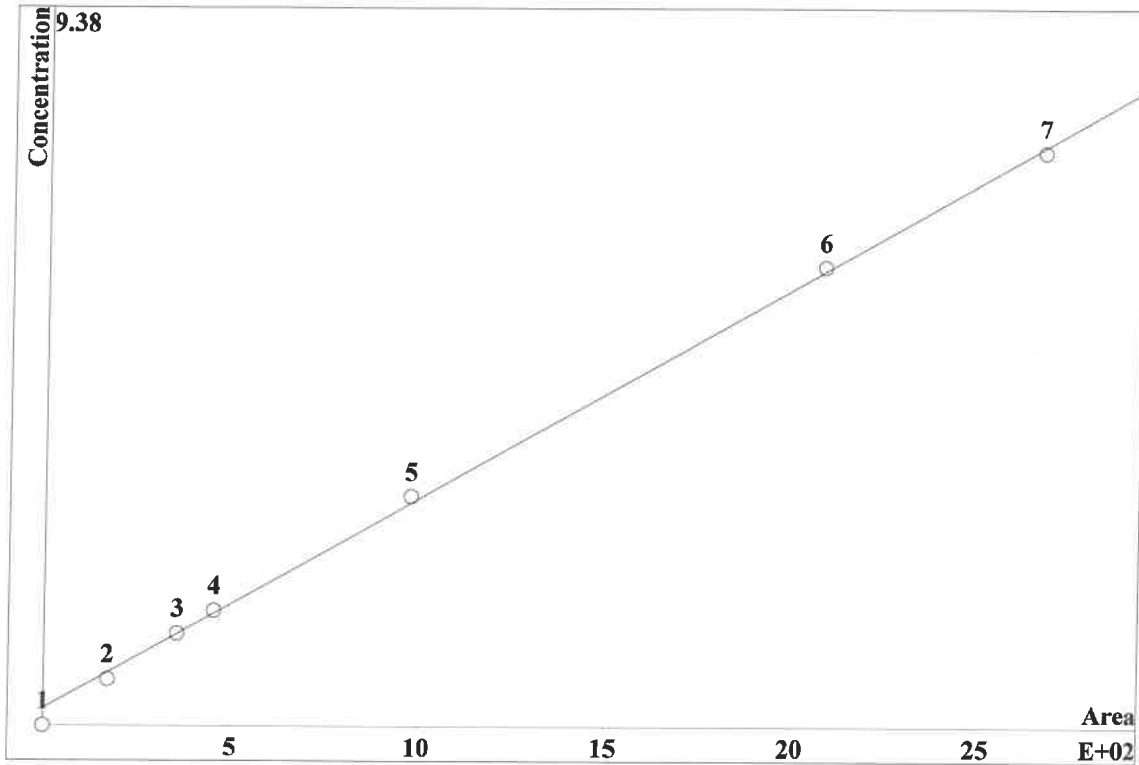


K3 = 0      K2 = 0      K1 = 0.0550348      K0 = 4.49555  
 Base: Area  
 Ref.channel: chl  
 ISTD:  
 Formula: Linear  
 Weight: 1

| Level | Height | Area  | Conc. | Vol/Dil | Retention | Used | File |
|-------|--------|-------|-------|---------|-----------|------|------|
| 1     | 0      | 0     | 0     | 0       | 0         |      | 0    |
| 2     | 8.357  | 171.6 | 0.6   | 20      | 10.93     |      |      |
| 3     | 16.93  | 354.9 | 1.2   | 20      | 10.93     |      |      |
| 4     | 21.77  | 451.9 | 1.5   | 20      | 10.93     |      |      |
| 5     | 46.72  | 977.8 | 3     | 20      | 10.93     |      |      |
| 6     | 94     | 2079  | 6     | 20      | 10.93     |      |      |
| 7     | 118.6  | 2670  | 7.5   | 20      | 10.93     |      |      |

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-111722.mtw  
 Equation:  $Q = 0.276738 \cdot A + 10.5754$   
 RSD: 2.120 %  
 Correlation coefficient: 0.999755

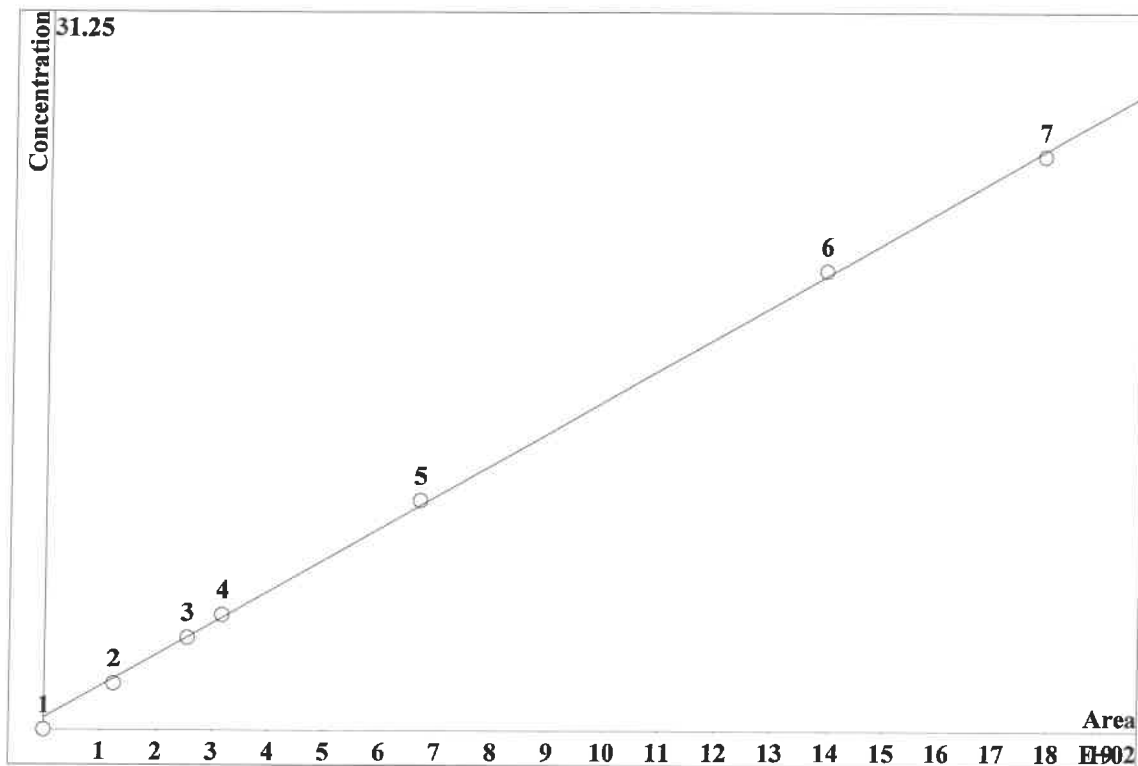


K3 = 0      K2 = 0      K1 = 0.276738      K0 = 10.5754  
 Base: Area  
 Ref.channel: ch1  
 ISTD:  
 Formula: Linear  
 Weight: 1

| Level | Height | Area  | Conc. | Vol/Dil | Retention | Used | File |
|-------|--------|-------|-------|---------|-----------|------|------|
| 1     | 0      | 0     | 0     | 0       | 0         |      |      |
| 2     | 5.489  | 123.8 | 2     | 20      | 14.56     |      |      |
| 3     | 11.12  | 254.3 | 4     | 20      | 14.56     |      |      |
| 4     | 13.86  | 315.5 | 5     | 20      | 14.56     |      |      |
| 5     | 30.24  | 669.3 | 10    | 20      | 14.56     |      |      |
| 6     | 64.02  | 1392  | 20    | 20      | 14.56     |      |      |
| 7     | 82.52  | 1786  | 25    | 20      | 14.56     |      |      |

## CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-111722.mtw  
 Equation:  $Q = 0.0488012 \cdot A + 2.54691$   
 RSD: 2.317 %  
 Correlation coefficient: 0.999707

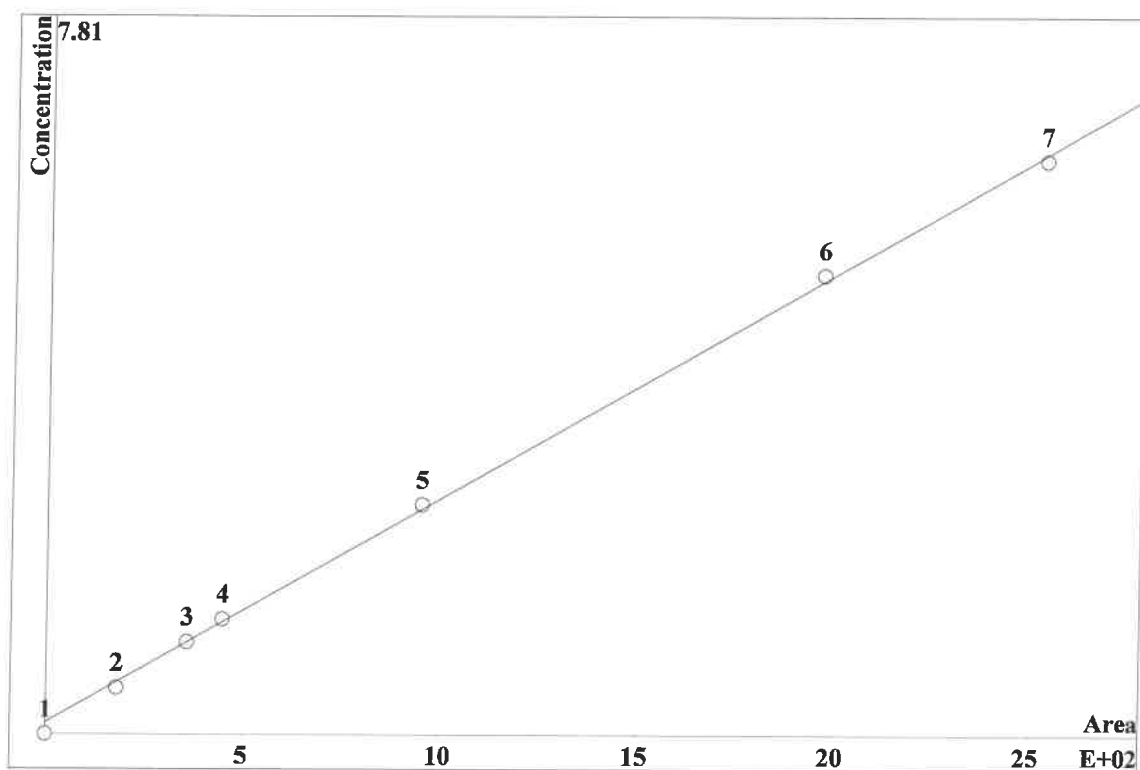


K3 = 0      K2 = 0      K1 = 0.0488012      K0 = 2.54691  
 Base: Area  
 Ref.channel: ch1  
 ISTD:  
 Formula: Linear  
 Weight: 1

| Level | Height | Area  | Conc. | Vol/Dil | Retention | Used | File |
|-------|--------|-------|-------|---------|-----------|------|------|
| 1     | 0      | 0     | 0     | 0       | 0         |      | 0    |
| 2     | 6.471  | 180.6 | 0.5   | 20      | 16.64     |      |      |
| 3     | 12.89  | 359.4 | 1     | 20      | 16.64     |      |      |
| 4     | 16.06  | 448.7 | 1.25  | 20      | 16.64     |      |      |
| 5     | 34.53  | 952.7 | 2.5   | 20      | 16.64     |      |      |
| 6     | 71.94  | 1971  | 5     | 20      | 16.64     |      |      |
| 7     | 92.61  | 2537  | 6.25  | 20      | 16.64     |      |      |

## CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-111722.mtw  
 Equation:  $Q = 0.0612059 \cdot A + 7.76808$   
 RSD: 1.443 %  
 Correlation coefficient: 0.999887

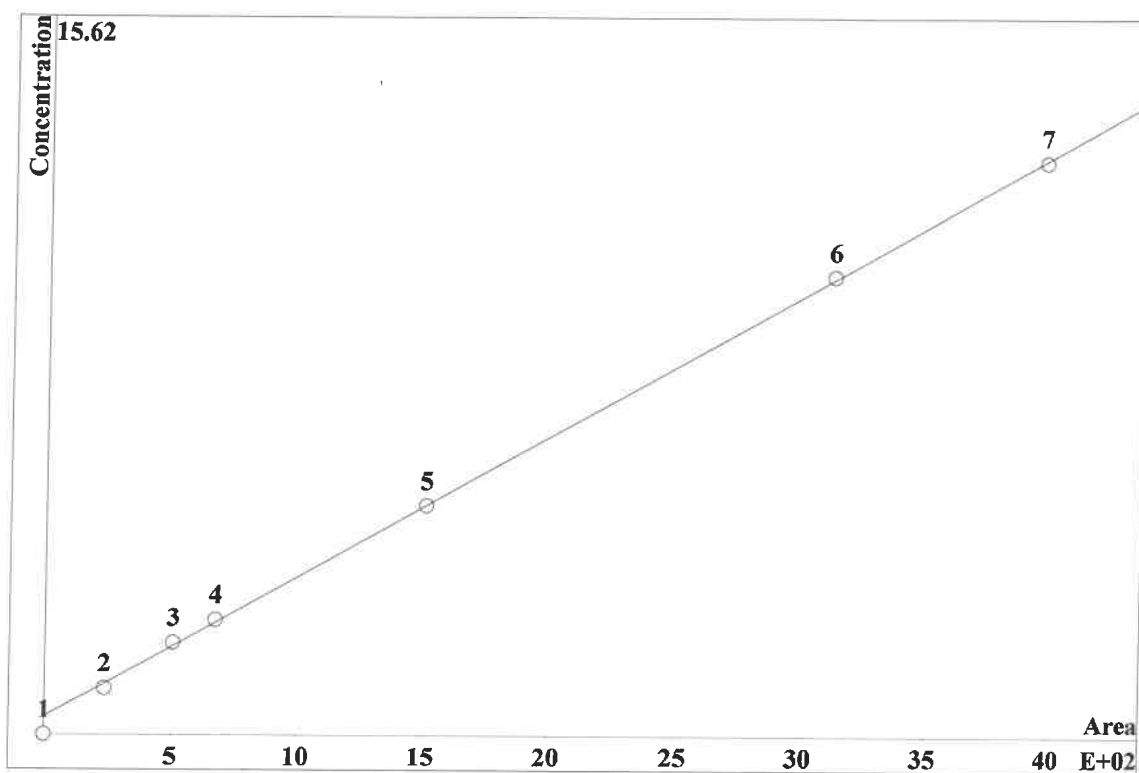


K3 = 0      K2 = 0      K1 = 0.0612059      K0 = 7.76808  
 Base: Area  
 Ref.channel: ch1  
 ISTD:  
 Formula: Linear  
 Weight: 1

| Level | Height | Area  | Conc. | Vol/Dil | Retention | Used | File |
|-------|--------|-------|-------|---------|-----------|------|------|
| 1     | 0      | 0     | 0     | 0       | 0         |      | 0    |
| 2     | 4.54   | 236.5 | 1     | 20      | 21.97     |      |      |
| 3     | 9.921  | 504.9 | 2     | 20      | 21.97     |      |      |
| 4     | 13.26  | 672.8 | 2.5   | 20      | 21.97     |      |      |
| 5     | 30.82  | 1511  | 5     | 20      | 21.97     |      |      |
| 6     | 66.43  | 3123  | 10    | 20      | 21.97     |      |      |
| 7     | 86.31  | 3973  | 12.5  | 20      | 21.97     |      |      |

## CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-111722.mtw  
 Equation:  $Q = 0.165332 \cdot A + 12.9661$   
 RSD: 1.785 %  
 Correlation coefficient: 0.999826

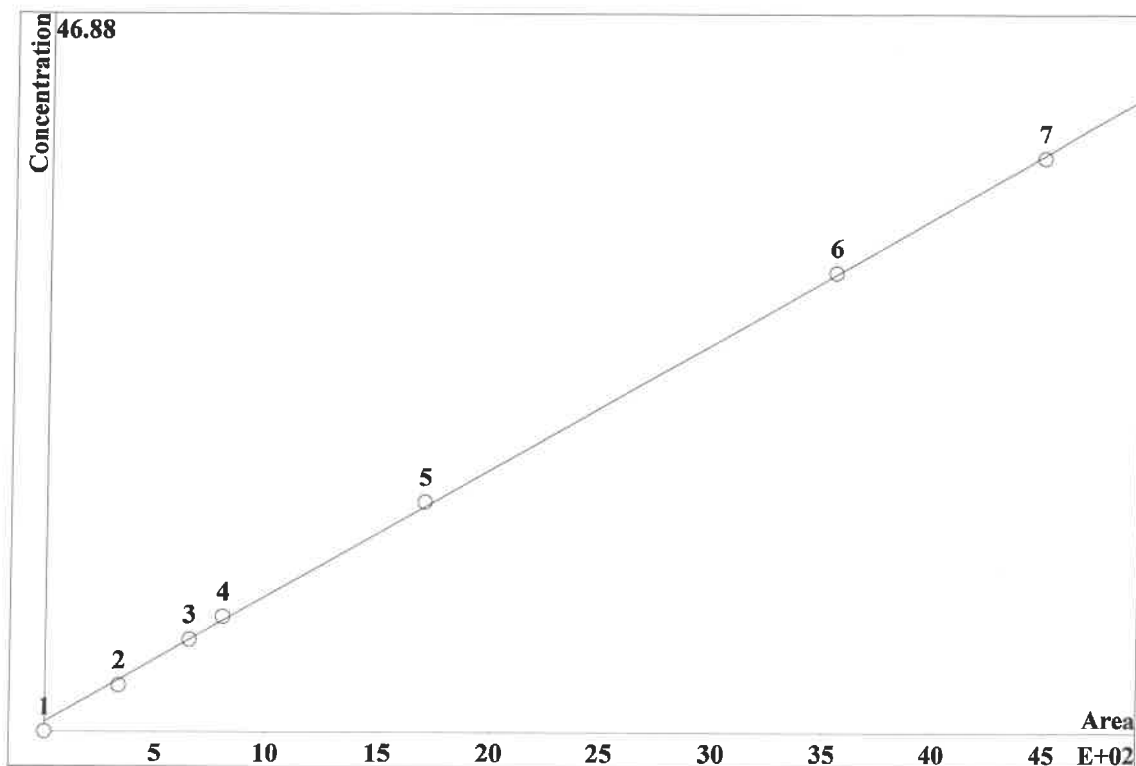

K3 = 0      K2 = 0      K1 = 0.165332      K0 = 12.9661

Base: Area

Ref.channel: ch1

ISTD:

Formula: Linear

Weight: 1

| Level | Height | Area  | Conc. | Vol/Dil | Retention | Used | File |
|-------|--------|-------|-------|---------|-----------|------|------|
| 1     | 0      | 0     | 0     | 0       | 0         |      | 0    |
| 2     | 8.868  | 332.3 | 3     | 20      | 25.5      |      |      |
| 3     | 17.58  | 651.2 | 6     | 20      | 25.5      |      |      |
| 4     | 21.79  | 801.3 | 7.5   | 20      | 25.5      |      |      |
| 5     | 46.89  | 1700  | 15    | 20      | 25.5      |      |      |
| 6     | 98.87  | 3539  | 30    | 20      | 25.5      |      |      |
| 7     | 126.9  | 4482  | 37.5  | 20      | 25.5      |      |      |

1. ☐

Report date: 11/18/2022 10:29:40 AM  
Printed by: wet


Ident: STD1  
Analysis from: 11/17/2022 11:09:27 AM  
File: \_2022-11-17\_

Last save: 11/17/2022 2:54:40 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32534

Last save: 11/17/2022 2:10

SAMPLE:  
: IZ/MA  
Vial number: 2  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

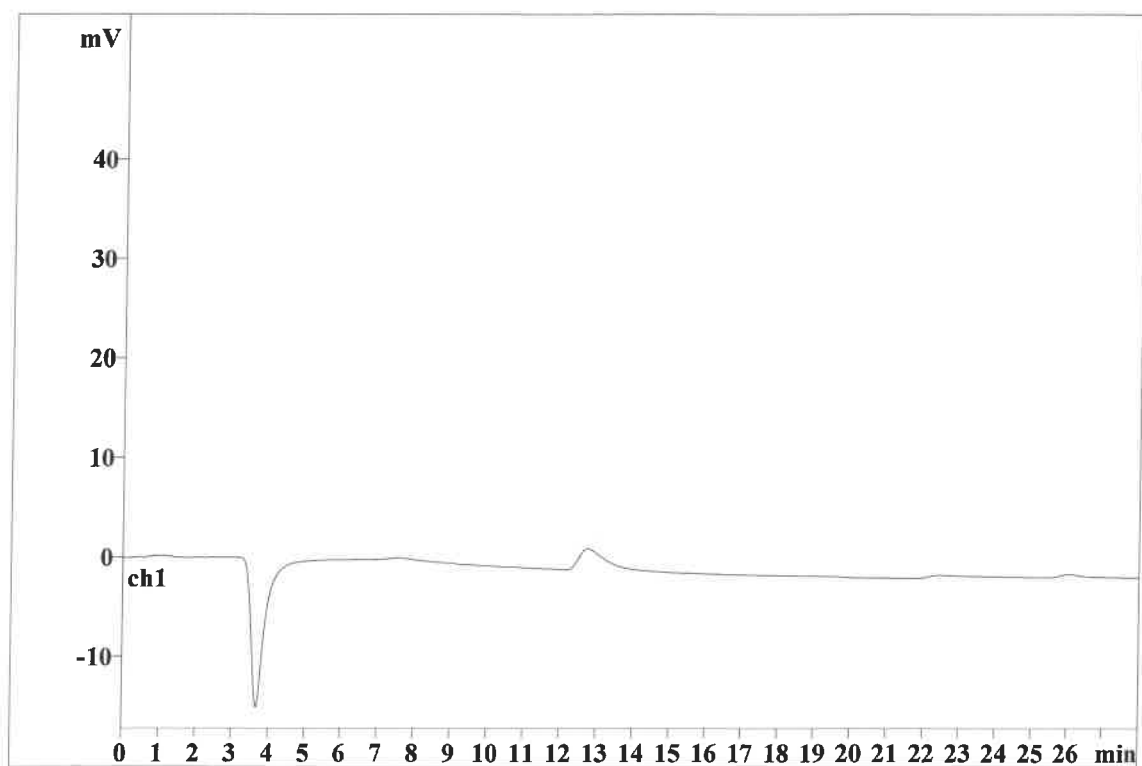

Quantitation method: Custom

No peaks

This report has been created by IC Net  
METROHM LTD

Report date: 11/18/2022 10:29:52 AM  
Printed by: wet


Ident: STD2  
Analysis from: 11/17/2022 11:40:05 AM  
File: \_2022-11-17\_

Last save: 11/17/2022 2:54:40 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32535

Last save: 11/17/2022 2:10

SAMPLE:  
: IZ/MA  
Vial number: 3  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

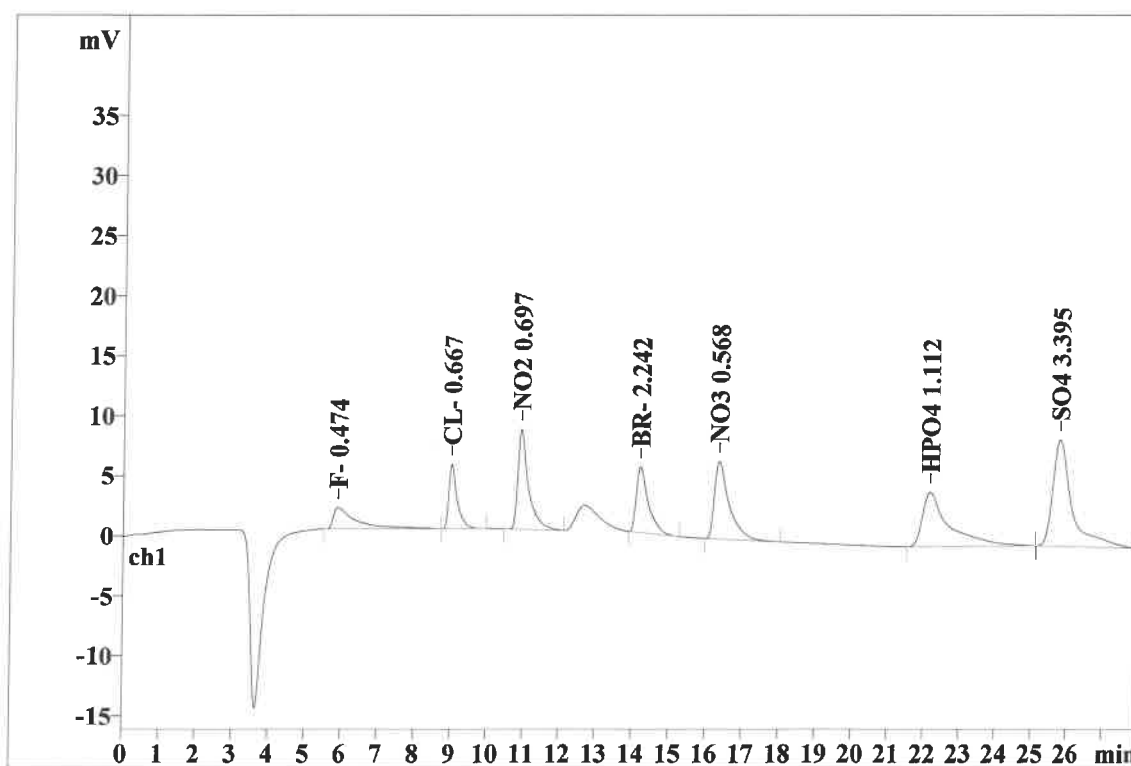

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.89             | 0.506          | 1.79         | 4.38        | 78.470         | 6.48      |
| 2  | 9.00             | 0.223          | 5.36         | 13.12       | 86.655         | 7.16      |
| 3  | 10.93            | 0.272          | 8.36         | 20.44       | 171.646        | 14.19     |
| 4  | 14.20            | 0.317          | 5.49         | 13.42       | 123.795        | 10.23     |
| 5  | 16.35            | 0.386          | 6.47         | 15.83       | 180.631        | 14.93     |
| 6  | 22.16            | 0.596          | 4.54         | 11.10       | 236.548        | 19.55     |
| 7  | 25.79            | 0.481          | 8.87         | 21.69       | 332.272        | 27.46     |
| 7  | 28.00            | 0.397          | 40.87        | 99.98       | 1210.017       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 11/18/2022 10:30:00 AM  
Printed by: wet


Ident: STD3  
Analysis from: 11/17/2022 12:10:43 PM  
File: \_2022-11-17\_

Last save: 11/17/2022 2:54:40 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32536

Last save: 11/17/2022 2:10

SAMPLE:  
: IZ/MA  
Vial number: 4  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

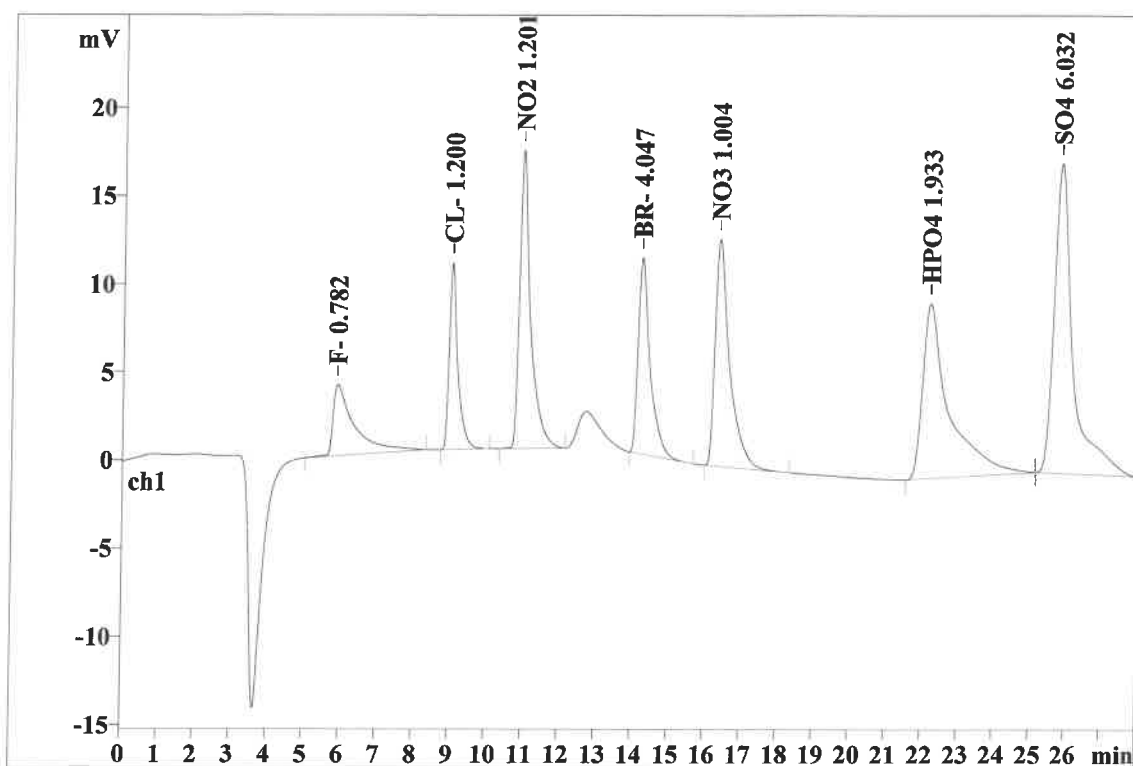

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.90             | 0.497          | 4.03         | 4.85        | 164.937        | 6.70      |
| 2  | 9.02             | 0.224          | 10.60        | 12.75       | 172.611        | 7.01      |
| 3  | 10.95            | 0.278          | 16.92        | 20.37       | 354.879        | 14.41     |
| 4  | 14.22            | 0.317          | 11.12        | 13.39       | 254.250        | 10.33     |
| 5  | 16.36            | 0.386          | 12.89        | 15.51       | 359.400        | 14.60     |
| 6  | 22.18            | 0.581          | 9.92         | 11.94       | 504.858        | 20.50     |
| 7  | 25.82            | 0.477          | 17.58        | 21.17       | 651.212        | 26.45     |
| 7  | 28.00            | 0.394          | 83.07        | 99.99       | 2462.147       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 11/18/2022 11:03:15 AM  
Printed by: wet


Ident: STD4  
Analysis from: 11/17/2022 12:41:21 PM  
File: \_2022-11-17\_

Last save: 11/17/2022 2:54:40 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32537

Last save: 11/17/2022 2:10

SAMPLE:  
: IZ/MA  
Vial number: 5  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

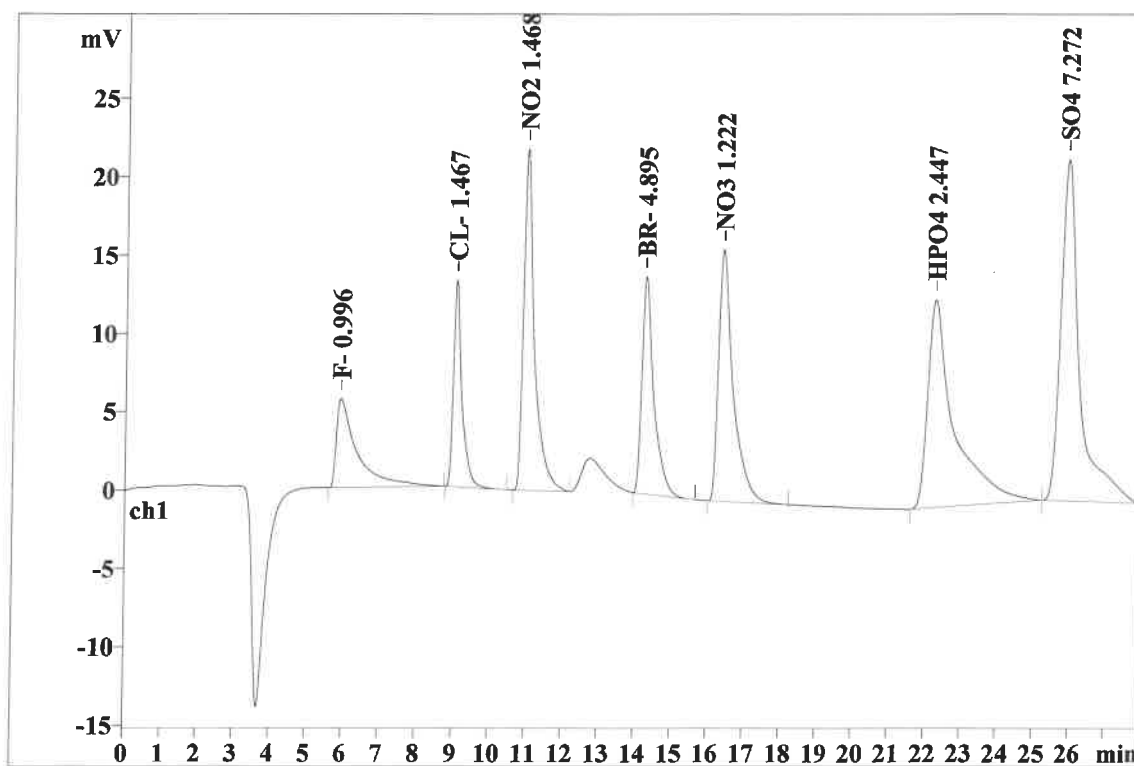

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.92             | 0.479          | 5.67         | 5.36        | 224.740        | 7.18      |
| 2  | 9.05             | 0.222          | 13.20        | 12.50       | 215.671        | 6.89      |
| 3  | 10.98            | 0.274          | 21.77        | 20.61       | 451.888        | 14.43     |
| 4  | 14.26            | 0.315          | 13.86        | 13.12       | 315.522        | 10.08     |
| 5  | 16.38            | 0.384          | 16.06        | 15.21       | 448.722        | 14.33     |
| 6  | 22.25            | 0.578          | 13.25        | 12.55       | 672.807        | 21.49     |
| 7  | 25.91            | 0.476          | 21.79        | 20.64       | 801.281        | 25.59     |
| 7  | 28.00            | 0.390          | 105.61       | 99.99       | 3130.631       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 11/18/2022 11:03:23 AM  
Printed by: wet


Ident: STD5  
Analysis from: 11/17/2022 1:11:58 PM  
File: \_2022-11-17\_

Last save: 11/17/2022 2:54:40 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32538

Last save: 11/17/2022 2:10

SAMPLE:  
: IZ/MA  
Vial number: 6  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

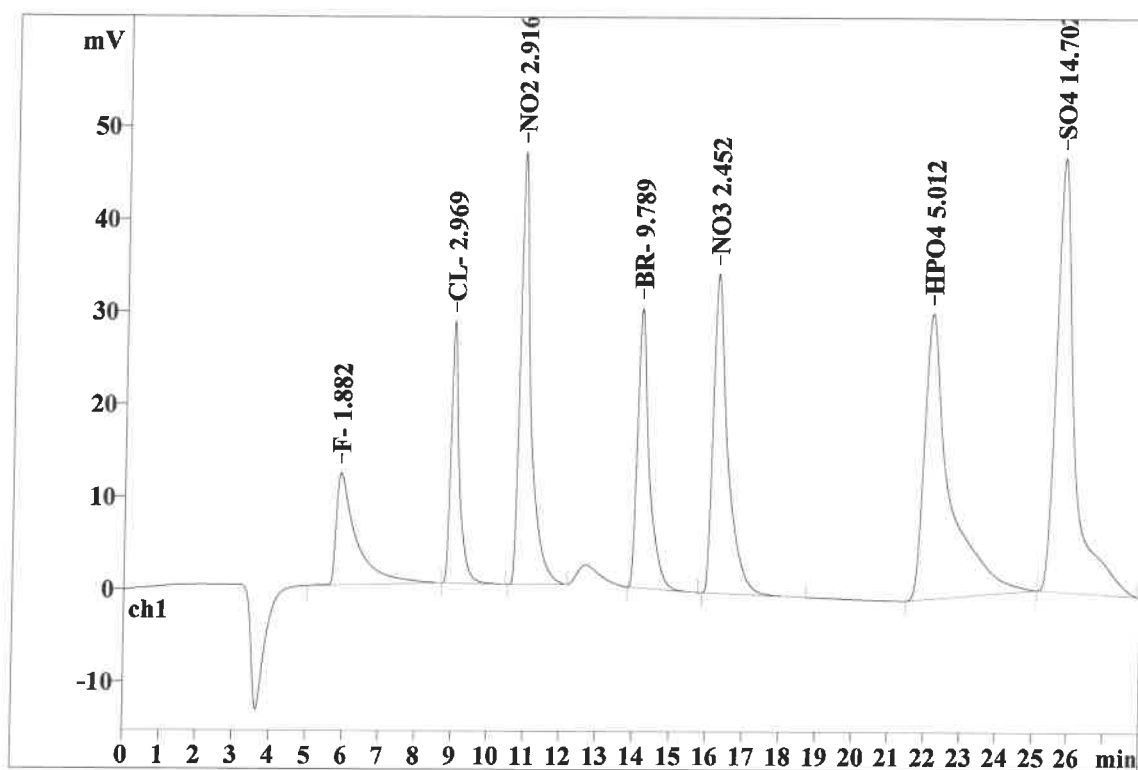

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.90             | 0.480          | 12.14        | 5.28        | 473.201        | 7.02      |
| 2  | 8.99             | 0.217          | 28.36        | 12.35       | 457.986        | 6.79      |
| 3  | 10.89            | 0.277          | 46.72        | 20.34       | 977.830        | 14.50     |
| 4  | 14.15            | 0.304          | 30.24        | 13.17       | 669.257        | 9.93      |
| 5  | 16.22            | 0.378          | 34.53        | 15.03       | 952.738        | 14.13     |
| 6  | 22.13            | 0.558          | 30.82        | 13.42       | 1510.974       | 22.41     |
| 7  | 25.77            | 0.467          | 46.89        | 20.41       | 1700.107       | 25.22     |
| 7  | 28.00            | 0.383          | 229.70       | 100.00      | 6742.092       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 11/18/2022 11:03:32 AM  
Printed by: wet


Ident: STD6  
Analysis from: 11/17/2022 1:42:36 PM  
File: \_2022-11-17\_

Last save: 11/17/2022 2:54:40 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32539

Last save: 11/17/2022 2:10

SAMPLE:  
: IZ/MA  
Vial number: 7  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

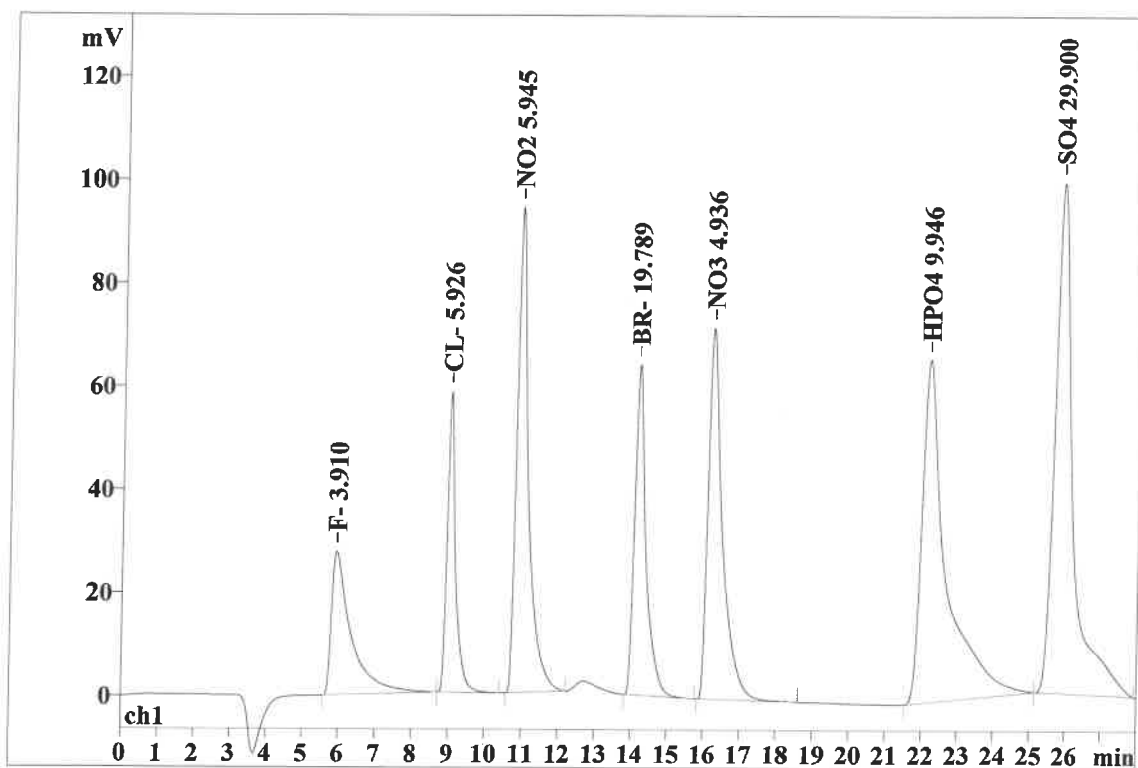

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.91             | 0.476          | 27.79        | 5.77        | 1041.813       | 7.40      |
| 2  | 9.00             | 0.216          | 58.28        | 12.11       | 935.068        | 6.64      |
| 3  | 10.89            | 0.297          | 93.99        | 19.53       | 2078.933       | 14.76     |
| 4  | 14.16            | 0.296          | 64.02        | 13.30       | 1391.957       | 9.89      |
| 5  | 16.18            | 0.375          | 71.94        | 14.95       | 1970.885       | 14.00     |
| 6  | 22.15            | 0.536          | 66.43        | 13.80       | 3123.164       | 22.18     |
| 7  | 25.82            | 0.463          | 98.87        | 20.54       | 3538.583       | 25.13     |
| 7  | 28.00            | 0.380          | 481.31       | 100.00      | 14080.402      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 11/18/2022 11:03:39 AM  
Printed by: wet


Ident: STD7  
Analysis from: 11/17/2022 2:13:13 PM  
File: \_2022-11-17\_

Last save: 11/17/2022 2:54:40 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32540

Last save: 11/17/2022 2:10

SAMPLE:  
: IZ/MA  
Vial number: 8  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

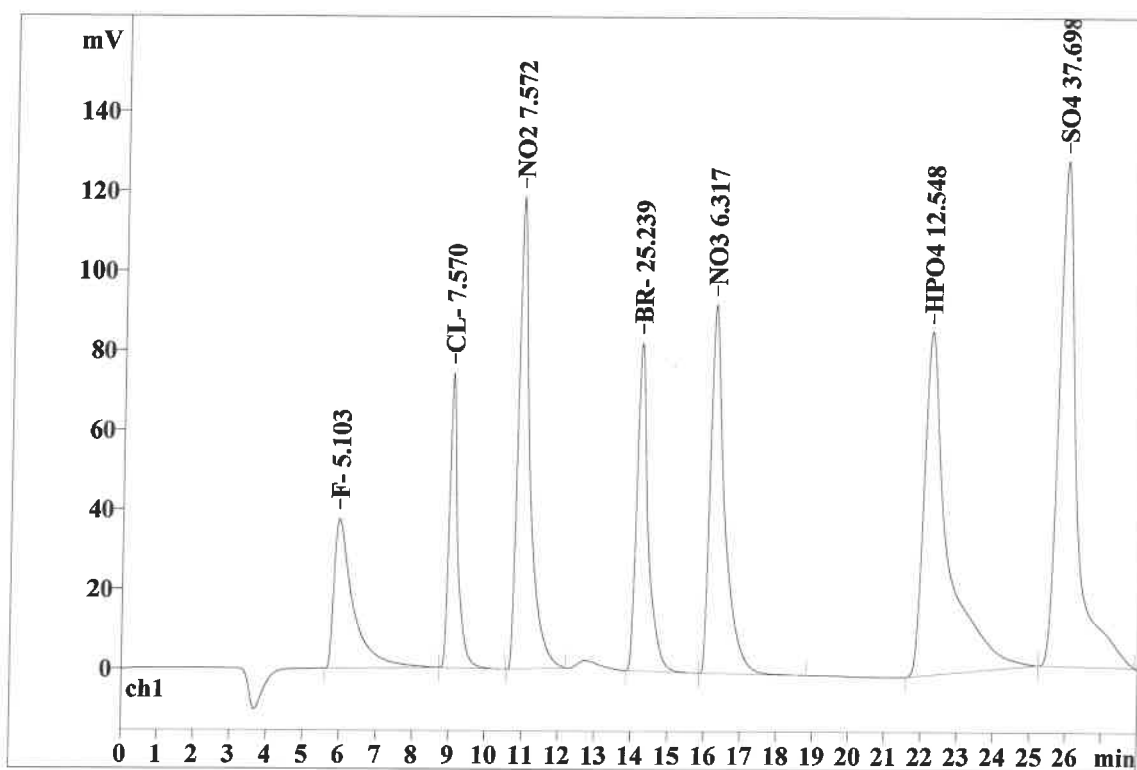

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.95             | 0.478          | 37.65        | 6.09        | 1376.113       | 7.63      |
| 2  | 9.03             | 0.217          | 74.06        | 11.97       | 1200.256       | 6.66      |
| 3  | 10.90            | 0.302          | 118.63       | 19.18       | 2670.160       | 14.81     |
| 4  | 14.19            | 0.294          | 82.52        | 13.34       | 1785.794       | 9.91      |
| 5  | 16.20            | 0.374          | 92.61        | 14.97       | 2536.621       | 14.07     |
| 6  | 22.20            | 0.525          | 86.31        | 13.95       | 3973.416       | 22.04     |
| 7  | 25.90            | 0.461          | 126.85       | 20.51       | 4481.909       | 24.87     |
| 7  | 28.00            | 0.379          | 618.62       | 100.00      | 18024.269      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 11/18/2022 11:03:53 AM  
Printed by: wet


Ident: ICV  
Analysis from: 11/17/2022 3:33:51 PM  
File: \_2022-11-17\_

Last save: 11/17/2022 4:02:51 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32542

Last save: 11/17/2022 2:55

SAMPLE:  
: IZ/MA  
Vial number: 24  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

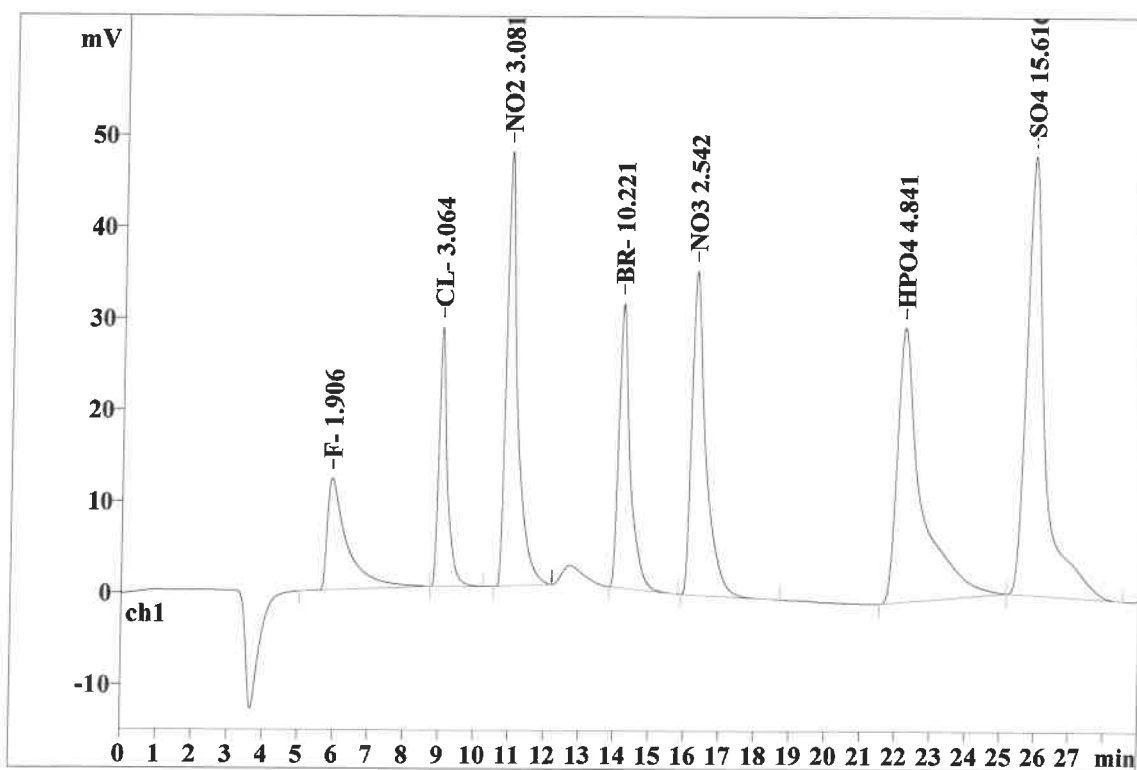

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.90             | 0.489          | 12.21        | 5.25        | 480.016        | 6.91      |
| 2  | 9.01             | 0.224          | 28.40        | 12.21       | 473.321        | 6.81      |
| 3  | 10.91            | 0.286          | 47.50        | 20.42       | 1038.150       | 14.94     |
| 4  | 14.16            | 0.309          | 31.06        | 13.36       | 700.471        | 10.08     |
| 5  | 16.24            | 0.384          | 35.41        | 15.23       | 989.558        | 14.24     |
| 6  | 22.17            | 0.551          | 30.03        | 12.91       | 1454.907       | 20.94     |
| 7  | 25.86            | 0.484          | 47.94        | 20.61       | 1810.600       | 26.06     |
| 7  | 29.00            | 0.389          | 232.55       | 100.00      | 6947.024       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 11/18/2022 11:04:02 AM  
Printed by: wet


Ident: ICB  
Analysis from: 11/17/2022 4:06:26 PM  
File: \_2022-11-17\_

Last save: 11/17/2022 4:35:26 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32543

Last save: 11/17/2022 2:55

SAMPLE:  
: IZ/MA  
Vial number: 10  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

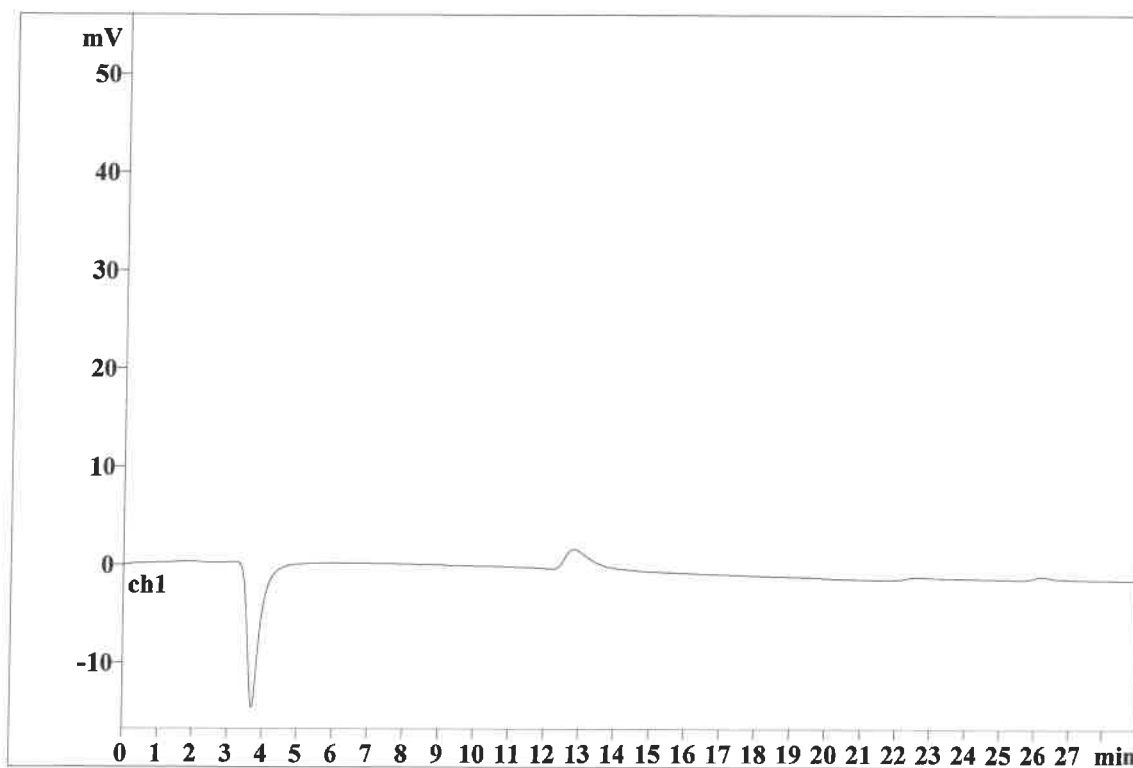

Quantitation method: Custom

No peaks

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:00:06 PM  
Printed by: wet


Ident: CCV  
Analysis from: 12/6/2022 10:30:03 AM  
File: \_2022-12-06\_

Last save: 12/6/2022 10:59:04 AM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32693

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 11  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

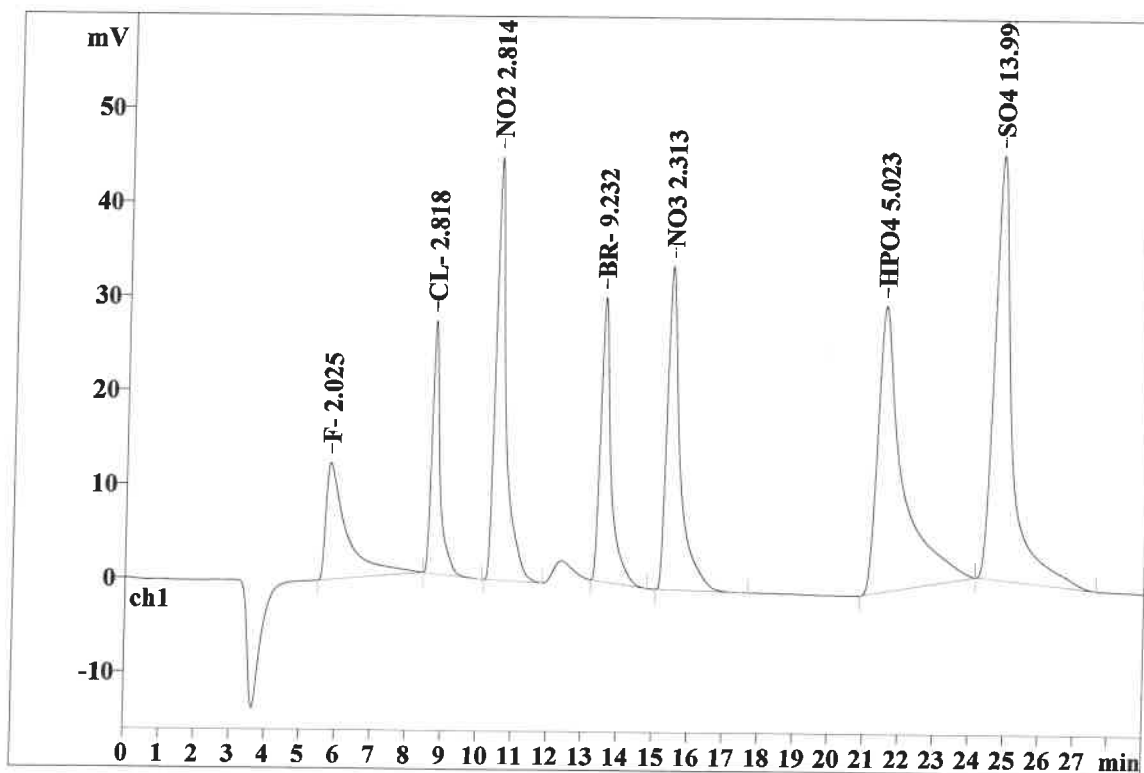

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.78             | 0.500          | 12.43        | 5.53        | 513.169        | 7.84      |
| 2  | 8.70             | 0.213          | 26.93        | 11.99       | 433.605        | 6.63      |
| 3  | 10.48            | 0.271          | 45.03        | 20.05       | 940.908        | 14.38     |
| 4  | 13.51            | 0.277          | 30.25        | 13.47       | 629.008        | 9.62      |
| 5  | 15.39            | 0.342          | 34.41        | 15.32       | 895.845        | 13.69     |
| 6  | 21.48            | 0.579          | 30.46        | 13.56       | 1514.436       | 23.15     |
| 7  | 24.75            | 0.455          | 45.11        | 20.08       | 1614.564       | 24.68     |
| 7  | 29.00            | 0.377          | 224.62       | 100.00      | 6541.535       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:00:13 PM  
Printed by: wet


Ident: CCB  
Analysis from: 12/6/2022 11:04:27 AM  
File: \_2022-12-06\_

Last save: 12/6/2022 11:33:28 AM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32694

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 12  
Volume: 20.0  $\mu$ L  
Dilution: 1.00  
Amount: 1.0000

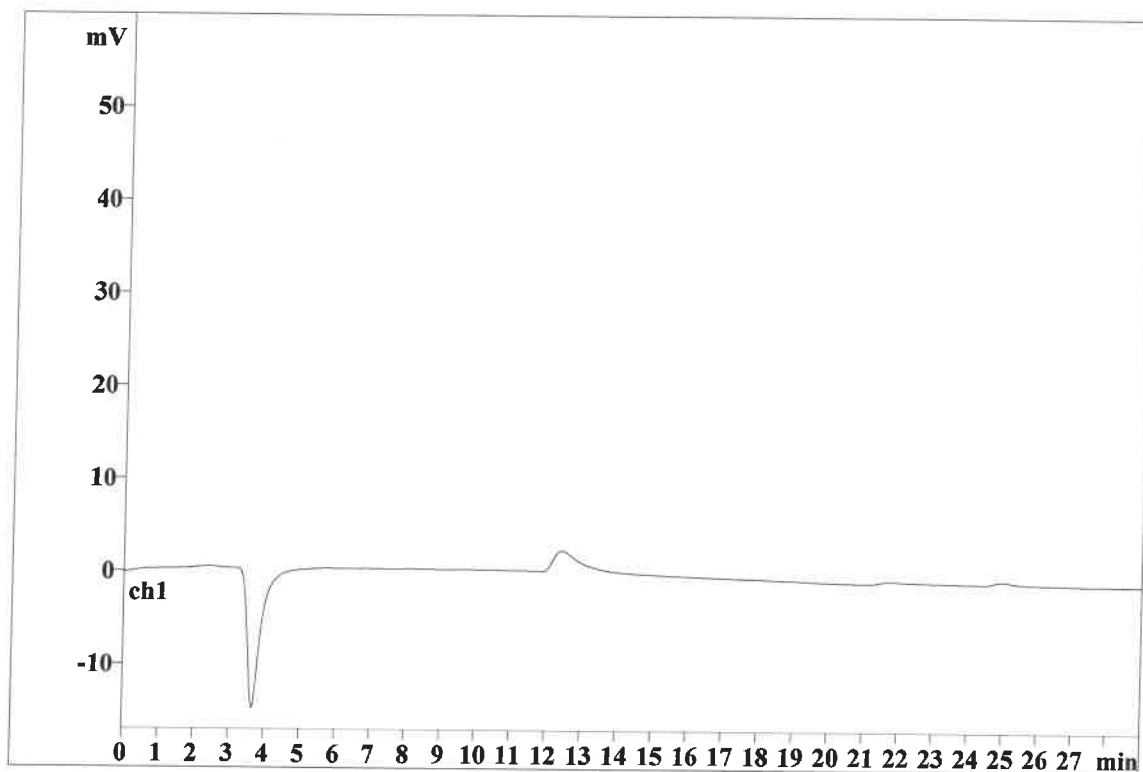

Quantitation method: Custom

No peaks

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:00:20 PM  
Printed by: wet


Ident: LB123150BLW  
Analysis from: 12/6/2022 11:36:05 AM  
File: \_2022-12-06\_

Last save: 12/7/2022 2:58:30 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32695

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 13  
Volume: 20.0  $\mu$ L  
Dilution: 1.00  
Amount: 1.0000

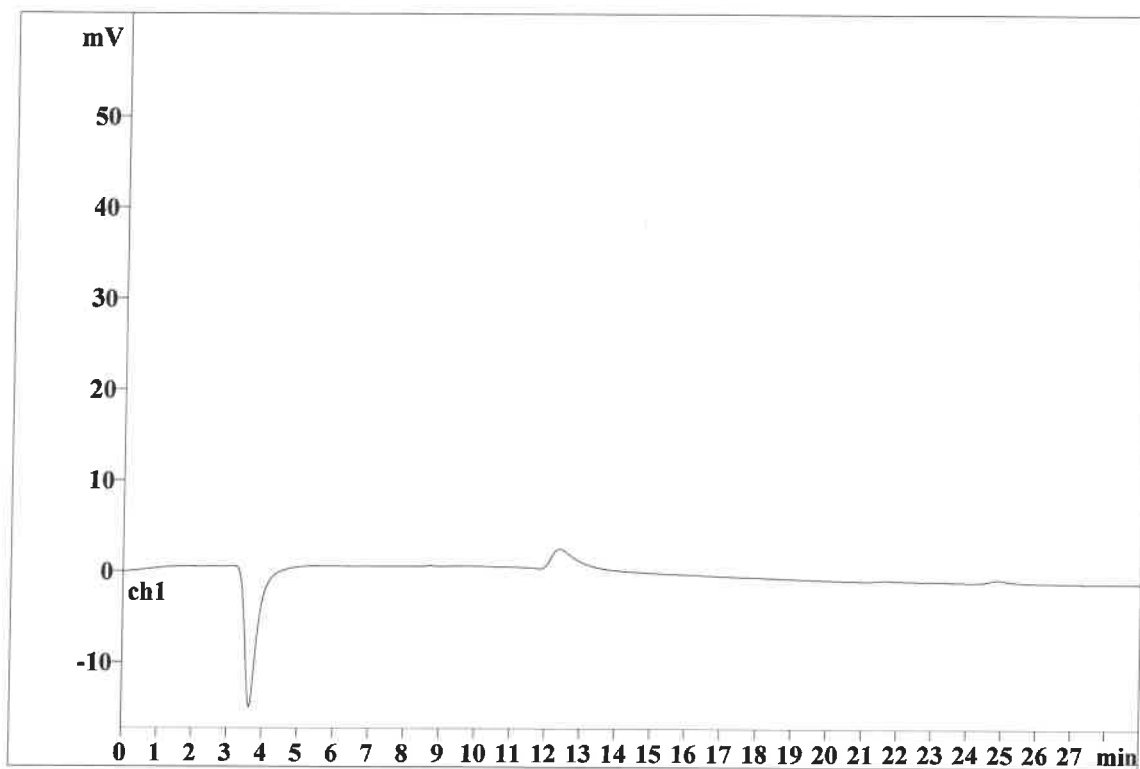

Quantitation method: Custom

No peaks

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:00:27 PM  
Printed by: wet


Ident: LB123150BSW  
Analysis from: 12/6/2022 12:07:43 PM  
File: \_2022-12-06\_

Last save: 12/7/2022 2:58:30 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32696

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 14  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

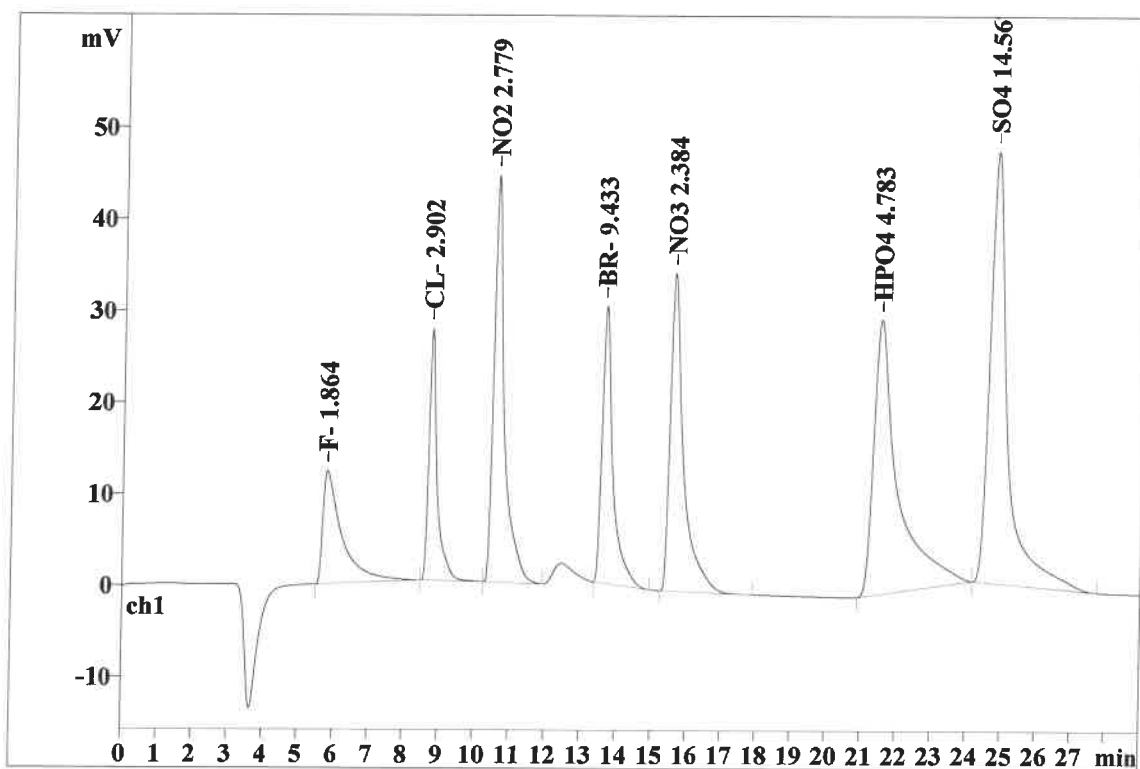

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.79             | 0.487          | 12.36        | 5.46        | 468.295        | 7.17      |
| 2  | 8.76             | 0.213          | 27.47        | 12.14       | 447.151        | 6.85      |
| 3  | 10.57            | 0.271          | 44.39        | 19.62       | 928.344        | 14.21     |
| 4  | 13.65            | 0.282          | 30.29        | 13.38       | 643.517        | 9.85      |
| 5  | 15.58            | 0.350          | 34.69        | 15.33       | 924.772        | 14.16     |
| 6  | 21.50            | 0.558          | 29.98        | 13.25       | 1435.994       | 21.98     |
| 7  | 24.78            | 0.455          | 47.09        | 20.81       | 1683.760       | 25.78     |
| 7  | 29.00            | 0.374          | 226.28       | 100.00      | 6531.834       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:00:43 PM  
Printed by: wet


Ident: N5841-01  
Analysis from: 12/6/2022 12:50:20 PM  
File: \_2022-12-06\_

Last save: 12/6/2022 1:19:20 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32697

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 17  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

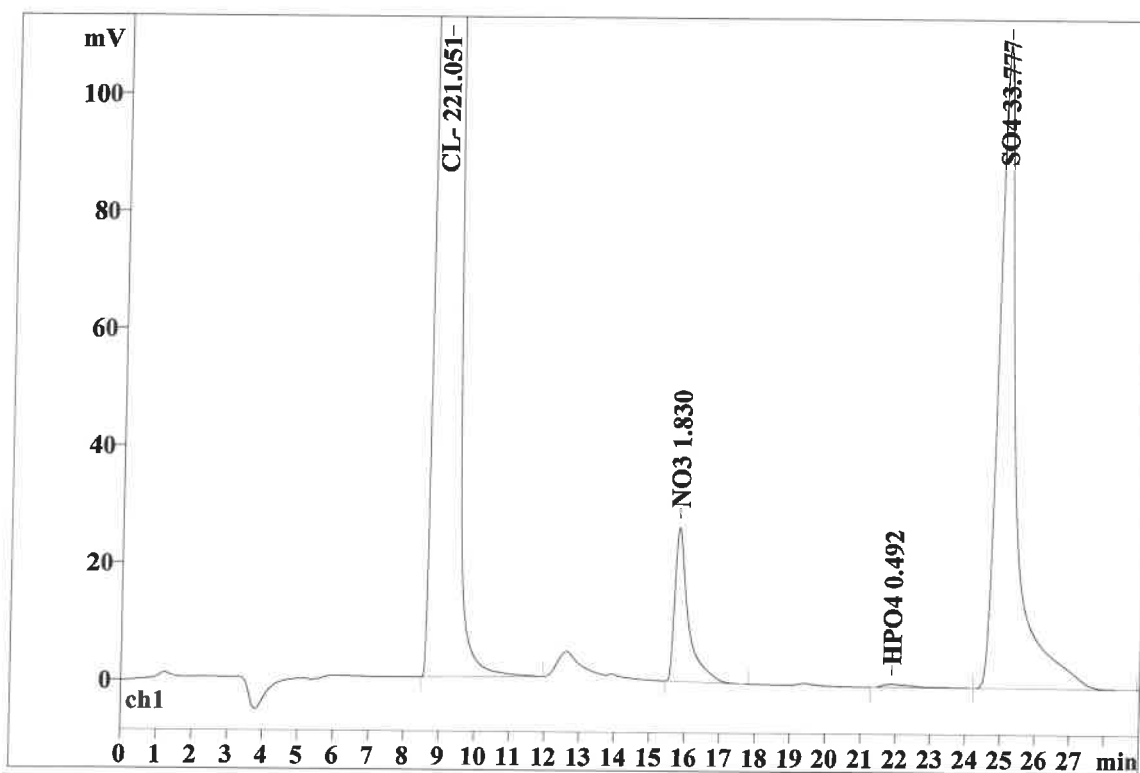

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 9.02             | 0.355          | 1497.61      | 91.65       | 35639.470      | 88.26     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 15.80            | 0.344          | 26.29        | 1.61        | 697.910        | 1.73      |
| 6  | 21.87            | 0.865          | 0.56         | 0.03        | 33.791         | 0.08      |
| 7  | 24.98            | 0.456          | 109.51       | 6.70        | 4007.491       | 9.92      |
| 7  | 29.00            | 0.289          | 1633.97      | 99.99       | 40378.662      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:00:53 PM  
Printed by: wet


Ident: N5841-03  
Analysis from: 12/6/2022 1:21:58 PM  
File: \_2022-12-06\_

Last save: 12/6/2022 1:50:58 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32698

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 18  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

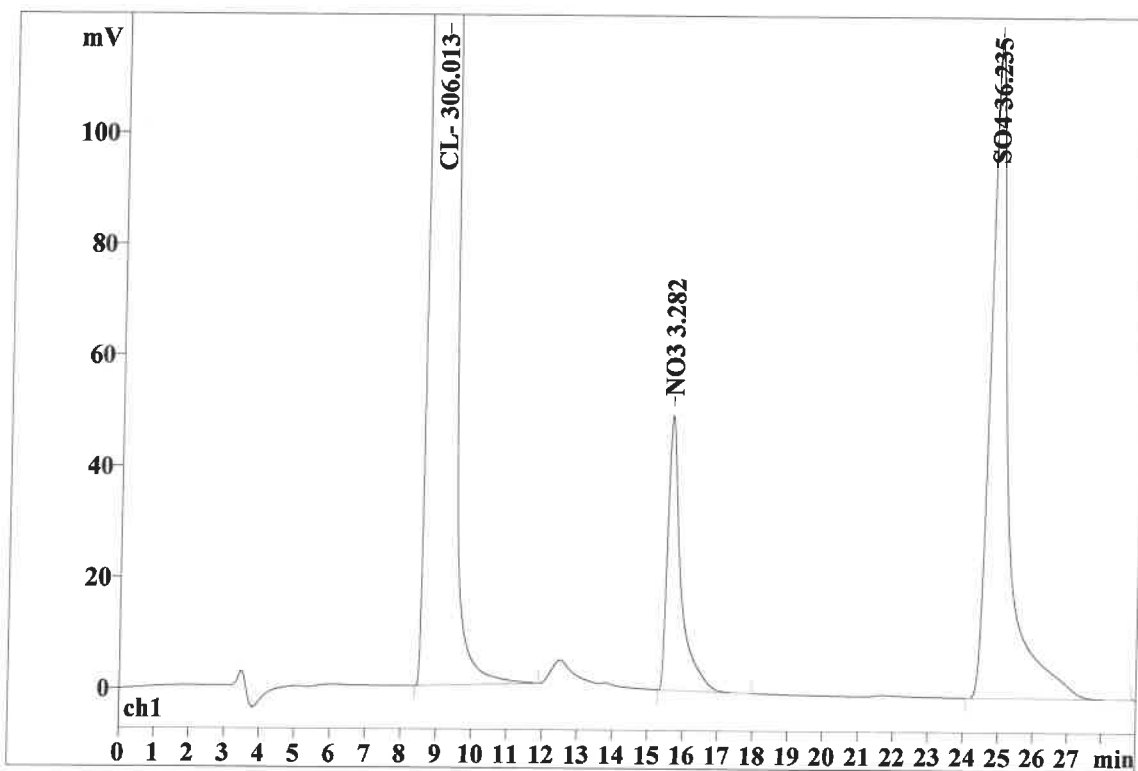

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 9.06             | 0.494          | 1581.71      | 90.42       | 49345.761      | 89.81     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 15.62            | 0.338          | 49.46        | 2.83        | 1293.034       | 2.35      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 24.81            | 0.454          | 118.10       | 6.75        | 4304.833       | 7.83      |
| 7  | 29.00            | 0.184          | 1749.27      | 100.00      | 54943.629      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:01:01 PM  
Printed by: wet


Ident: N5841-05  
Analysis from: 12/6/2022 1:53:35 PM  
File: \_2022-12-06\_

Last save: 12/6/2022 2:22:35 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32699

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 19  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

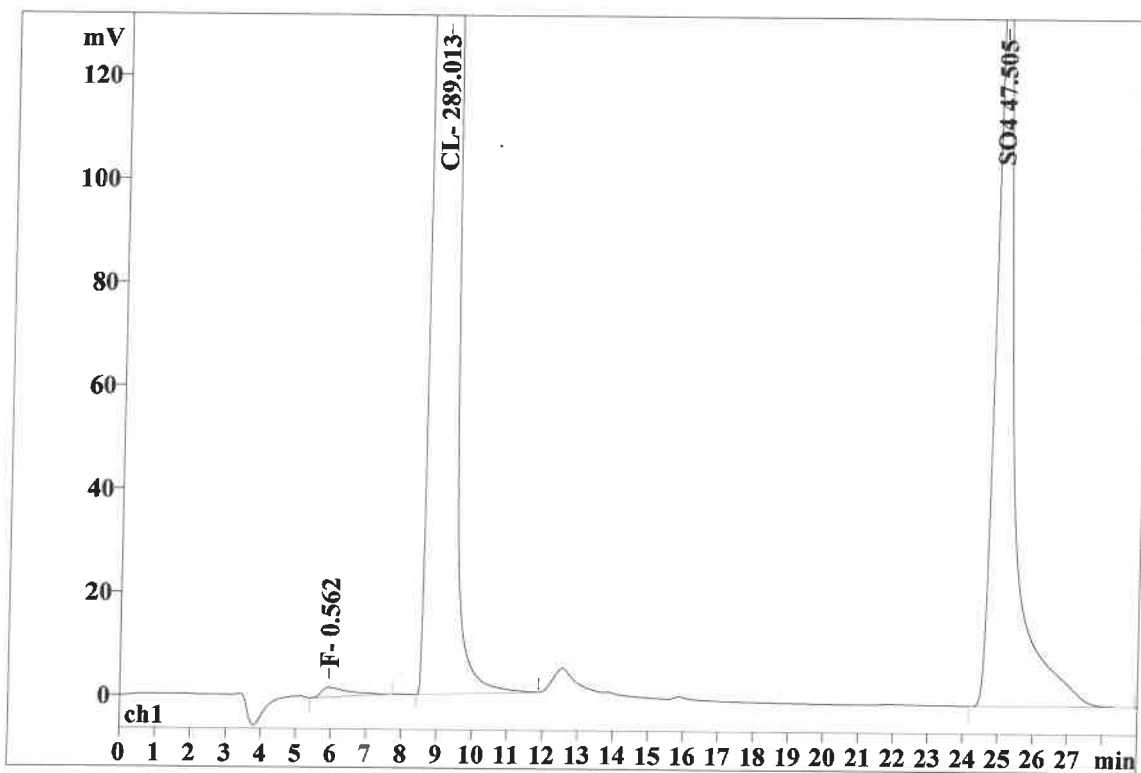

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.93             | 0.762          | 1.91         | 0.11        | 103.181        | 0.20      |
| 2  | 9.06             | 0.466          | 1568.78      | 90.93       | 46603.284      | 88.98     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 24.95            | 0.456          | 154.37       | 8.95        | 5668.157       | 10.82     |
| 7  | 29.00            | 0.241          | 1725.06      | 99.99       | 52374.623      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:01:10 PM  
Printed by: wet


Ident: N5841-07  
Analysis from: 12/6/2022 2:25:23 PM  
File: \_2022-12-06\_

Last save: 12/6/2022 2:54:23 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32700

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 20  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

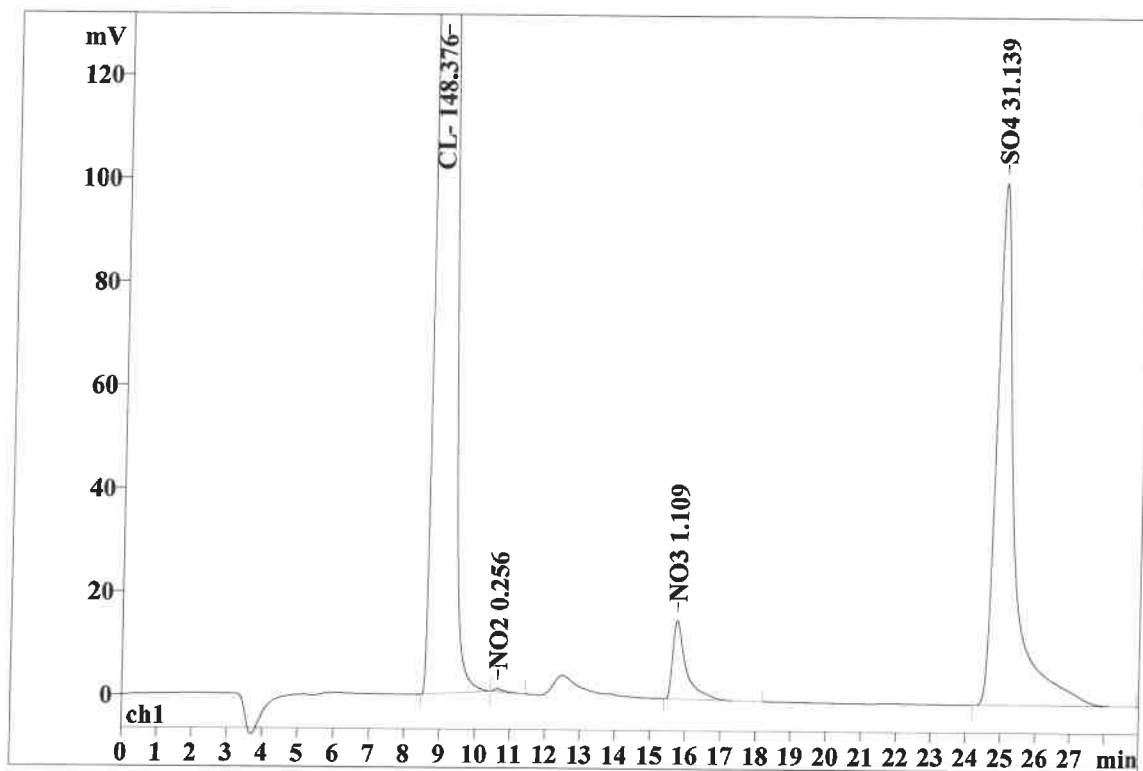

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 8.90             | 0.248          | 1340.09      | 91.98       | 23915.281      | 85.36     |
| 3  | 10.65            | 0.260          | 0.60         | 0.04        | 11.462         | 0.04      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 15.74            | 0.344          | 15.17        | 1.04        | 402.112        | 1.44      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 24.95            | 0.454          | 101.05       | 6.94        | 3688.385       | 13.16     |
| 7  | 29.00            | 0.187          | 1456.91      | 100.00      | 28017.239      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:01:16 PM  
Printed by: wet


Ident: N5841-09  
Analysis from: 12/6/2022 3:18:57 PM  
File: \_2022-12-06\_

Last save: 12/6/2022 3:47:57 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32701

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 21  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

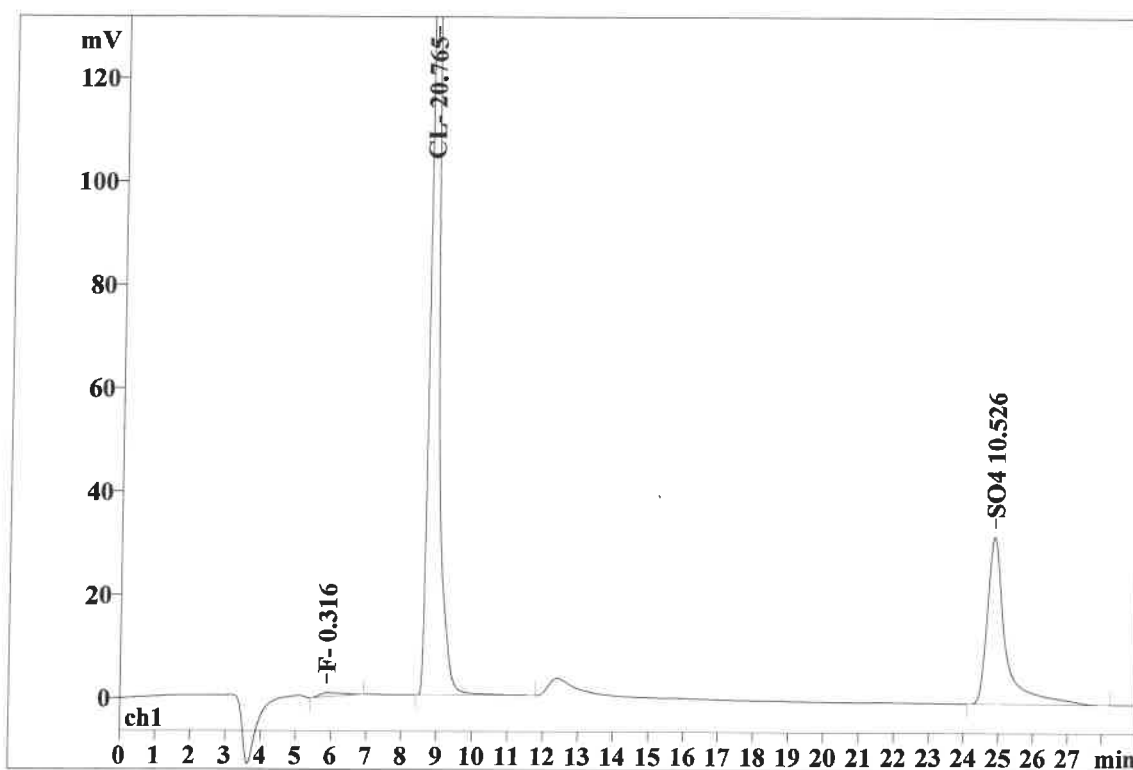

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.87             | 0.731          | 0.76         | 0.30        | 34.346         | 0.75      |
| 2  | 8.76             | 0.195          | 220.36       | 86.93       | 3328.916       | 73.03     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 24.84            | 0.459          | 32.36        | 12.76       | 1194.885       | 26.21     |
| 7  | 29.00            | 0.198          | 253.48       | 100.00      | 4558.147       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:01:23 PM  
Printed by: wet


Ident: N5841-11  
Analysis from: 12/6/2022 3:50:36 PM  
File: \_2022-12-06\_

Last save: 12/6/2022 4:19:36 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32702

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 22  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

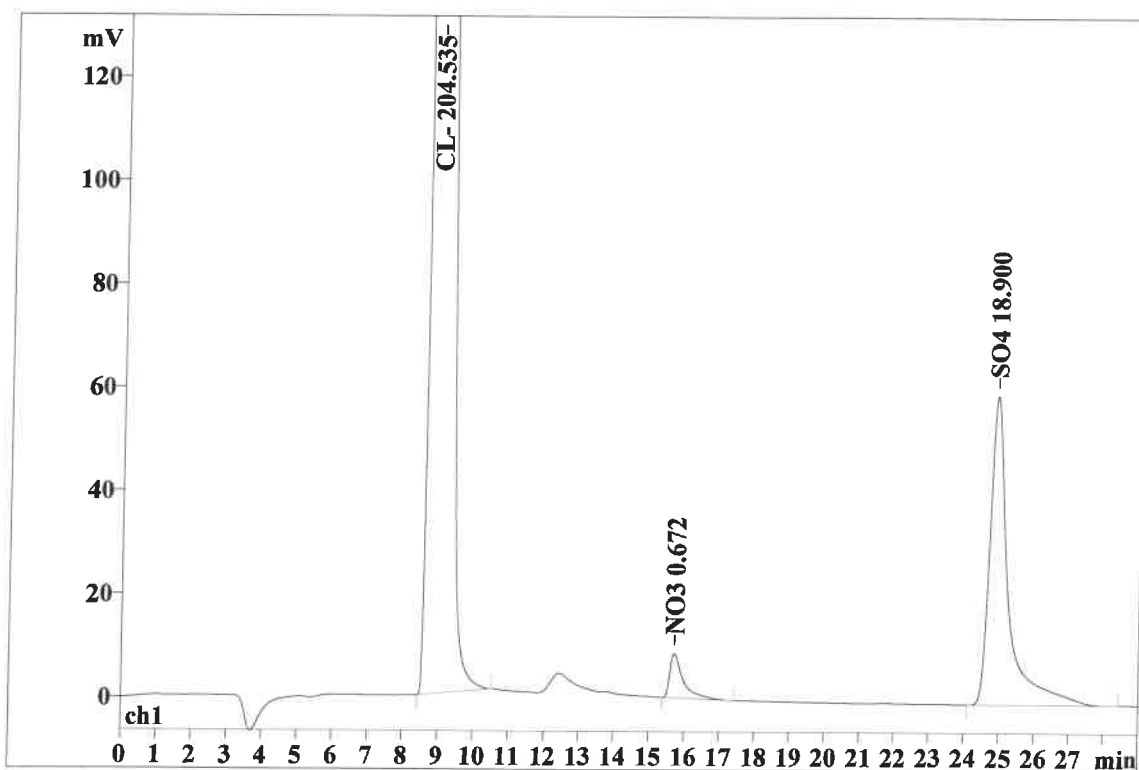

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 8.94             | 0.329          | 1481.02      | 95.60       | 32975.107      | 93.13     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 15.72            | 0.341          | 8.53         | 0.55        | 223.013        | 0.63      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 24.88            | 0.458          | 59.70        | 3.85        | 2207.931       | 6.24      |
| 7  | 29.00            | 0.161          | 1549.25      | 100.00      | 35406.051      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:01:30 PM  
Printed by: wet


Ident: N5841-13  
Analysis from: 12/6/2022 4:22:14 PM  
File: \_2022-12-06\_

Last save: 12/6/2022 4:51:14 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32703

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 23  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

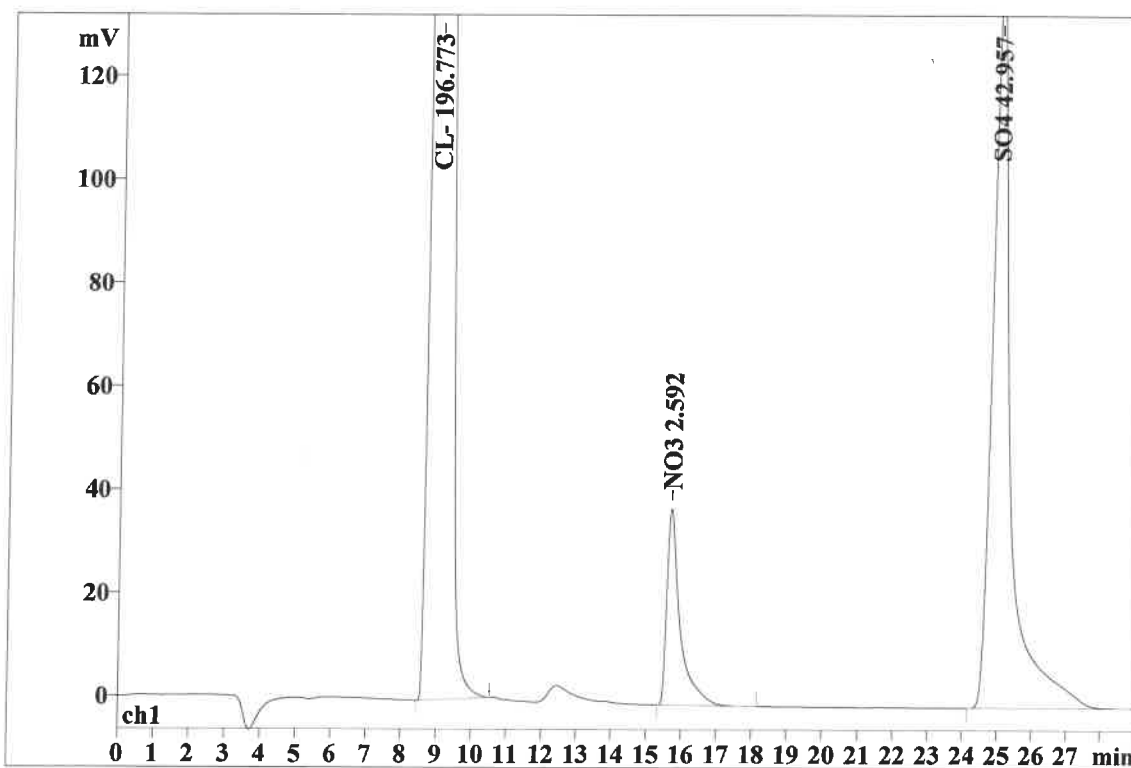

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 8.97             | 0.318          | 1467.73      | 89.11       | 31722.860      | 83.81     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 15.67            | 0.343          | 38.05        | 2.31        | 1010.192       | 2.67      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 24.92            | 0.453          | 141.32       | 8.58        | 5118.065       | 13.52     |
| 7  | 29.00            | 0.159          | 1647.10      | 100.00      | 37851.117      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:01:39 PM  
Printed by: wet


Ident: N5841-15  
Analysis from: 12/6/2022 4:53:56 PM  
File: \_2022-12-06\_

Last save: 12/6/2022 5:22:56 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32704

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 24  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

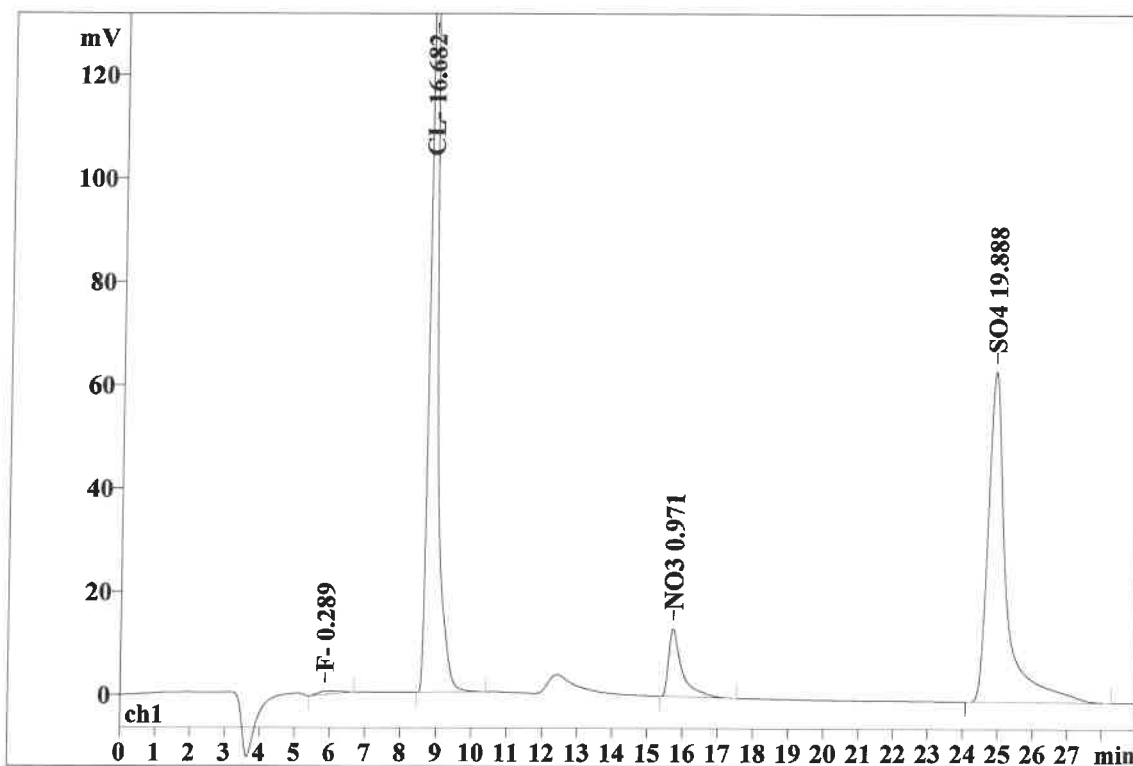

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.85             | 0.685          | 0.65         | 0.26        | 26.684         | 0.50      |
| 2  | 8.77             | 0.200          | 173.05       | 69.00       | 2670.238       | 49.73     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 15.71            | 0.341          | 13.10        | 5.22        | 345.705        | 6.44      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 24.85            | 0.453          | 63.99        | 25.52       | 2327.348       | 43.34     |
| 7  | 29.00            | 0.240          | 250.79       | 100.00      | 5369.975       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:01:48 PM  
Printed by: wet


Ident: CCV  
Analysis from: 12/6/2022 5:25:39 PM  
File: \_2022-12-06\_

Last save: 12/6/2022 5:54:39 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32705

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 11  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

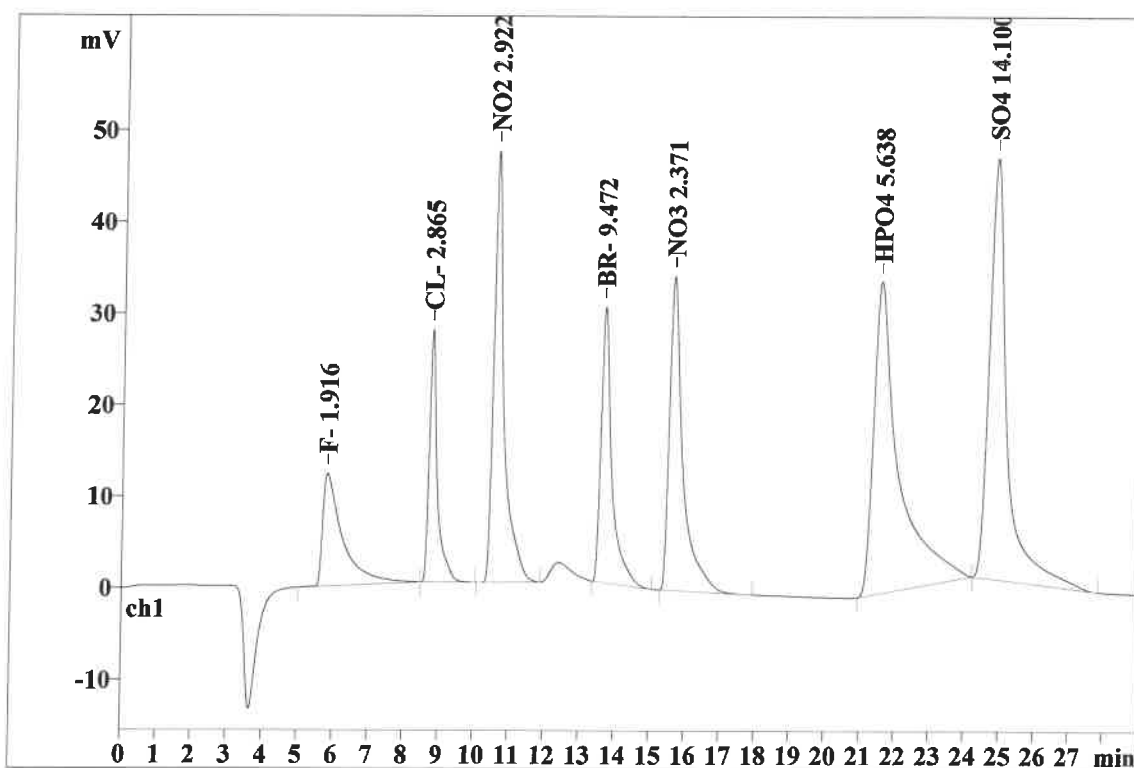

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.80             | 0.505          | 12.33        | 5.32        | 482.616        | 7.08      |
| 2  | 8.77             | 0.209          | 27.61        | 11.92       | 441.202        | 6.48      |
| 3  | 10.58            | 0.267          | 47.09        | 20.34       | 980.053        | 14.39     |
| 4  | 13.66            | 0.282          | 30.11        | 13.00       | 646.351        | 9.49      |
| 5  | 15.61            | 0.349          | 34.33        | 14.83       | 919.499        | 13.50     |
| 6  | 21.53            | 0.590          | 34.10        | 14.73       | 1715.546       | 25.18     |
| 7  | 24.81            | 0.454          | 45.97        | 19.85       | 1627.284       | 23.89     |
| 7  | 29.00            | 0.379          | 231.55       | 100.00      | 6812.551       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:01:55 PM  
Printed by: wet


Ident: CCB  
Analysis from: 12/6/2022 5:57:17 PM  
File: \_2022-12-06\_

Last save: 12/6/2022 6:26:17 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32706

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 12  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

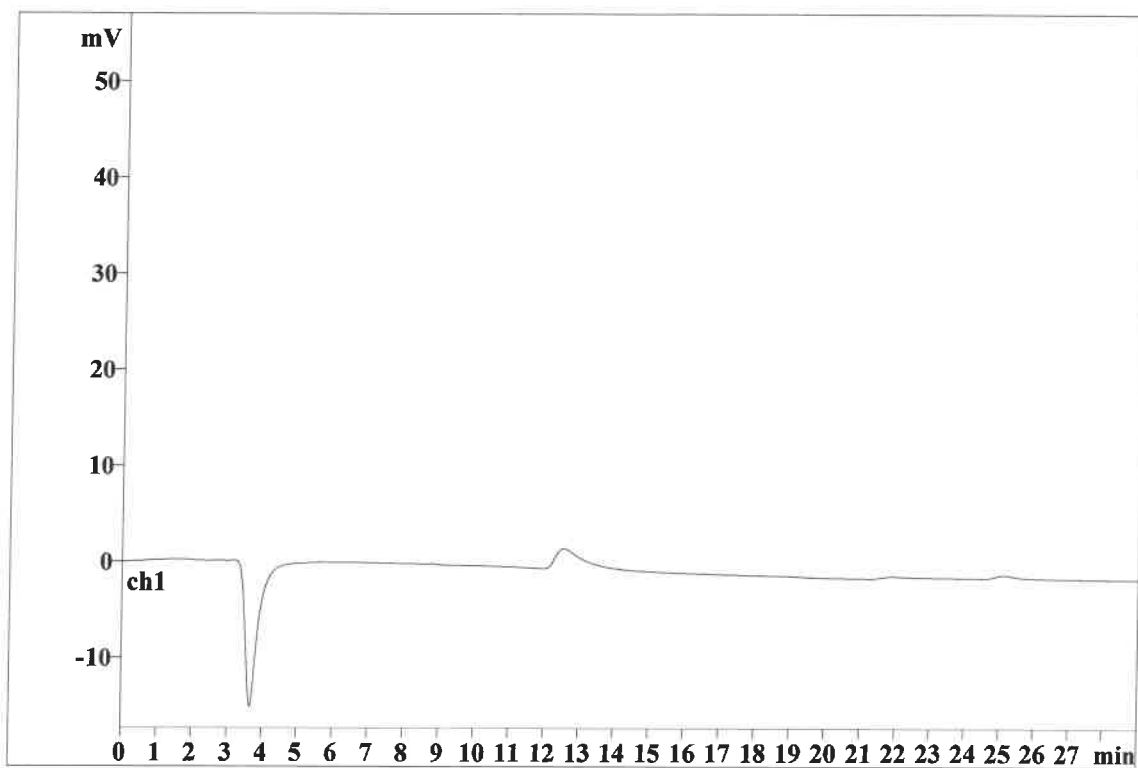

Quantitation method: Custom

No peaks

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:02:12 PM  
Printed by: wet


Ident: N5841-17  
Analysis from: 12/6/2022 6:28:59 PM  
File: \_2022-12-06\_

Last save: 12/6/2022 6:57:59 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32707

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 25  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

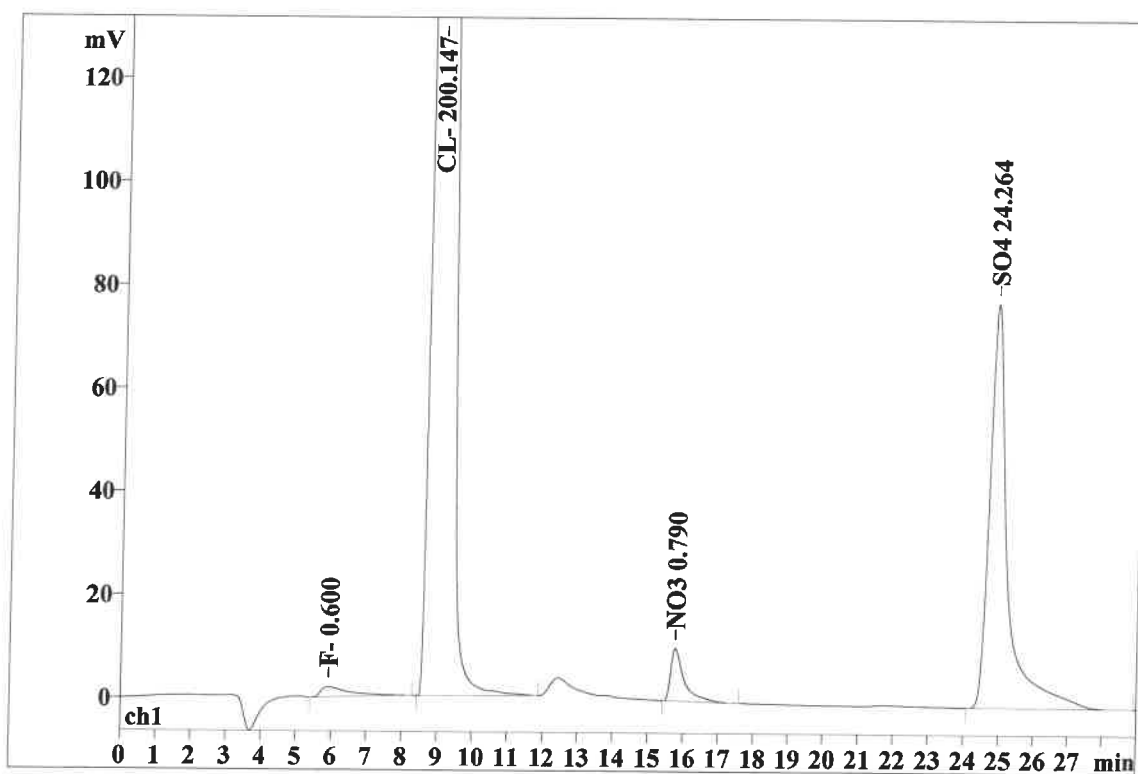

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.91             | 0.781          | 1.94         | 0.12        | 113.822        | 0.32      |
| 2  | 8.95             | 0.321          | 1475.93      | 94.23       | 32267.173      | 90.87     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 15.76            | 0.345          | 10.20        | 0.65        | 271.663        | 0.77      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 24.84            | 0.453          | 78.24        | 5.00        | 2856.730       | 8.04      |
| 7  | 29.00            | 0.271          | 1566.31      | 100.00      | 35509.387      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:02:20 PM  
Printed by: wet


Ident: N5841-19  
Analysis from: 12/6/2022 7:00:37 PM  
File: \_2022-12-06\_

Last save: 12/6/2022 7:29:37 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32708

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 26  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

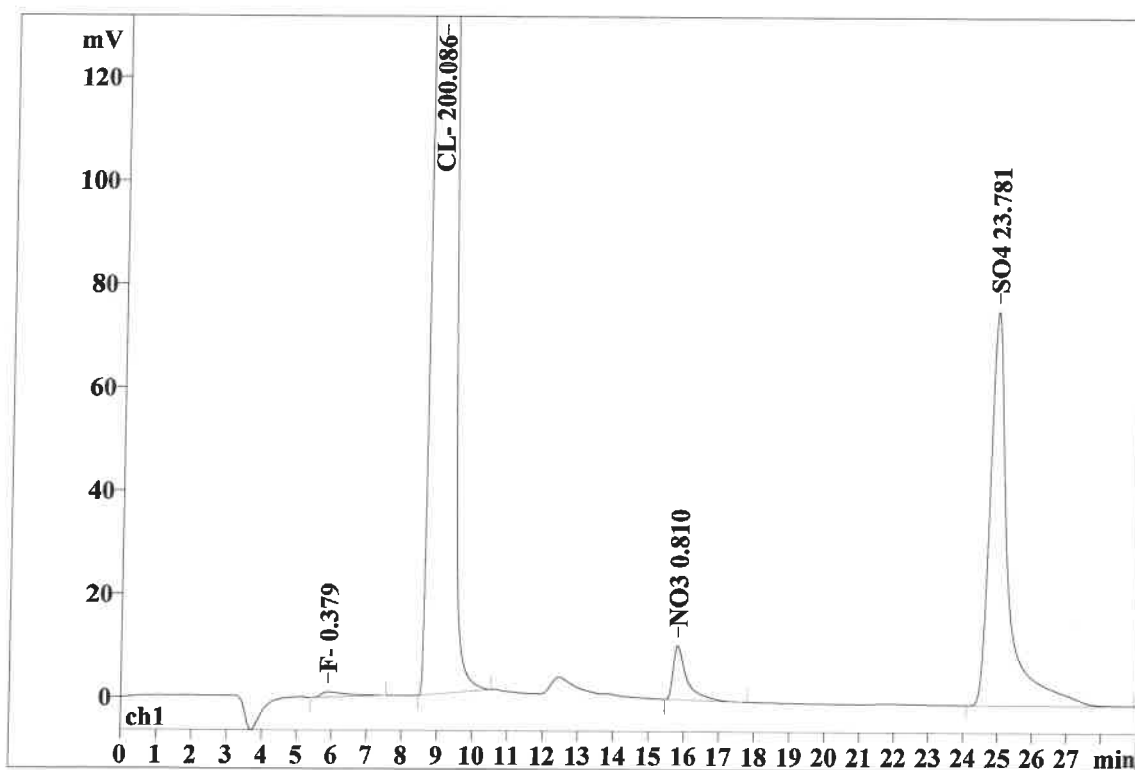

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.89             | 0.752          | 1.00         | 0.06        | 51.806         | 0.15      |
| 2  | 8.97             | 0.322          | 1475.54      | 94.39       | 32257.258      | 91.16     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 15.81            | 0.347          | 10.46        | 0.67        | 279.671        | 0.79      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 24.88            | 0.455          | 76.26        | 4.88        | 2798.311       | 7.91      |
| 7  | 29.00            | 0.268          | 1563.26      | 100.00      | 35387.046      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:02:39 PM  
Printed by: wet


Ident: N5861-01  
Analysis from: 12/6/2022 8:03:53 PM  
File: \_2022-12-06\_

Last save: 12/6/2022 8:32:53 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32710

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 27  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

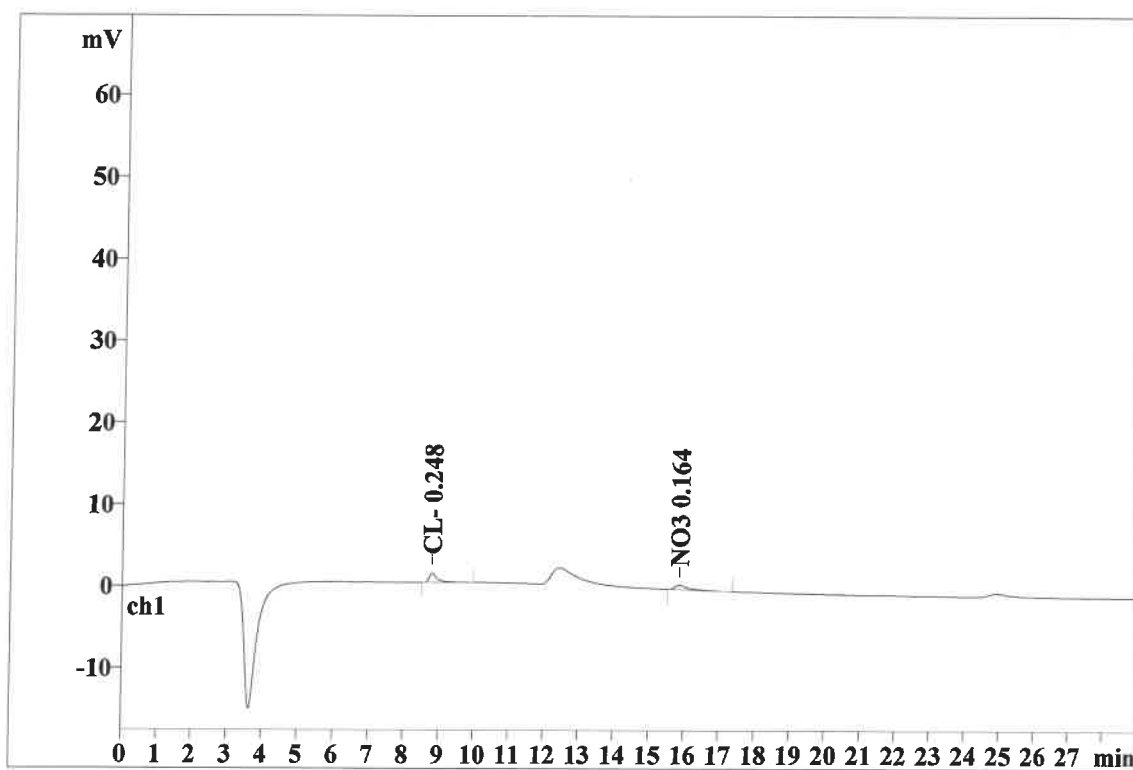

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 8.79             | 0.210          | 1.14         | 67.65       | 19.013         | 55.54     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 15.85            | 0.369          | 0.54         | 32.17       | 15.218         | 44.46     |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 29.00            | 0.083          | 1.67         | 99.82       | 34.231         | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:02:46 PM  
Printed by: wet


Ident: N5861-01MS  
Analysis from: 12/6/2022 8:35:31 PM  
File: \_2022-12-06\_

Last save: 12/6/2022 9:04:31 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32711

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 28  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

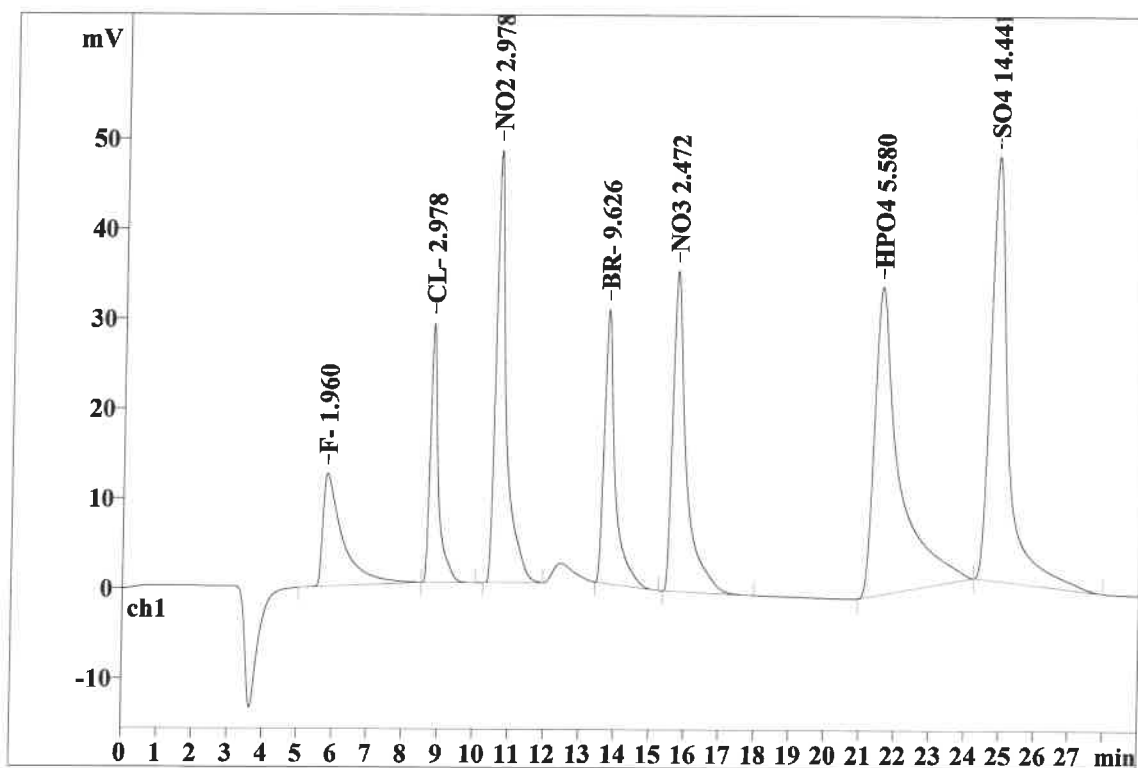

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.80             | 0.506          | 12.56        | 5.30        | 495.009        | 7.13      |
| 2  | 8.79             | 0.208          | 28.86        | 12.17       | 459.416        | 6.62      |
| 3  | 10.62            | 0.267          | 48.14        | 20.30       | 1000.571       | 14.42     |
| 4  | 13.73            | 0.282          | 30.48        | 12.85       | 657.430        | 9.48      |
| 5  | 15.69            | 0.349          | 35.65        | 15.03       | 961.019        | 13.85     |
| 6  | 21.53            | 0.579          | 34.26        | 14.45       | 1696.578       | 24.45     |
| 7  | 24.82            | 0.453          | 47.21        | 19.90       | 1668.441       | 24.05     |
| 7  | 29.00            | 0.378          | 237.16       | 100.00      | 6938.463       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:02:52 PM  
Printed by: wet


Ident: N5861-01MSD  
Analysis from: 12/6/2022 9:07:10 PM  
File: \_2022-12-06\_

Last save: 12/6/2022 9:36:10 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32712

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 29  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

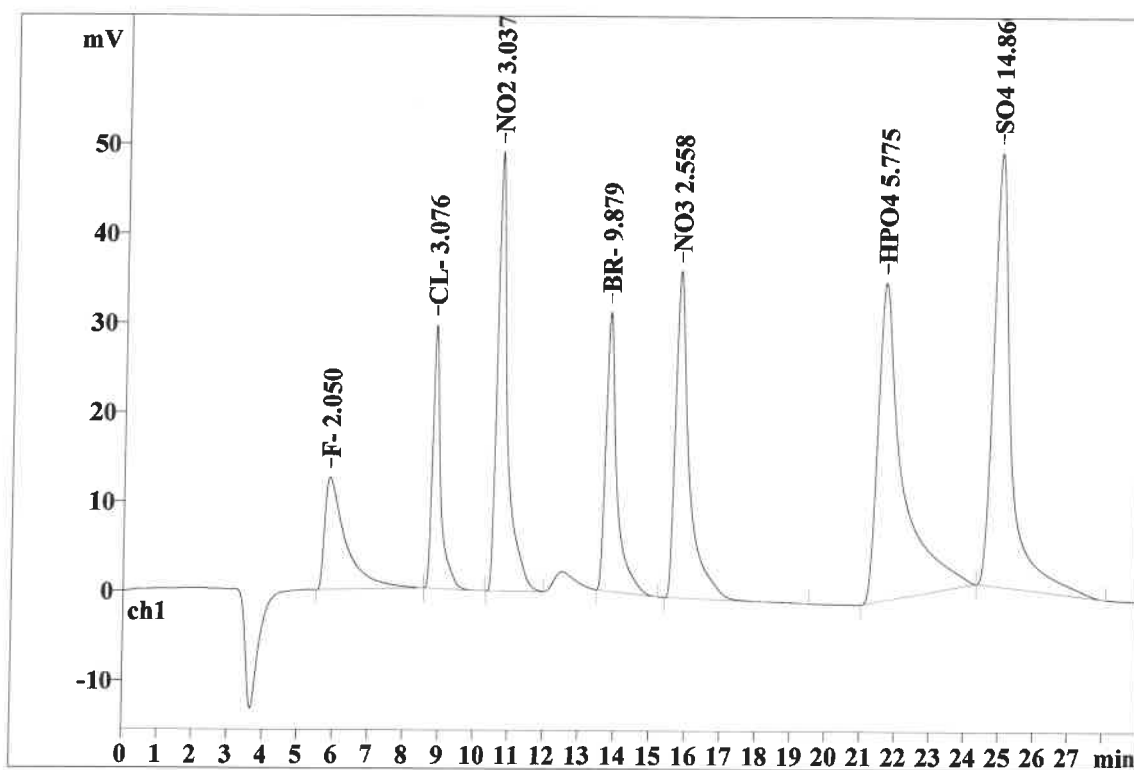

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.85             | 0.545          | 12.57        | 5.17        | 520.249        | 7.26      |
| 2  | 8.83             | 0.209          | 29.51        | 12.14       | 475.210        | 6.63      |
| 3  | 10.66            | 0.265          | 49.11        | 20.20       | 1021.887       | 14.26     |
| 4  | 13.79            | 0.283          | 31.22        | 12.84       | 675.756        | 9.43      |
| 5  | 15.75            | 0.351          | 36.58        | 15.05       | 995.999        | 13.89     |
| 6  | 21.61            | 0.578          | 35.61        | 14.65       | 1760.057       | 24.55     |
| 7  | 24.92            | 0.455          | 48.48        | 19.94       | 1719.218       | 23.98     |
| 7  | 29.00            | 0.384          | 243.08       | 100.00      | 7168.375       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:03:01 PM  
Printed by: wet


Ident: N5869-01  
Analysis from: 12/6/2022 9:38:47 PM  
File: \_2022-12-06\_

Last save: 12/6/2022 10:07:47 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32713

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 30  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

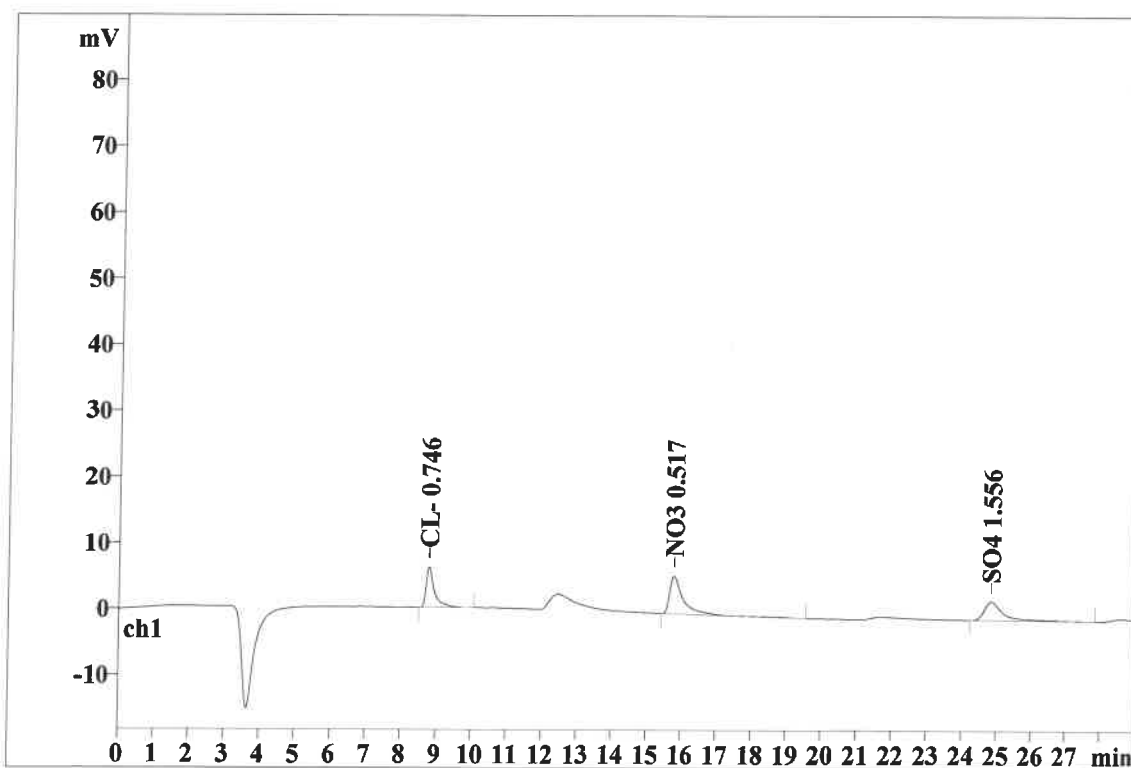

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 8.79             | 0.210          | 6.12         | 41.81       | 99.392         | 26.96     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 15.78            | 0.351          | 5.69         | 38.88       | 159.494        | 43.26     |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 24.84            | 0.487          | 2.82         | 19.30       | 109.812        | 29.78     |
| 7  | 29.00            | 0.150          | 14.63        | 99.99       | 368.698        | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:03:08 PM  
Printed by: wet


Ident: N5853-01  
Analysis from: 12/6/2022 10:10:25 PM  
File: \_2022-12-06\_

Last save: 12/6/2022 10:39:25 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32714

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 31  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

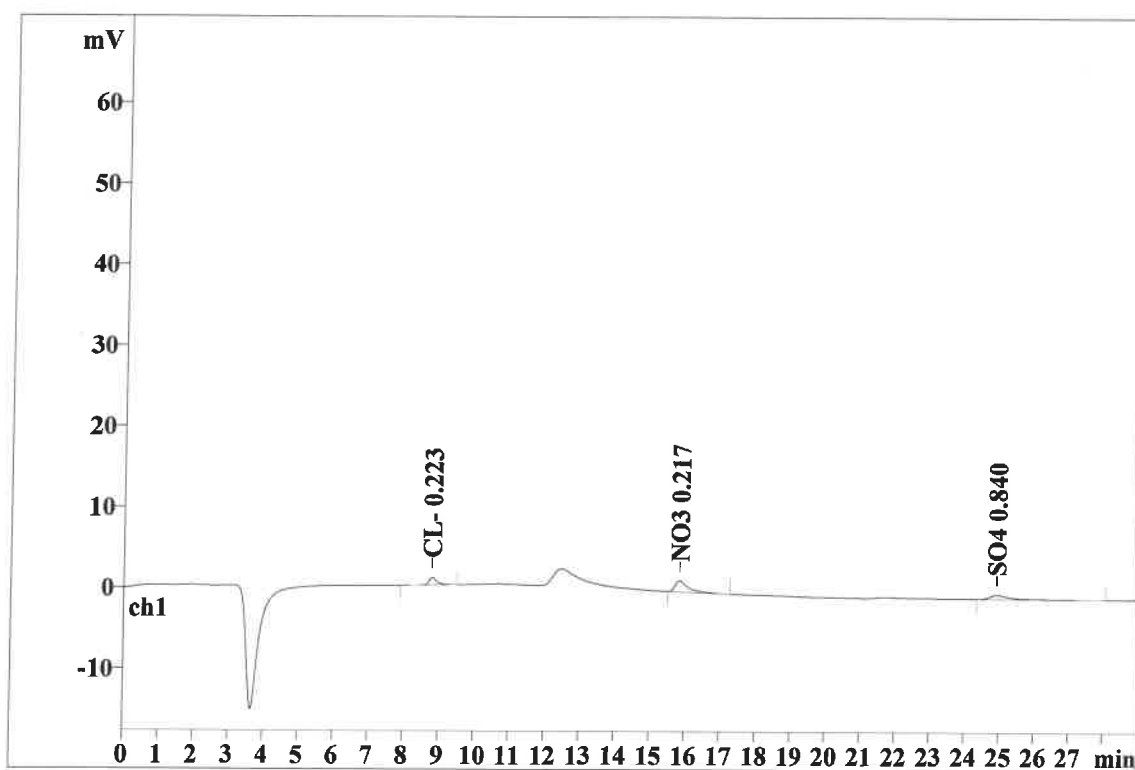

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 8.80             | 0.205          | 0.96         | 33.61       | 14.975         | 20.00     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 15.84            | 0.355          | 1.38         | 48.02       | 36.728         | 49.05     |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 24.91            | 0.556          | 0.52         | 18.24       | 23.180         | 30.96     |
| 7  | 29.00            | 0.159          | 2.86         | 99.87       | 74.884         | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:03:19 PM  
Printed by: wet


Ident: N5865-03  
Analysis from: 12/6/2022 10:42:02 PM  
File: \_2022-12-06\_

Last save: 12/7/2022 11:24:36 AM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32715

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 32  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

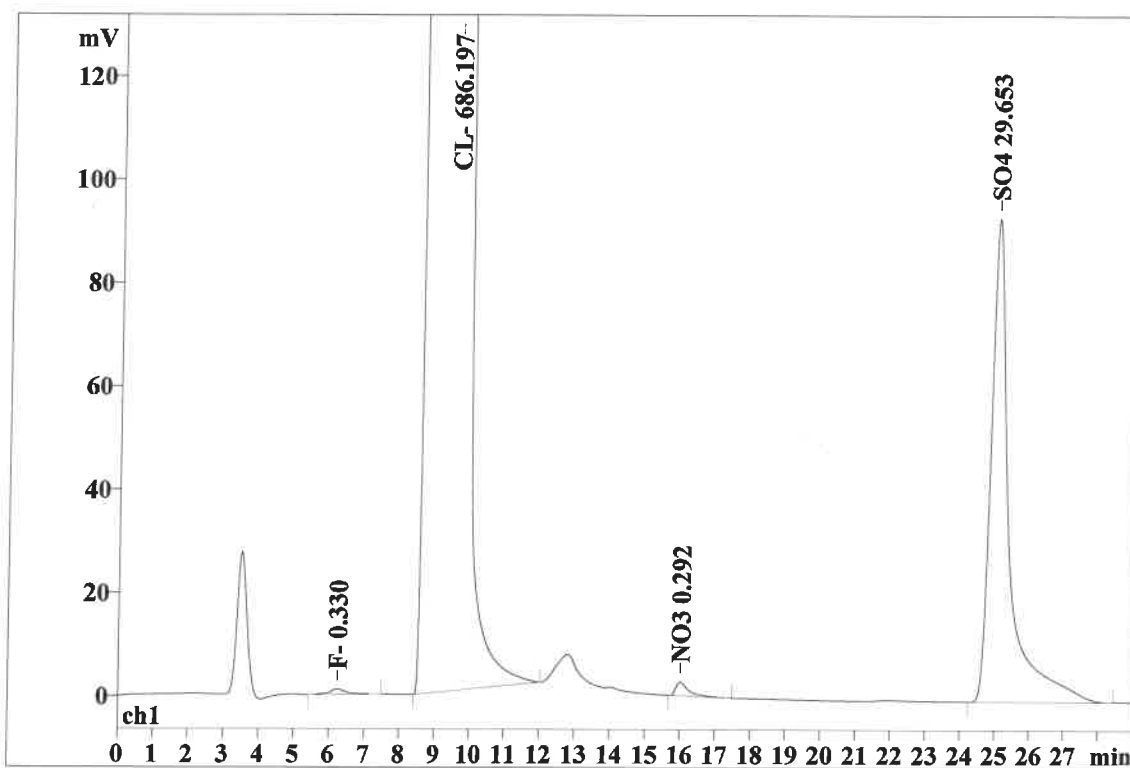

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 6.23             | 0.430          | 1.08         | 0.06        | 38.056         | 0.03      |
| 2  | 9.59             | 1.123          | 1684.41      | 94.54       | 110677.829     | 96.84     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 16.01            | 0.338          | 2.63         | 0.15        | 67.676         | 0.06      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 24.99            | 0.458          | 93.52        | 5.25        | 3508.620       | 3.07      |
| 7  | 29.00            | 0.335          | 1781.63      | 100.00      | 114292.180     | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:03:25 PM  
Printed by: wet


Ident: N5865-05  
Analysis from: 12/6/2022 11:13:40 PM  
File: \_2022-12-06\_

Last save: 12/6/2022 11:42:40 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32716

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 33  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

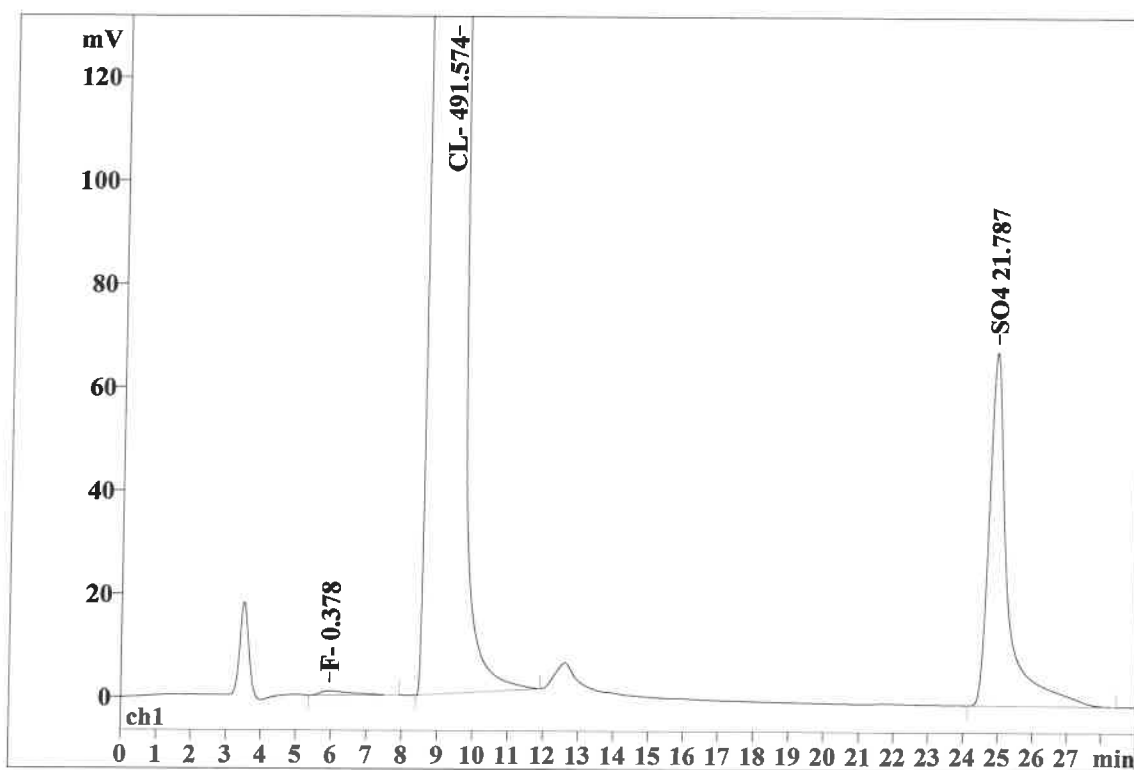

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.95             | 0.960          | 0.80         | 0.05        | 51.483         | 0.06      |
| 2  | 9.29             | 0.802          | 1650.67      | 95.98       | 79280.880      | 96.81     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 24.86            | 0.457          | 68.39        | 3.98        | 2557.112       | 3.12      |
| 7  | 29.00            | 0.317          | 1719.86      | 100.00      | 81889.475      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:03:32 PM  
Printed by: wet


Ident: N5865-07  
Analysis from: 12/6/2022 11:45:18 PM  
File: \_2022-12-06\_

Last save: 12/7/2022 12:14:18 AM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32717

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 34  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

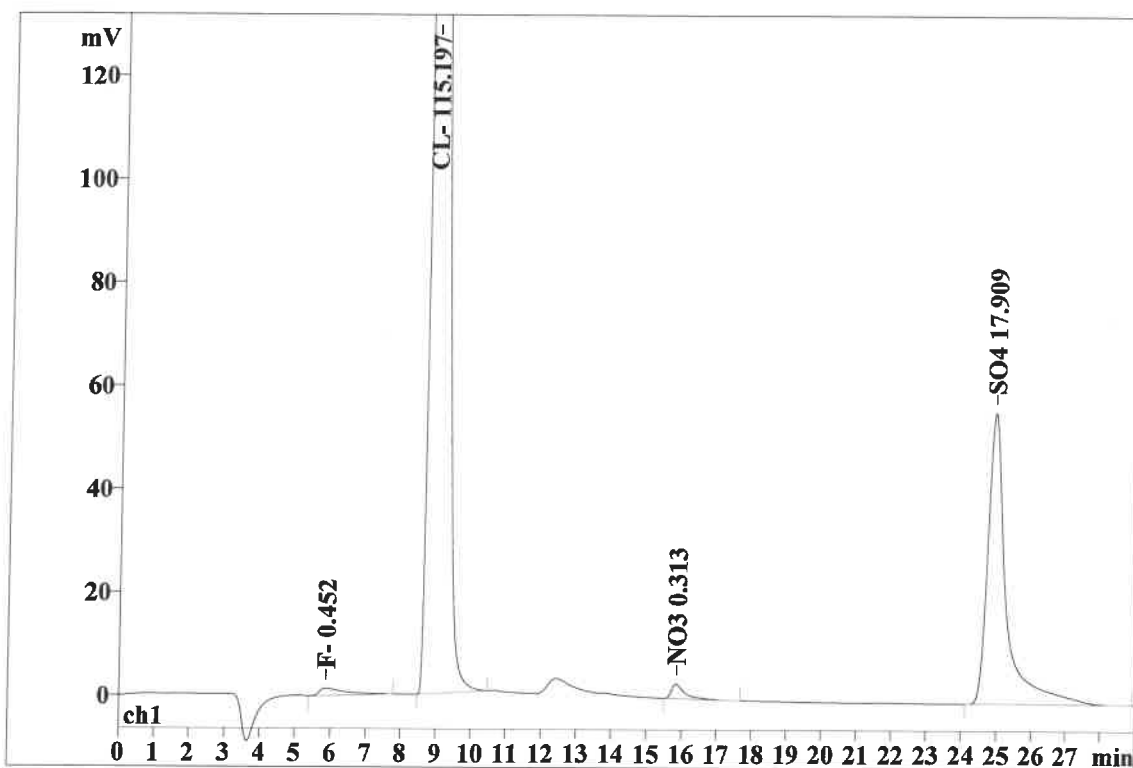

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.87             | 0.722          | 1.41         | 0.11        | 72.327         | 0.35      |
| 2  | 8.87             | 0.206          | 1207.69      | 95.23       | 18562.894      | 89.25     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 15.84            | 0.349          | 2.85         | 0.22        | 76.025         | 0.37      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 24.88            | 0.458          | 56.38        | 4.45        | 2088.035       | 10.04     |
| 7  | 29.00            | 0.248          | 1268.33      | 100.01      | 20799.281      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:03:40 PM  
Printed by: wet


Ident: CCV  
Analysis from: 12/7/2022 12:17:04 AM  
File: \_2022-12-07\_

Last save: 12/7/2022 12:46:04 AM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32718

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 11  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

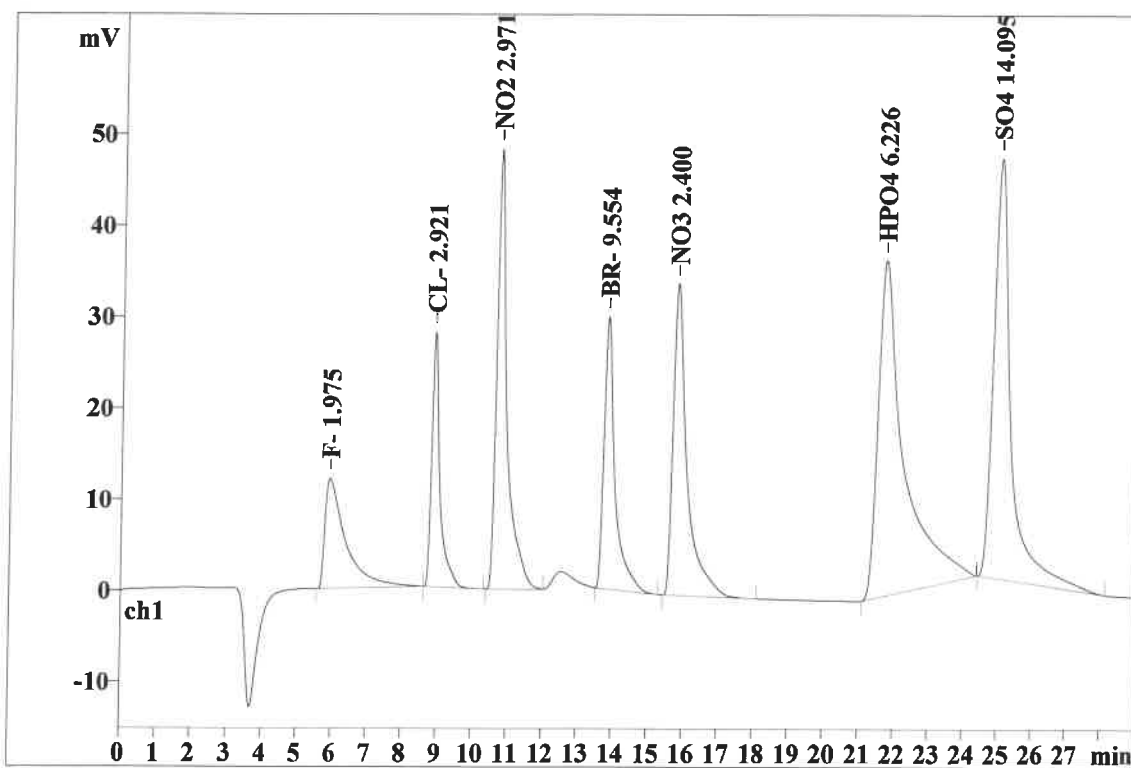

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.92             | 0.547          | 12.06        | 5.13        | 499.400        | 7.07      |
| 2  | 8.89             | 0.209          | 27.90        | 11.87       | 450.305        | 6.37      |
| 3  | 10.72            | 0.264          | 48.20        | 20.50       | 997.849        | 14.12     |
| 4  | 13.82            | 0.285          | 29.85        | 12.70       | 652.236        | 9.23      |
| 5  | 15.79            | 0.352          | 34.20        | 14.55       | 931.596        | 13.19     |
| 6  | 21.69            | 0.609          | 36.84        | 15.67       | 1907.416       | 27.00     |
| 7  | 24.99            | 0.456          | 46.07        | 19.59       | 1626.612       | 23.02     |
| 7  | 29.00            | 0.389          | 235.12       | 100.00      | 7065.415       | 100.00    |

Report date: 12/7/2022 3:03:46 PM  
Printed by: wet


Ident: CCB  
Analysis from: 12/7/2022 12:48:42 AM  
File: \_2022-12-07\_

Last save: 12/7/2022 1:17:42 AM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32719

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 12  
Volume: 20.0  $\mu$ L  
Dilution: 1.00  
Amount: 1.0000

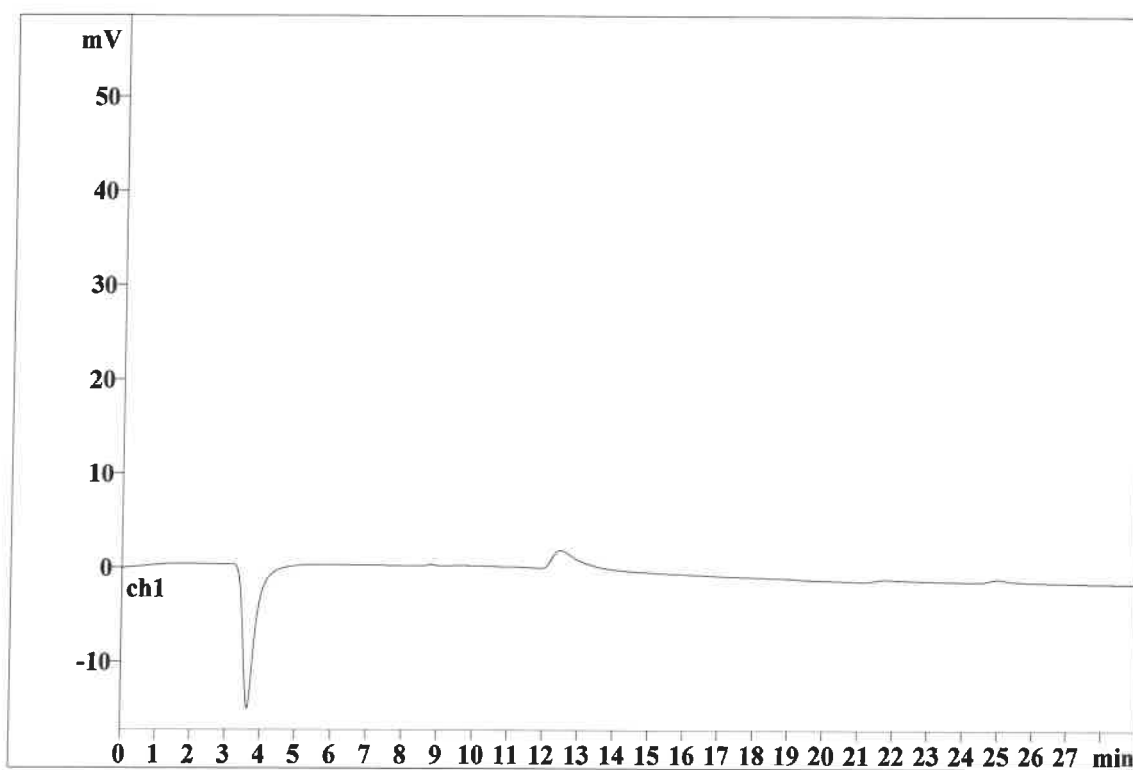

Quantitation method: Custom

No peaks

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:03:55 PM  
Printed by: wet


Ident: N5865-09  
Analysis from: 12/7/2022 1:20:28 AM  
File: \_2022-12-07\_

Last save: 12/7/2022 1:49:28 AM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32720

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 35  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

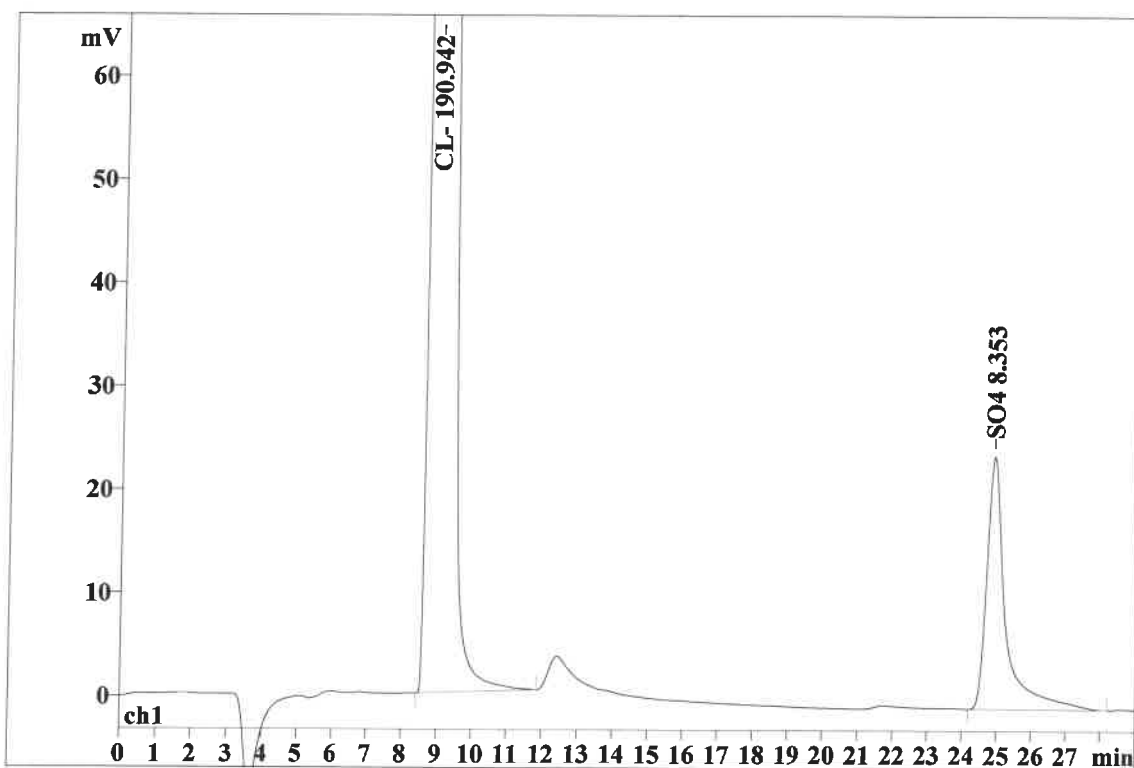

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 8.95             | 0.306          | 1461.83      | 98.35       | 30782.180      | 97.06     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 24.87            | 0.468          | 24.43        | 1.64        | 932.029        | 2.94      |
| 7  | 29.00            | 0.111          | 1486.26      | 100.00      | 31714.209      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:04:01 PM  
Printed by: wet


Ident: N5865-11  
Analysis from: 12/7/2022 1:52:05 AM  
File: \_2022-12-07\_

Last save: 12/7/2022 2:21:05 AM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32721

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 36  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

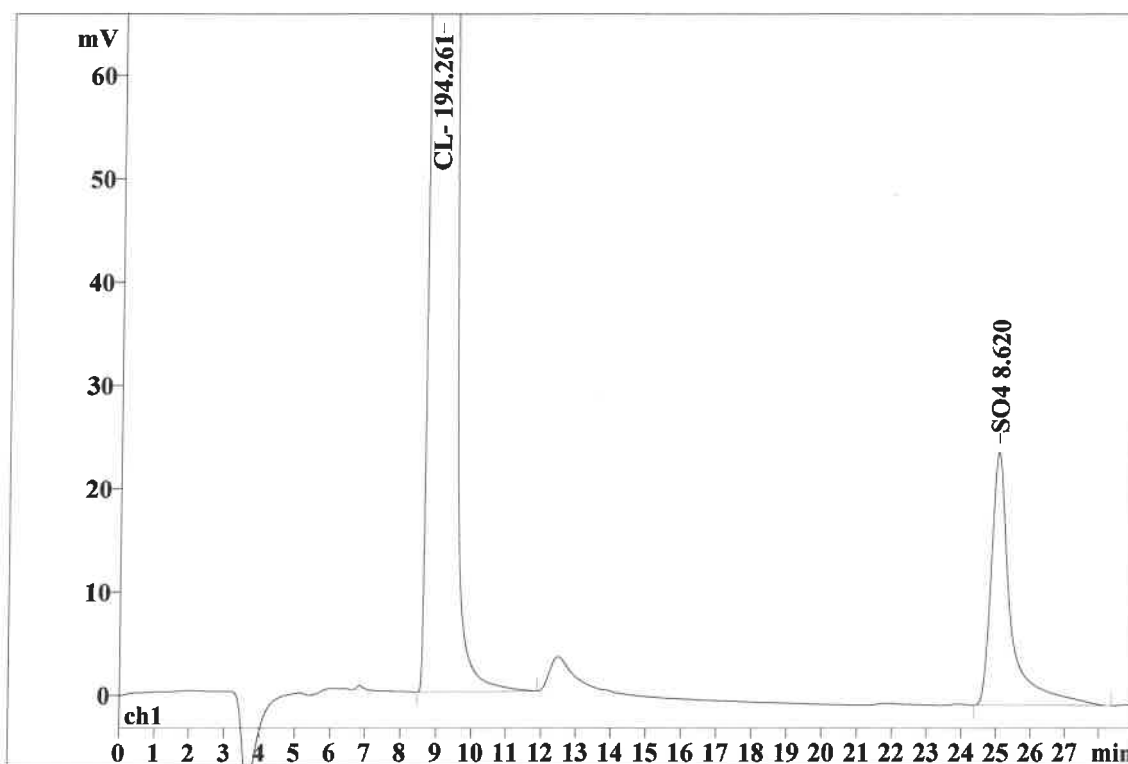

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 8.99             | 0.311          | 1463.90      | 98.35       | 31317.663      | 97.01     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 25.03            | 0.483          | 24.56        | 1.65        | 964.337        | 2.99      |
| 7  | 29.00            | 0.113          | 1488.46      | 100.00      | 32281.999      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:04:09 PM  
Printed by: wet


Ident: N5865-13  
Analysis from: 12/7/2022 2:23:43 AM  
File: \_2022-12-07\_

Last save: 12/7/2022 2:52:43 AM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32722

Last save: 12/1/2022 4:34:

SAMPLE:  
:  
Vial number: 37  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

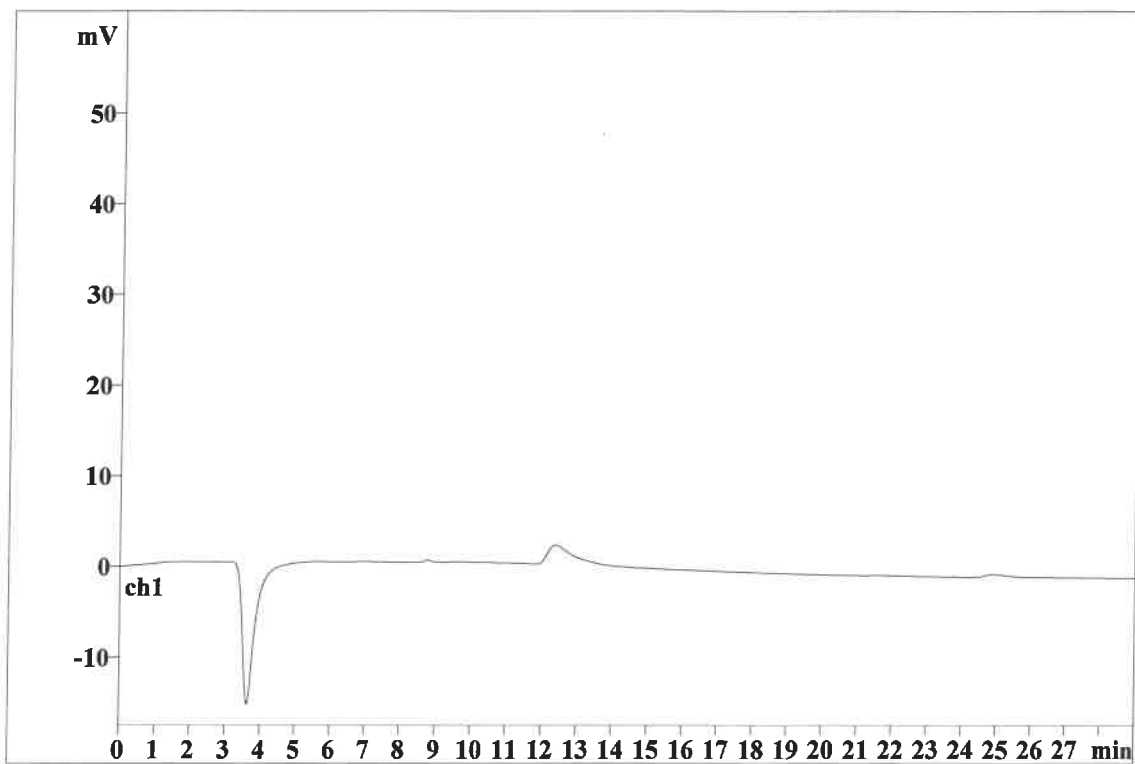

Quantitation method: Custom

No peaks

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:04:20 PM  
Printed by: wet


Ident: N5865-11MS  
Analysis from: 12/7/2022 2:55:21 AM  
File: \_2022-12-07\_

Last save: 12/7/2022 11:27:46 AM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32723

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 38  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

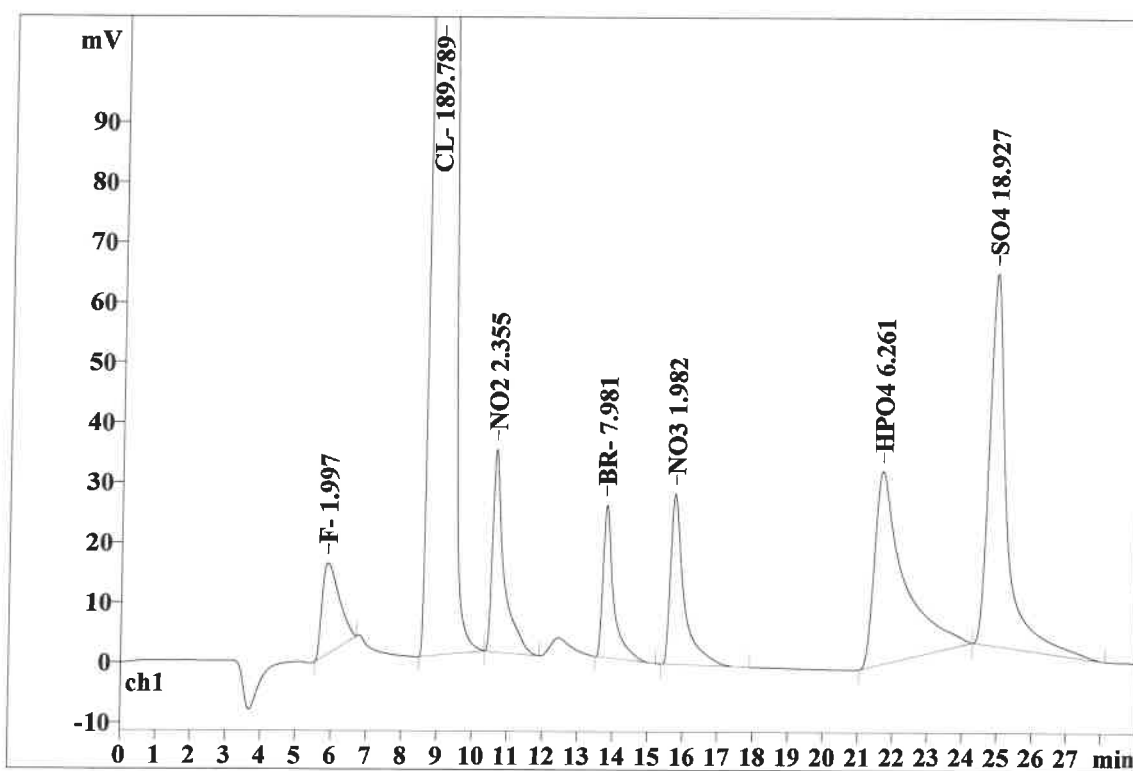

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.86             | 0.531          | 15.26        | 0.92        | 505.523        | 1.36      |
| 2  | 8.95             | 0.304          | 1458.20      | 88.09       | 30596.180      | 82.02     |
| 3  | 10.63            | 0.282          | 33.74        | 2.04        | 774.219        | 2.08      |
| 4  | 13.78            | 0.273          | 25.42        | 1.54        | 538.603        | 1.44      |
| 5  | 15.72            | 0.342          | 28.38        | 1.71        | 760.202        | 2.04      |
| 6  | 21.64            | 0.732          | 32.24        | 1.95        | 1919.105       | 5.14      |
| 7  | 24.88            | 0.456          | 62.02        | 3.75        | 2211.175       | 5.93      |
| 7  | 29.00            | 0.417          | 1655.27      | 100.00      | 37305.008      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:04:27 PM  
Printed by: wet


Ident: N5865-11MSD  
Analysis from: 12/7/2022 3:26:59 AM  
File: \_2022-12-07\_

Last save: 12/7/2022 11:27:59 AM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32724

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 39  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

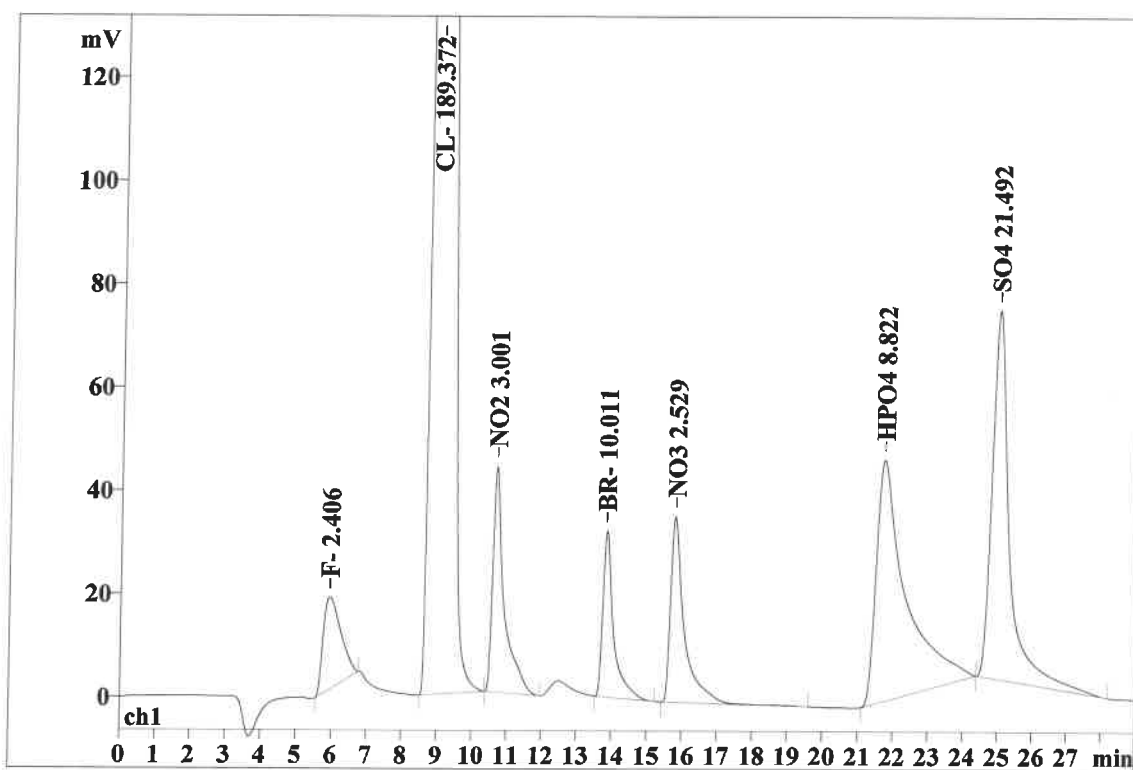

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.91             | 0.557          | 17.96        | 1.06        | 620.137        | 1.59      |
| 2  | 8.98             | 0.304          | 1452.03      | 85.40       | 30528.843      | 78.07     |
| 3  | 10.66            | 0.281          | 43.70        | 2.57        | 1008.812       | 2.58      |
| 4  | 13.83            | 0.273          | 32.21        | 1.89        | 685.296        | 1.75      |
| 5  | 15.77            | 0.344          | 36.02        | 2.12        | 984.099        | 2.52      |
| 6  | 21.69            | 0.717          | 46.84        | 2.75        | 2755.938       | 7.05      |
| 7  | 24.96            | 0.455          | 71.44        | 4.20        | 2521.436       | 6.45      |
| 7  | 29.00            | 0.419          | 1700.20      | 100.00      | 39104.559      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:04:34 PM  
Printed by: wet


Ident: N5841-05DLX2  
Analysis from: 12/7/2022 3:58:37 AM  
File: \_2022-12-07\_

Last save: 12/7/2022 4:27:37 AM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32725

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 40  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

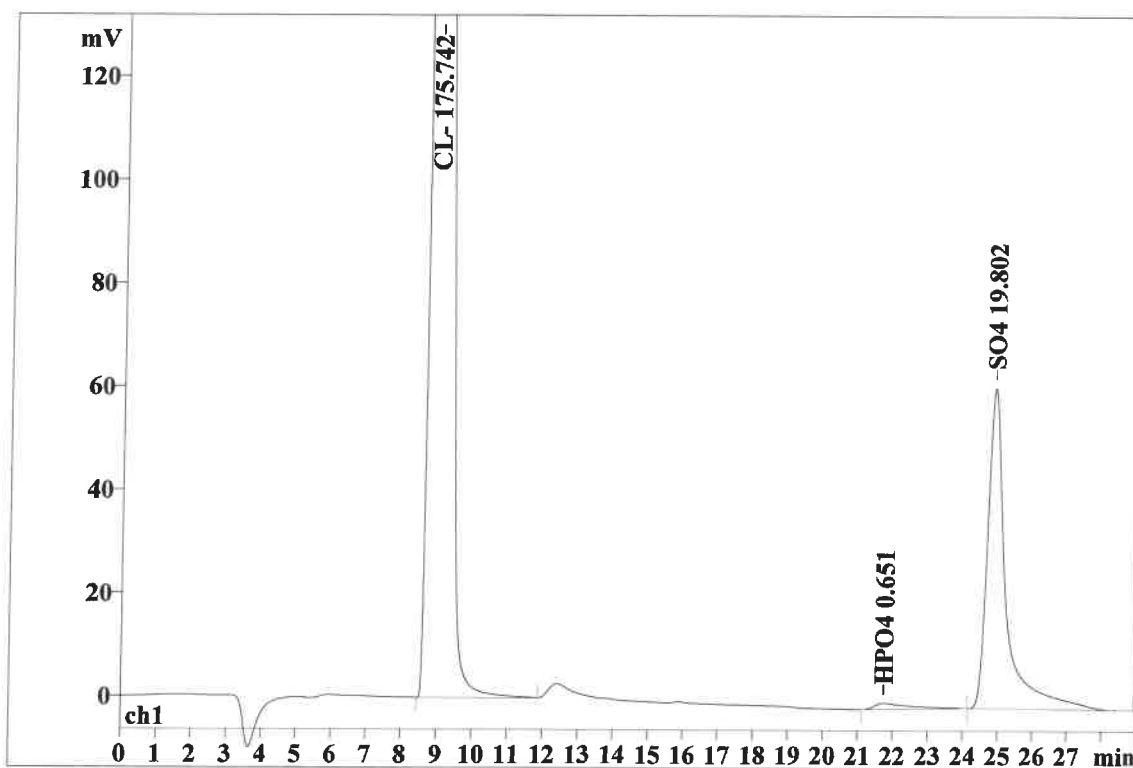

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 8.93             | 0.283          | 1430.42      | 95.76       | 28330.110      | 92.18     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 6  | 21.73            | 1.036          | 1.18         | 0.08        | 85.815         | 0.28      |
| 7  | 24.84            | 0.459          | 62.01        | 4.15        | 2317.046       | 7.54      |
| 7  | 29.00            | 0.254          | 1493.61      | 100.00      | 30732.970      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:04:42 PM  
Printed by: wet


Ident: CCV  
Analysis from: 12/7/2022 4:30:24 AM  
File: \_2022-12-07\_

Last save: 12/7/2022 4:59:24 AM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32726

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 14  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

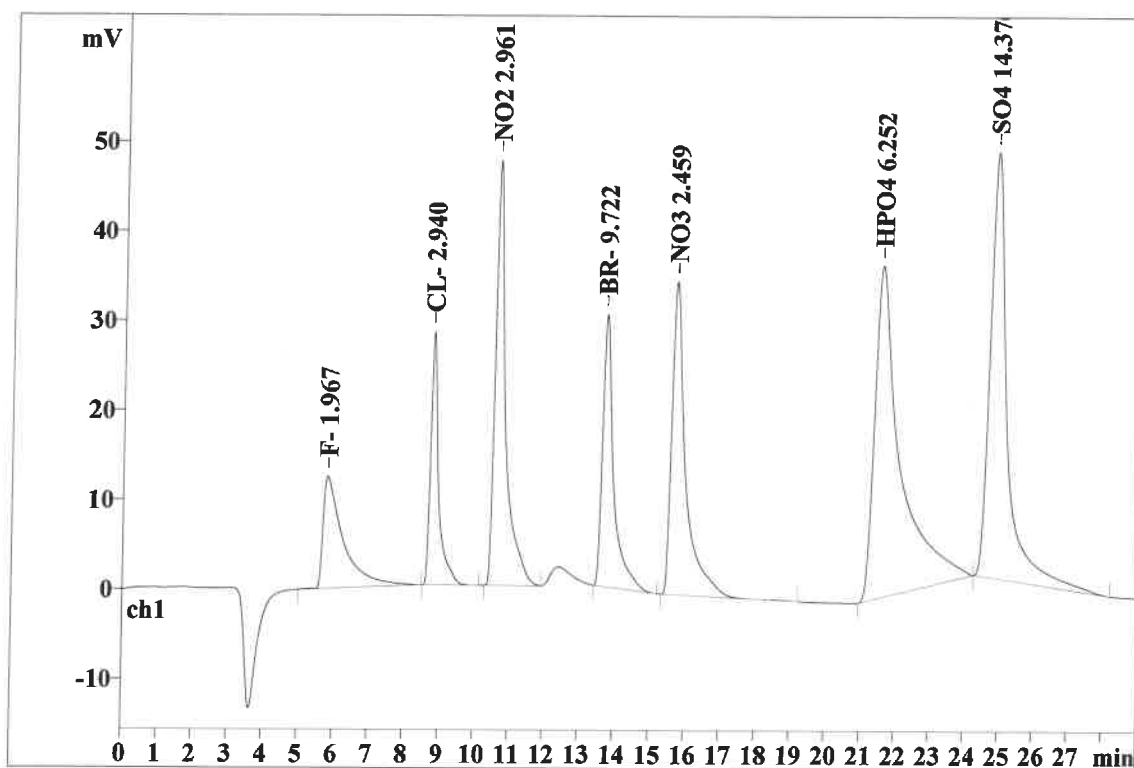

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.81             | 0.516          | 12.51        | 5.25        | 497.023        | 6.96      |
| 2  | 8.79             | 0.207          | 28.29        | 11.87       | 453.284        | 6.35      |
| 3  | 10.62            | 0.265          | 47.50        | 19.93       | 994.525        | 13.93     |
| 4  | 13.72            | 0.282          | 30.44        | 12.77       | 664.410        | 9.30      |
| 5  | 15.68            | 0.349          | 34.99        | 14.68       | 955.527        | 13.38     |
| 6  | 21.54            | 0.612          | 37.12        | 15.57       | 1916.162       | 26.83     |
| 7  | 24.85            | 0.453          | 47.54        | 19.94       | 1660.617       | 23.25     |
| 7  | 29.00            | 0.383          | 238.38       | 100.00      | 7141.548       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:04:49 PM  
Printed by: wet


Ident: CCB  
Analysis from: 12/7/2022 5:02:03 AM  
File: \_2022-12-07\_

Last save: 12/7/2022 5:31:03 AM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32727

Last save: 12/1/2022 4:34:

SAMPLE:  
:  
Vial number: 13  
Volume: 20.0  $\mu$ L  
Dilution: 1.00  
Amount: 1.0000

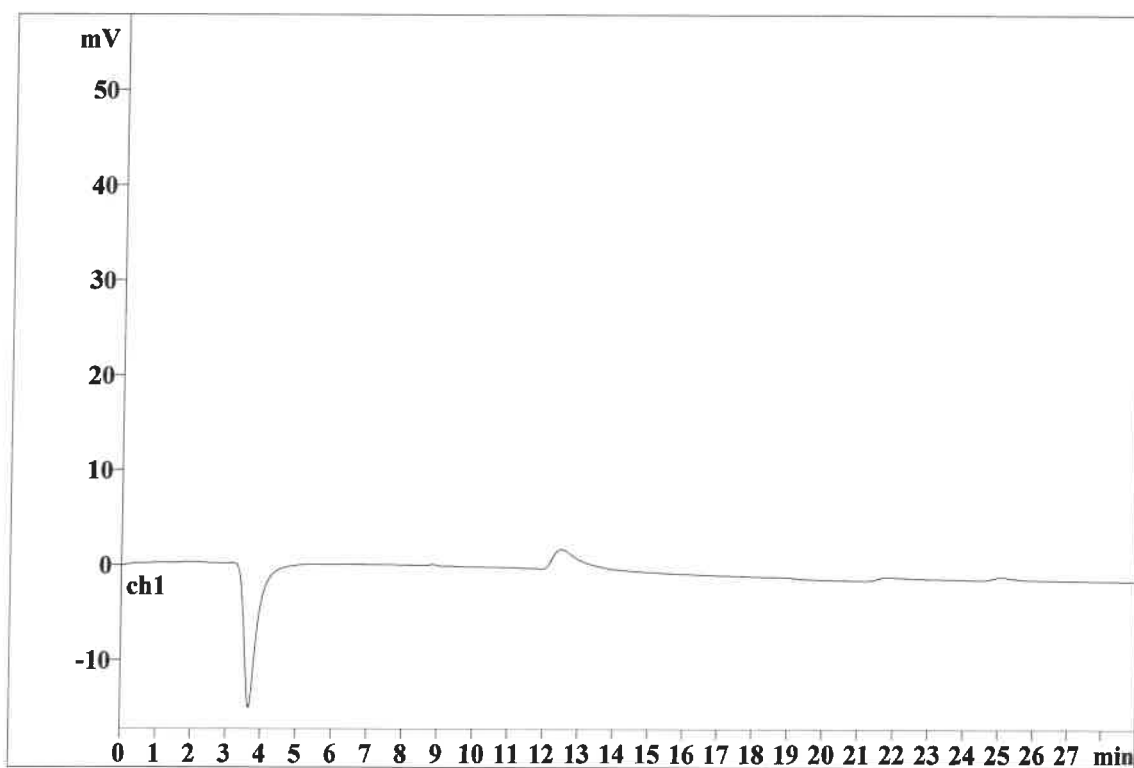

Quantitation method: Custom

No peaks

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:04:57 PM  
Printed by: wet


Ident: CCV  
Analysis from: 12/7/2022 9:54:16 AM  
File: \_2022-12-07\_

Last save: 12/7/2022 10:23:16 AM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32730

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 11  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

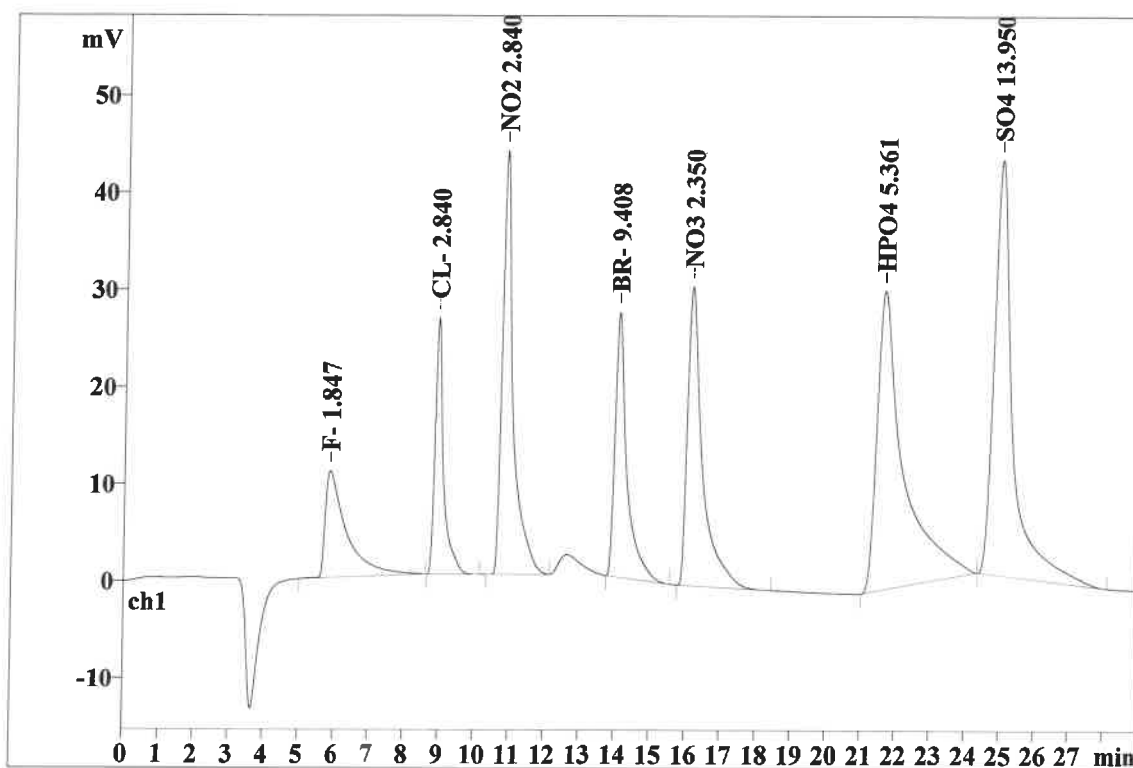

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.85             | 0.546          | 11.00        | 5.17        | 463.304        | 6.98      |
| 2  | 8.92             | 0.215          | 26.38        | 12.40       | 437.117        | 6.59      |
| 3  | 10.82            | 0.277          | 43.63        | 20.51       | 950.568        | 14.32     |
| 4  | 14.06            | 0.306          | 27.30        | 12.83       | 641.683        | 9.67      |
| 5  | 16.12            | 0.383          | 30.83        | 14.49       | 910.945        | 13.72     |
| 6  | 21.62            | 0.620          | 30.79        | 14.48       | 1624.990       | 24.48     |
| 7  | 24.94            | 0.473          | 42.76        | 20.11       | 1609.033       | 24.24     |
| 7  | 29.00            | 0.403          | 212.69       | 100.00      | 6637.640       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:05:05 PM  
Printed by: wet


Ident: CCB  
Analysis from: 12/7/2022 10:26:20 AM  
File: \_2022-12-07\_

Last save: 12/7/2022 10:55:20 AM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32731

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 12  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

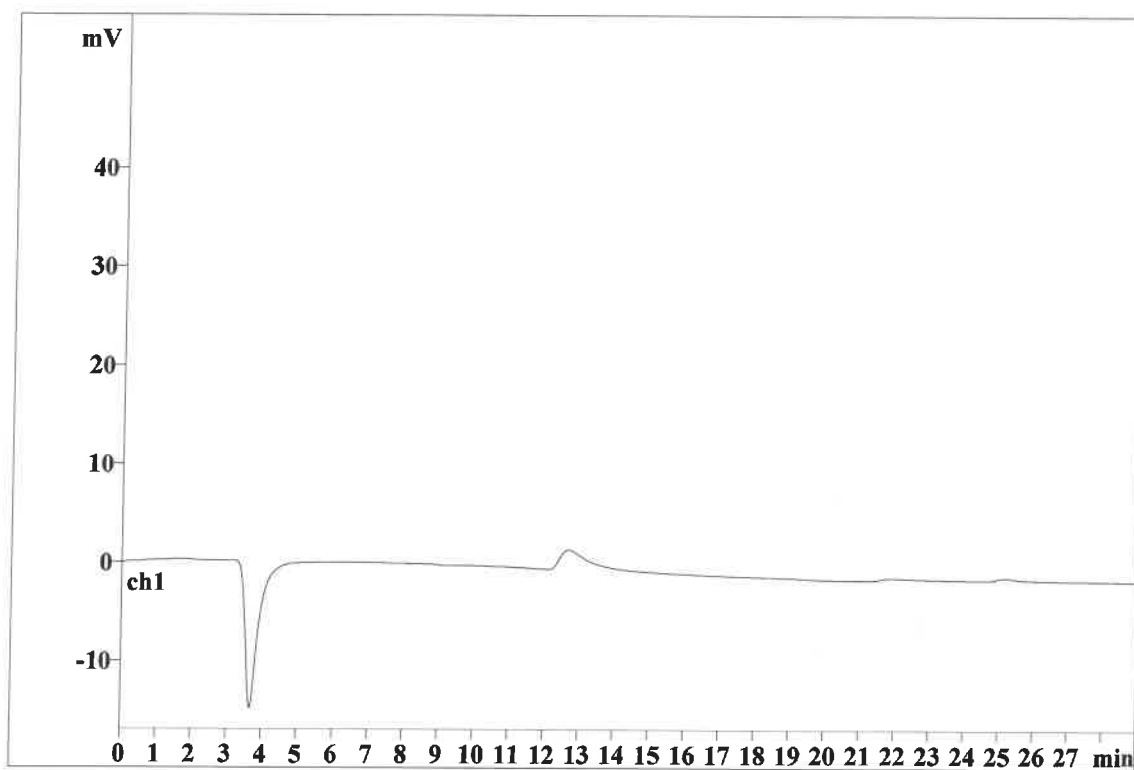

Quantitation method: Custom

No peaks

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:05:11 PM  
Printed by: wet


Ident: LB123150BLW2  
Analysis from: 12/7/2022 10:57:58 AM  
File: \_2022-12-07\_

Last save: 12/7/2022 2:58:30 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32732

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 13  
Volume: 20.0  $\mu$ L  
Dilution: 1.00  
Amount: 1.0000

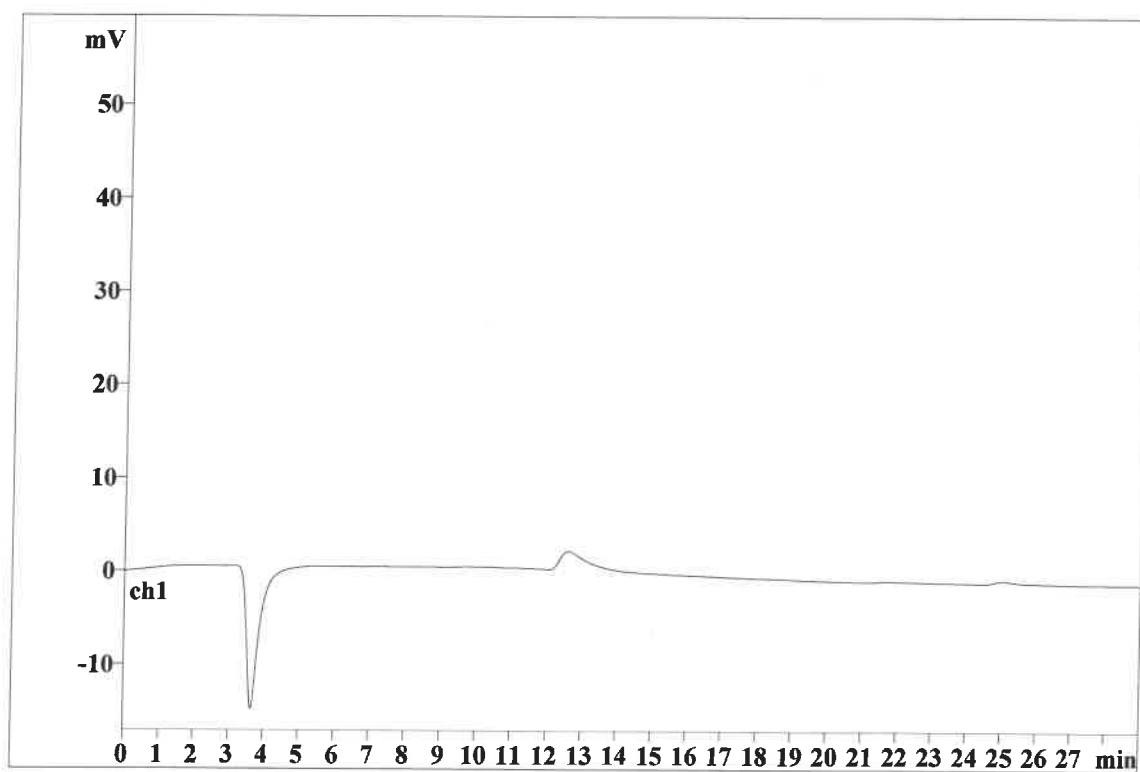

Quantitation method: Custom

No peaks

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:05:17 PM  
Printed by: wet


Ident: LB123150BSW2  
Analysis from: 12/7/2022 11:29:36 AM  
File: \_2022-12-07\_

Last save: 12/7/2022 2:58:30 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32733

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 14  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

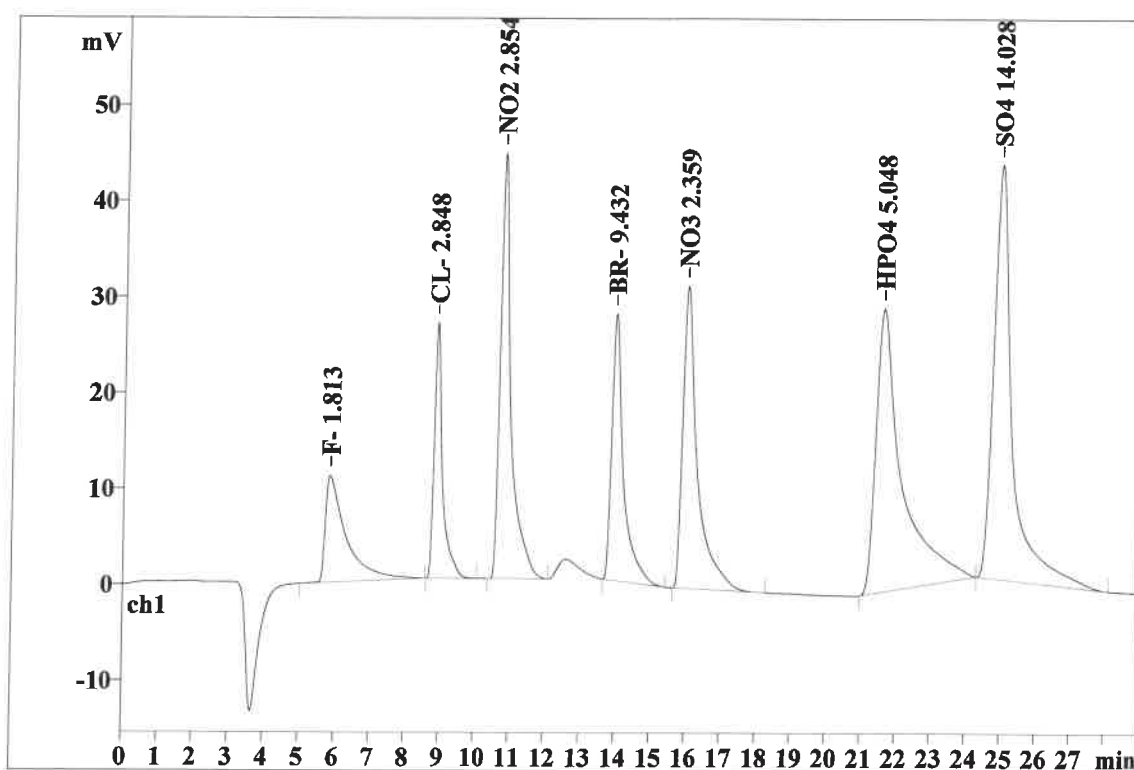

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.84             | 0.527          | 11.12        | 5.19        | 453.984        | 6.93      |
| 2  | 8.88             | 0.213          | 26.68        | 12.45       | 438.390        | 6.70      |
| 3  | 10.75            | 0.273          | 44.38        | 20.70       | 955.411        | 14.59     |
| 4  | 13.95            | 0.300          | 27.86        | 13.00       | 643.425        | 9.83      |
| 5  | 15.98            | 0.375          | 31.53        | 14.71       | 914.742        | 13.97     |
| 6  | 21.58            | 0.603          | 29.57        | 13.80       | 1522.675       | 23.26     |
| 7  | 24.91            | 0.470          | 43.21        | 20.16       | 1618.586       | 24.72     |
| 7  | 29.00            | 0.394          | 214.35       | 100.00      | 6547.213       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:05:30 PM  
Printed by: wet


Ident: N5841-13DLX2  
Analysis from: 12/7/2022 12:53:16 PM  
File: \_2022-12-07\_

Last save: 12/7/2022 1:22:16 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32735

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 15  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

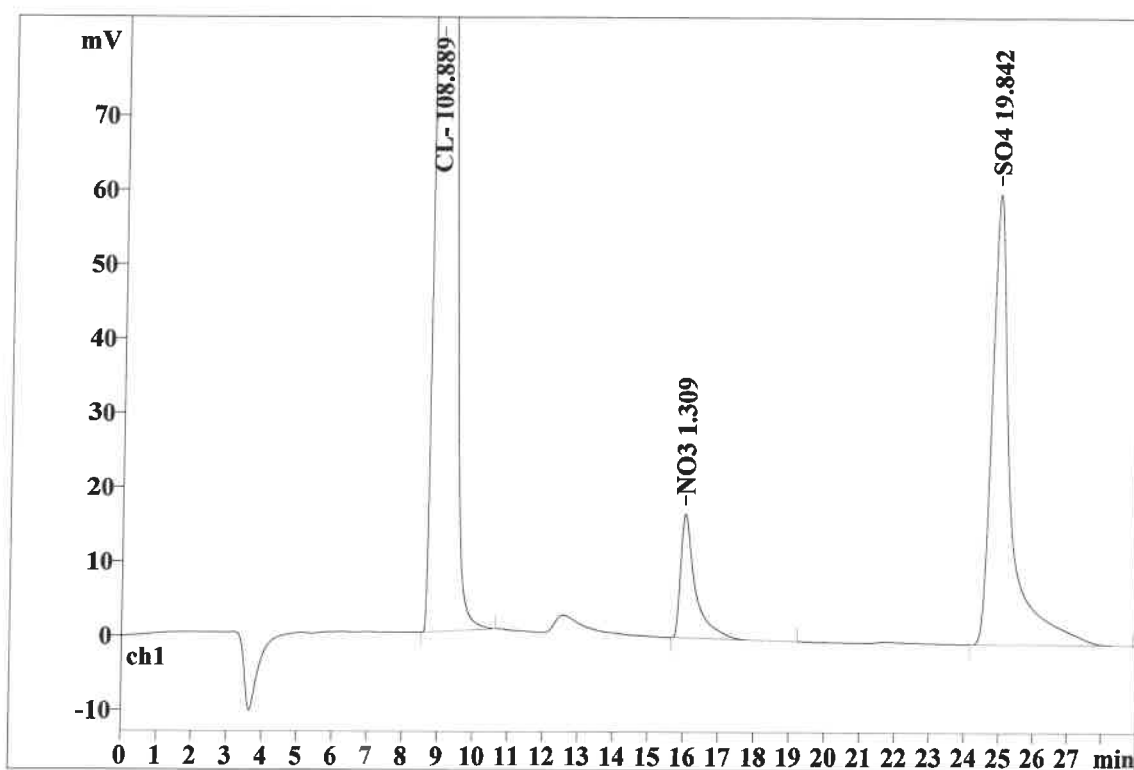

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 8.94             | 0.199          | 1174.80      | 93.84       | 17545.259      | 86.21     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 16.01            | 0.372          | 16.72        | 1.34        | 484.325        | 2.38      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 24.89            | 0.469          | 60.57        | 4.84        | 2321.787       | 11.41     |
| 7  | 29.00            | 0.149          | 1252.08      | 100.01      | 20351.371      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:05:37 PM  
Printed by: wet


Ident: CCV  
Analysis from: 12/7/2022 1:26:21 PM  
File: \_2022-12-07\_

Last save: 12/7/2022 1:55:21 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32736

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 11  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

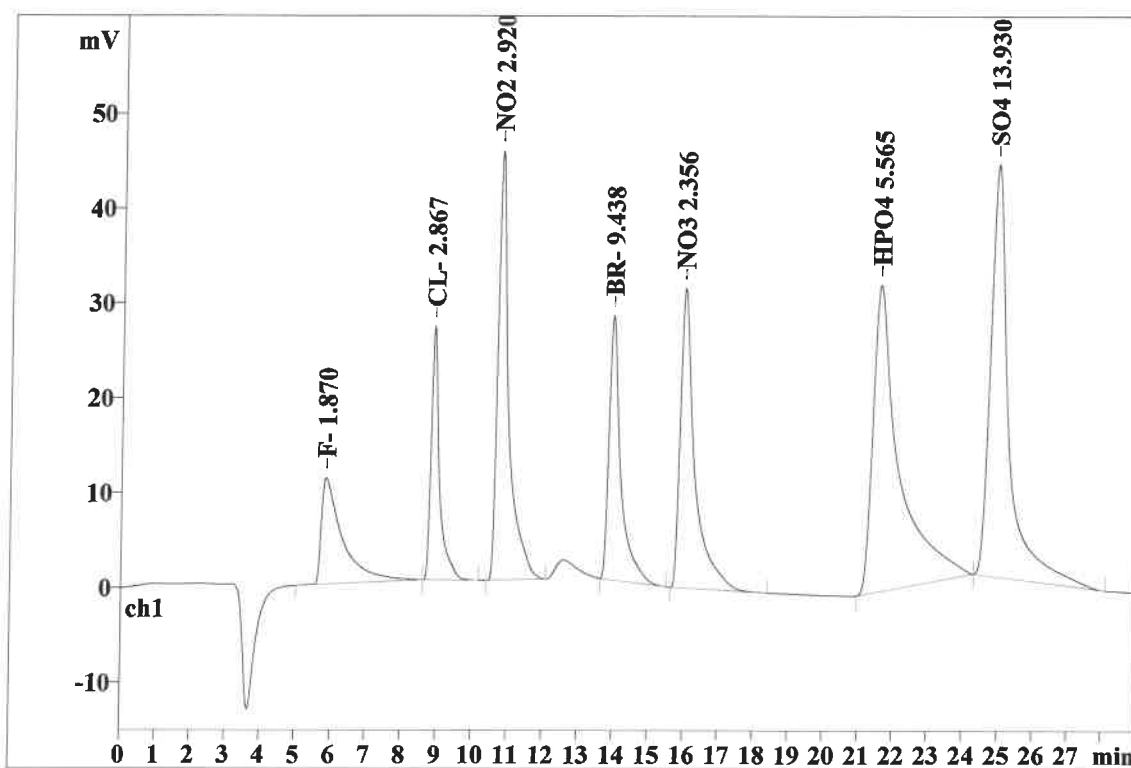

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 5.84             | 0.537          | 11.22        | 5.14        | 469.959        | 6.97      |
| 2  | 8.88             | 0.214          | 26.73        | 12.23       | 441.586        | 6.55      |
| 3  | 10.75            | 0.275          | 45.25        | 20.71       | 979.427        | 14.52     |
| 4  | 13.94            | 0.300          | 27.87        | 12.76       | 643.863        | 9.54      |
| 5  | 15.97            | 0.373          | 31.59        | 14.46       | 913.343        | 13.54     |
| 6  | 21.57            | 0.614          | 32.35        | 14.81       | 1691.599       | 25.07     |
| 7  | 24.90            | 0.468          | 43.45        | 19.89       | 1606.638       | 23.81     |
| 7  | 29.00            | 0.397          | 218.47       | 100.00      | 6746.416       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 12/7/2022 3:05:49 PM  
Printed by: wet


Ident: CCB  
Analysis from: 12/7/2022 1:57:59 PM  
File: \_2022-12-07\_

Last save: 12/7/2022 2:26:59 PM

Method: AnionsIC2-111722.mtw  
Run operator: wet  
Analysis number: 32737

Last save: 12/1/2022 4:34:

SAMPLE:  
: IZ/MA  
Vial number: 12  
Volume: 20.0  $\mu$ L  
Dilution: 1.00  
Amount: 1.0000

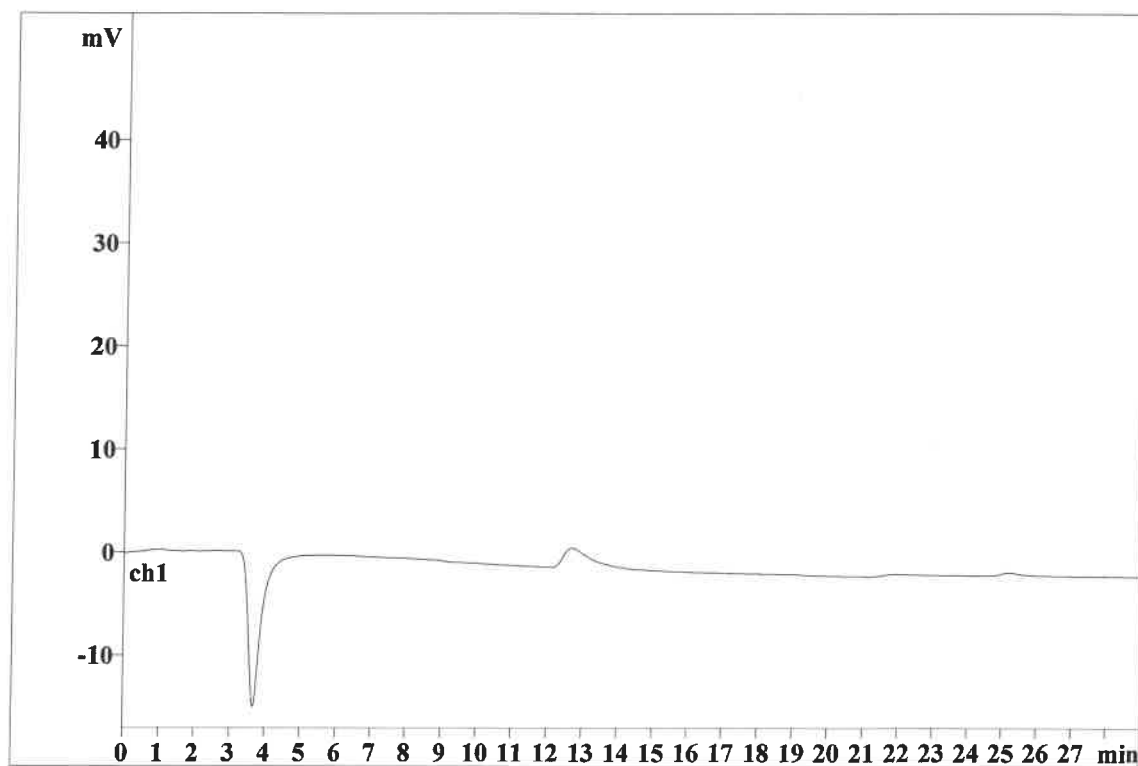

Quantitation method: Custom

No peaks

This report has been created by IC Net  
METROHM LTD