


LB123158

7470A

INSTRUMENT ID: CV2

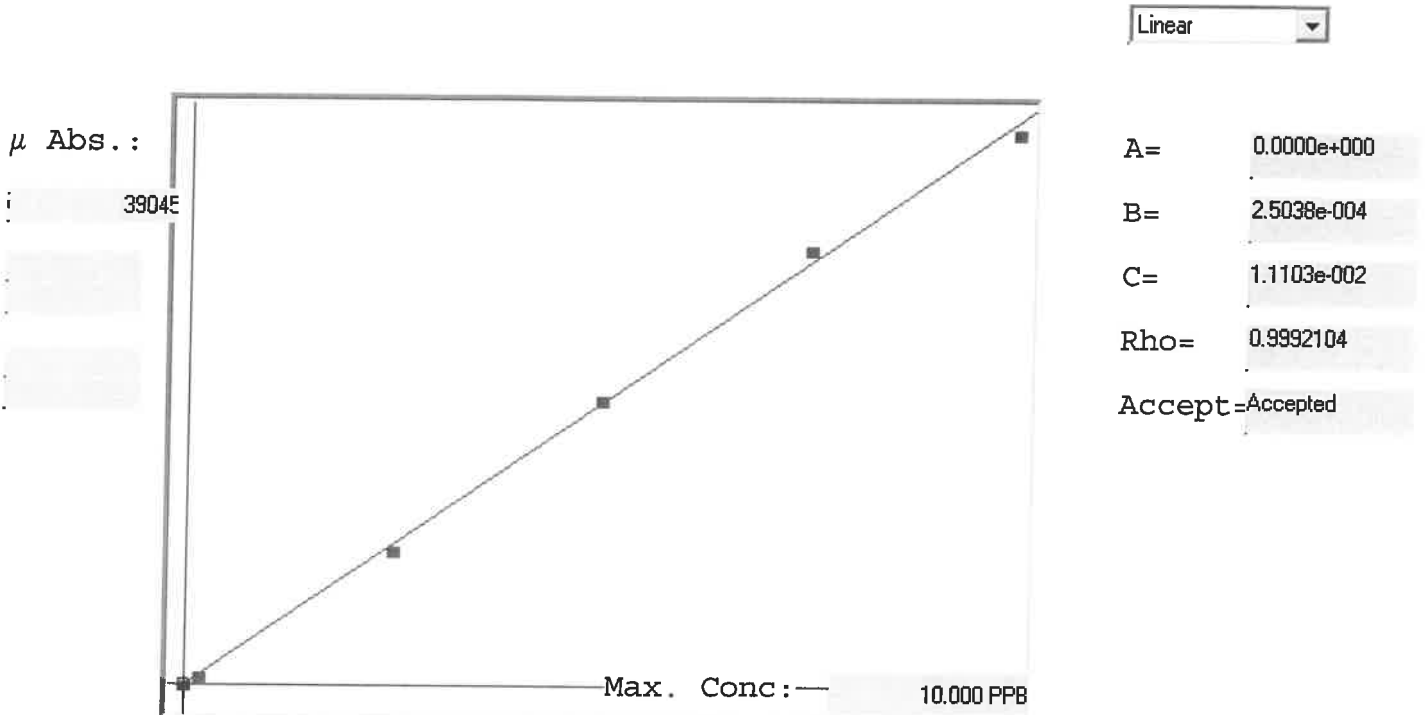

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	$\sigma/11$
0.0	0.000	0.016	0.016	20	0.000	20					
0.2	0.200	0.179	-0.021	671	0.0 %	671					-11
2.5	2.500	2.387	-0.113	9488	0.0 %	9488					-5
5.0	5.000	5.078	0.078	20237	0.0 %	20237					2
7.5	7.500	7.753	0.253	30921	0.0 %	30921					3
10.0	10.000	9.787	-0.213	39045	0.0 %	39045					-2

LB123158 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 08 Dec 2022 10:44:09

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	20	-	0.0000	7470A	PPB	08 Dec 2022 10:56:26	S	Std
0.2 - 1	50.2	671	-	0.2000	7470A	PPB	08 Dec 2022 10:58:44	S	Std
2.5 - 1	52.5	9488	-	2.5000	7470A	PPB	08 Dec 2022 11:01:01	S	Std
5.0 - 1	55	20237	-	5.0000	7470A	PPB	08 Dec 2022 11:03:18	S	Std
7.5 - 1	57.5	30921	-	7.5000	7470A	PPB	08 Dec 2022 11:05:35	S	Std
10.0 - 1	510	39045	-	10.0000	7470A	PPB	08 Dec 2022 11:07:51	S	Std
ICV49 - 1	ICV49	17220	4.3226	-	7470A	PPB	08 Dec 2022 11:10:39	U	SMPL
ICB49 - 1	ICB49	47	0.0229	-	7470A	PPB	08 Dec 2022 11:12:54	U	SMPL
CCV38 - 1	CCV38	18877	4.7375	-	7470A	PPB	08 Dec 2022 11:15:10	U	SMPL
CCB38 - 1	CCB38	-18	0.0066	-	7470A	PPB	08 Dec 2022 11:17:24	U	SMPL
CRA - 1	CRA	668	0.1784	-	7470A	PPB	08 Dec 2022 11:19:39	U	SMPL
HighStd - 1	HighStd	38178	9.5700	-	7470A	PPB	08 Dec 2022 11:21:55	U	SMPL
ChkStd - 1	ChkStd	26443	6.6318	-	7470A	PPB	08 Dec 2022 11:24:10	U	SMPL
PB149459BL - 1	PBW	-59	-0.0037	-	7470A	PPB	08 Dec 2022 11:26:26	U	SMPL
PB149459BS - 1	LCSW	15341	3.8521	-	7470A	PPB	08 Dec 2022 11:28:42	U	SMPL
N5868-02 - 1	TP-0	41	0.0214	-	7470A	PPB	08 Dec 2022 11:30:58	U	SMPL
N5878-01 - 1	MET-PAINT-1205	24	0.0171	-	7470A	PPB	08 Dec 2022 11:33:15	U	SMPL
N5883-02 - 1	MH-18	-8	0.0091	-	7470A	PPB	08 Dec 2022 11:35:32	U	SMPL
N5886-01 - 1	17208	-41	0.0008	-	7470A	PPB	08 Dec 2022 11:37:49	U	SMPL
N5886-02 - 1	COMP-1-1206	-8	0.0091	-	7470A	PPB	08 Dec 2022 11:40:04	U	SMPL
CCV39 - 1	CCV39	19749	4.9558	-	7470A	PPB	08 Dec 2022 11:42:19	U	SMPL
CCB39 - 1	CCB39	-68	-0.0059	-	7470A	PPB	08 Dec 2022 11:44:35	U	SMPL
N5895-02 - 1	MH-19	-8	0.0091	-	7470A	PPB	08 Dec 2022 11:46:50	U	SMPL
N5897-02 - 1	COMPOSITE	17	0.0154	-	7470A	PPB	08 Dec 2022 11:49:06	U	SMPL
N5897-02DUP - 1	COMPOSITEDUP	118	0.0406	-	7470A	PPB	08 Dec 2022 11:51:21	U	SMPL
N5897-02MS - 1	COMPOSITEMS	15081	3.7870	-	7470A	PPB	08 Dec 2022 11:53:38	U	SMPL
N5897-02MSD - 1	COMPOSITMSD	15757	3.9563	-	7470A	PPB	08 Dec 2022 11:55:53	U	SMPL
PB149460BL - 1	PBW	-28	0.0041	-	7470A	PPB	08 Dec 2022 11:58:09	U	SMPL
PB149460BS - 1	LCSW	14826	3.7232	-	7470A	PPB	08 Dec 2022 12:00:26	U	SMPL
N5886-03 - 1	COMP-2-1206	27	0.0179	-	7470A	PPB	08 Dec 2022 12:02:43	U	SMPL
N5886-03DUP - 1	COMP-2-1206DUP	79	0.0309	-	7470A	PPB	08 Dec 2022 12:04:59	U	SMPL
N5886-03MS - 1	COMP-2-1206MS	15915	3.9959	-	7470A	PPB	08 Dec 2022 12:07:15	U	SMPL
CCV40 - 1	CCV40	19273	4.8366	-	7470A	PPB	08 Dec 2022 12:09:31	U	SMPL
CCB40 - 1	CCB40	-33	0.0028	-	7470A	PPB	08 Dec 2022 12:11:46	U	SMPL
N5886-03MSD - 1	COMP-2-1206MSD	14650	3.6791	-	7470A	PPB	08 Dec 2022 12:14:02	U	SMPL
PB149461BL - 1	PBW	-14	0.0076	-	7470A	PPB	08 Dec 2022 12:16:18	U	SMPL
PB149461BS - 1	LCSW	16120	4.0472	-	7470A	PPB	08 Dec 2022 12:18:33	U	SMPL
N5890-03 - 1	COMP-1	681	0.1816	-	7470A	PPB	08 Dec 2022 12:20:49	U	SMPL
N5890-03DUP - 1	COMP-1DUP	639	0.1711	-	7470A	PPB	08 Dec 2022 12:26:12	U	SMPL
N5890-03MS - 1	COMP-1MS	13788	3.4633	-	7470A	PPB	08 Dec 2022 12:28:28	U	SMPL
N5890-03MSD - 1	COMP-1MSD	15396	3.8659	-	7470A	PPB	08 Dec 2022 12:30:44	U	SMPL
N5890-07 - 1	COMP-2	299349	HIGH	-	7470A	PPB	08 Dec 2022 12:33:01	X	
N5902-04 - 1	34503	67375	16.8803	-	7470A	PPB	08 Dec 2022 12:34:53	U	SMPL
N5903-01 - 1	34291	385	0.1075	-	7470A	PPB	08 Dec 2022 12:39:56	U	SMPL
CCV41 - 1	CCV41	20374	5.1123	-	7470A	PPB	08 Dec 2022 12:43:59	U	SMPL
CCB41 - 1	CCB41	-87	-0.0107	-	7470A	PPB	08 Dec 2022 12:46:14	U	SMPL
N5909-02 - 1	COMP	438	0.1208	-	7470A	PPB	08 Dec 2022 12:48:30	U	SMPL
N5911-01 - 1	A3594TOG	31	0.0189	-	7470A	PPB	08 Dec 2022 12:50:45	U	SMPL
N5912-01 - 1	FMC-TOTE-1207	273	0.0795	-	7470A	PPB	08 Dec 2022 12:53:01	U	SMPL
PB149440TB - 1	PB149440TB	-54	-0.0024	-	7470A	PPB	08 Dec 2022 12:55:16	U	SMPL
PB149452TB - 1	PB149452TB	-49	-0.0012	-	7470A	PPB	08 Dec 2022 12:57:32	U	SMPL
N5890-07DLX10 - 1		38745	9.7120	-	7470A	PPB	08 Dec 2022 12:59:49	U	SMPL
N5902-04DLX5 - 1		10231	2.5727	-	7470A	PPB	08 Dec 2022 13:02:05	U	SMPL
CCV42 - 1	CCV42	20430	5.1263	-	7470A	PPB	08 Dec 2022 13:04:22	U	SMPL
CCB42 - 1	CCB42	-10	0.0086	-	7470A	PPB	08 Dec 2022 13:06:39	U	SMPL
N5897-02LX5 - 1		-43	0.0003	-	7470A	PPB	08 Dec 2022 13:11:28	U	SMPL
N5897-02A - 1		17810	4.4703	-	7470A	PPB	08 Dec 2022 13:13:43	U	SMPL
N5886-03LX5 - 1		-44	0.0001	-	7470A	PPB	08 Dec 2022 13:15:59	U	SMPL
N5886-03A - 1		17053	4.2808	-	7470A	PPB	08 Dec 2022 13:18:15	U	SMPL
N5890-03 <i>4x5 ms</i>		-22	0.0056	-	7470A	PPB	08 Dec 2022 13:20:30	U	SMPL
N5890-03A - 1 <i>128122</i>		17470	4.3852	-	7470A	PPB	08 Dec 2022 13:24:01	U	SMPL
CCV43 - 1	CCV43	20466	5.1353	-	7470A	PPB	08 Dec 2022 13:26:17	U	SMPL
CCB43 - 1	CCB43	-35	0.0023	-	7470A	PPB	08 Dec 2022 13:28:32	U	SMPL