


69123287

7470A

INSTRUMENT ID: CV1

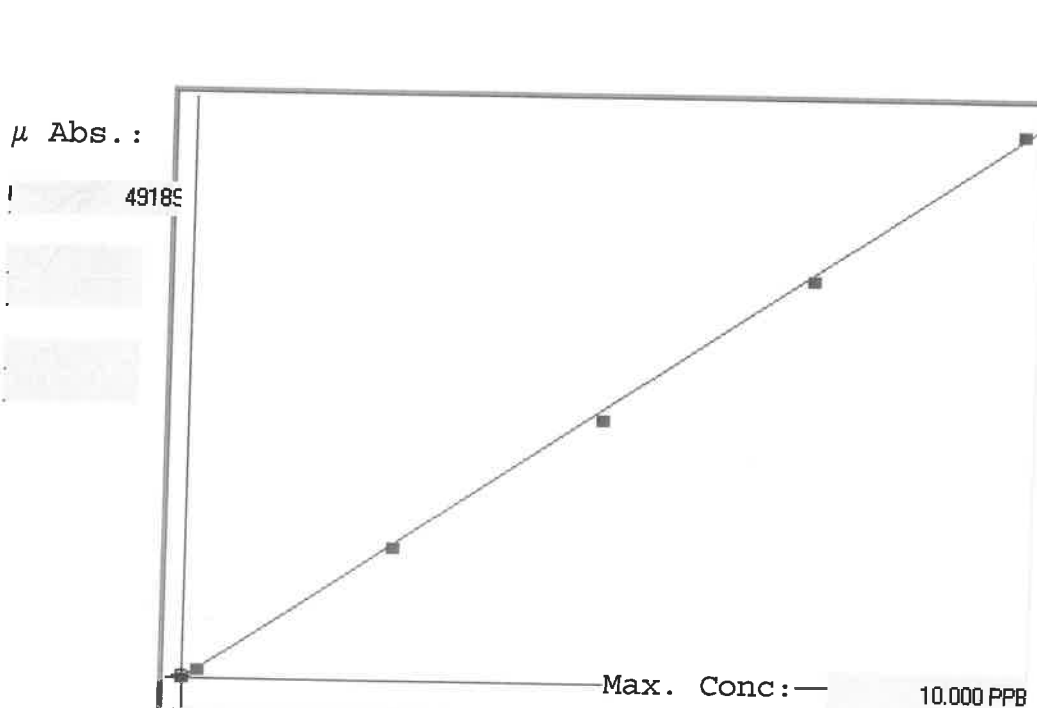

A= 0.0000e+000

B= 2.0495e-004

C= 2.0895e-002

Rho= 0.9997799

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	
0.0	0.000	0.063	0.063	206	0.000	206					0/00
0.2	0.200	0.225	0.025	998	0.0 %	998					13
2.5	2.500	2.494	-0.006	12068	0.0 %	12068					0
5.0	5.000	4.865	-0.135	23633	0.0 %	23633					3
7.5	7.500	7.450	-0.050	36249	0.0 %	36249					1
10.0	10.000	10.102	0.102	49189	0.0 %	49189					1

LB123287 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 15 Dec 2022 11:16:53

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	206	-	0.0000	7470A	PPB	15 Dec 2022 11:20:50	S	Std
0.2 - 1	50.2	998	-	0.2000	7470A	PPB	15 Dec 2022 11:23:07	S	Std
2.5 - 1	52.5	12068	-	2.5000	7470A	PPB	15 Dec 2022 11:25:24	S	Std
5.0 - 1	55	23633	-	5.0000	7470A	PPB	15 Dec 2022 11:27:41	S	Std
7.5 - 1	57.5	36249	-	7.5000	7470A	PPB	15 Dec 2022 11:29:57	S	Std
10.0 - 1	510	49189	-	10.0000	7470A	PPB	15 Dec 2022 11:34:46	S	Std
ICV56 - 1	ICV56	18009	3.7119	-	7470A	PPB	15 Dec 2022 11:37:29	U	SMPL
ICB56 - 1	ICB56	23	0.0256	-	7470A	PPB	15 Dec 2022 11:39:44	U	SMPL
CCV72 - 1	CCV72	23245	4.7850	-	7470A	PPB	15 Dec 2022 11:44:29	U	SMPL
CCB72 - 1	CCB72	-65	0.0076	-	7470A	PPB	15 Dec 2022 11:46:44	U	SMPL
CRA - 1	CRA	1053	0.2367	-	7470A	PPB	15 Dec 2022 11:54:07	U	SMPL
HighStd - 1	HighStd	49303	10.1257	-	7470A	PPB	15 Dec 2022 11:56:22	U	SMPL
ChkStd - 1	ChkStd	28734	5.9100	-	7470A	PPB	15 Dec 2022 11:58:38	U	SMPL
PB149650BL - 1	PBW	-39	0.0129	-	7470A	PPB	15 Dec 2022 12:00:53	U	SMPL
PB149650BS - 1	LCSW	17601	3.6283	-	7470A	PPB	15 Dec 2022 12:03:09	U	SMPL
N6024-02 - 1	TP-Q	27	0.0264	-	7470A	PPB	15 Dec 2022 12:05:25	U	SMPL
N6024-05 - 1	MH-21	34	0.0279	-	7470A	PPB	15 Dec 2022 12:07:42	U	SMPL
N6029-01 - 1	BLDG-77-STRUCTURAL-STEEL-PAINT	72	0.0357	-	7470A	PPB	15 Dec 2022 12:09:59	U	SMPL
N6035-02 - 1	BIC-1272	13	0.0236	-	7470A	PPB	15 Dec 2022 12:12:16	U	SMPL
N6048-02 - 1	MH-22	4	0.0217	-	7470A	PPB	15 Dec 2022 12:14:31	U	SMPL
CCV73 - 1	CCV73	23467	4.8305	-	7470A	PPB	15 Dec 2022 12:19:31	U	SMPL
CCB73 - 1	CCB73	-26	0.0156	-	7470A	PPB	15 Dec 2022 12:21:46	U	SMPL
N6048-05 - 1	TP-R	46	0.0303	-	7470A	PPB	15 Dec 2022 12:24:01	U	SMPL
N6048-05DUP - 1	TP-RDUP	66	0.0344	-	7470A	PPB	15 Dec 2022 12:26:17	U	SMPL
N6048-05MS - 1	TP-RMS	18372	3.7863	-	7470A	PPB	15 Dec 2022 12:28:32	U	SMPL
N6048-05MSD - 1	TP-RMSD	16774	3.4588	-	7470A	PPB	15 Dec 2022 12:30:48	U	SMPL
N6048-05LX5 - 1		-13	0.0182	-	7470A	PPB	15 Dec 2022 12:33:04	U	SMPL
N6048-05A - 1		18558	3.8244	-	7470A	PPB	15 Dec 2022 12:35:39	U	SMPL
PB149592TB - 1	PB149592TB	5	0.0219	-	7470A	PPB	15 Dec 2022 12:37:55	U	SMPL
CCV74 - 1	CCV74	23693	4.8769	-	7470A	PPB	15 Dec 2022 12:40:13	U	SMPL
CCB74 - 1	CCB74	-26	0.0156	-	7470A	PPB	15 Dec 2022 12:42:30	U	SMPL