


68123523

7470A

INSTRUMENT ID: CV2

Linear

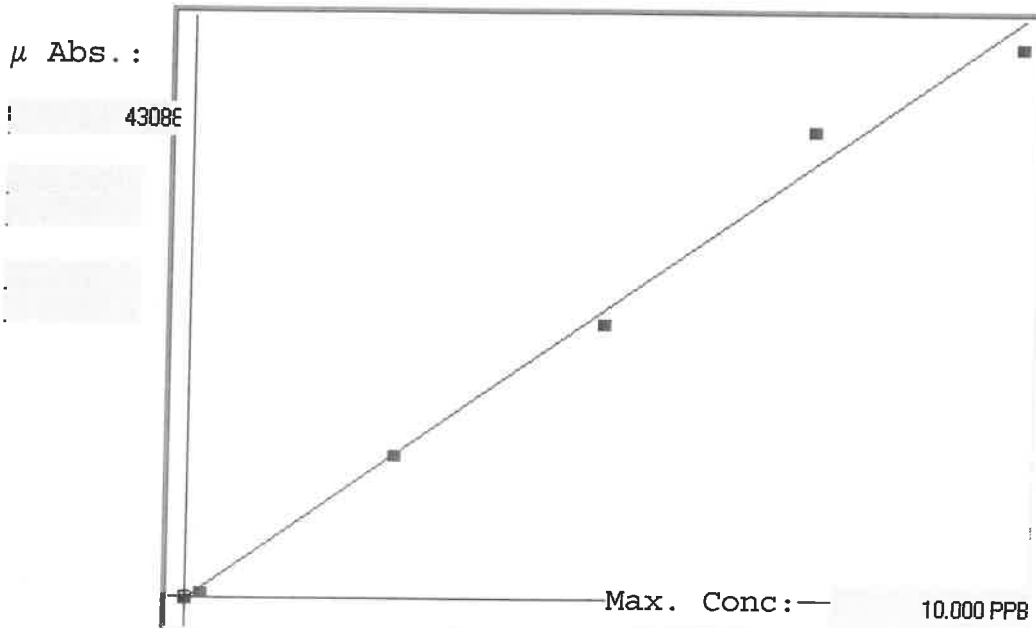

A= 0.0000e+000

B= 2.2132e-004

C= 3.3410e-002

Rho= 0.9961992

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.037	0.037	14	0.000	14					-
0.2	0.200	0.159	-0.041	569	0.0 %	569					-21
2.5	2.500	2.516	0.016	11217	0.0 %	11217					1
5.0	5.000	4.795	-0.205	21514	0.0 %	21514					-4
7.5	7.500	8.124	0.624	36556	0.0 %	36556					8
10.0	10.000	9.570	-0.430	43088	0.0 %	43088					-4

LB123523 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 04 Jan 2023 11:22:44

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	14	-	0.0000	7470A	PPB	04 Jan 2023 11:26:38	S	Std
0.2 - 1	502	569	-	0.2000	7470A	PPB	04 Jan 2023 11:28:56	S	Std
2.5 - 1	52.5	11217	-	2.5000	7470A	PPB	04 Jan 2023 11:31:14	S	Std
5.0 - 1	55	21514	-	5.0000	7470A	PPB	04 Jan 2023 11:33:33	S	Std
7.5 - 1	57.5	36556	-	7.5000	7470A	PPB	04 Jan 2023 11:35:49	S	Std
10.0 - 1	510	43088	-	10.0000	7470A	PPB	04 Jan 2023 11:40:41	S	Std
ICV88 - 1	ICV88	18419	4.1099	-	7470A	PPB	04 Jan 2023 11:43:39	U	SMPL
ICB88 - 1	ICB88	89	0.0531	-	7470A	PPB	04 Jan 2023 11:45:55	U	SMPL
CCV92 - 1	CCV92	20749	4.6255	-	7470A	PPB	04 Jan 2023 11:48:10	U	SMPL
CCB92 - 1	CCB92	15	0.0367	-	7470A	PPB	04 Jan 2023 11:50:25	U	SMPL
CRA - 1	CRA	841	0.2195	-	7470A	PPB	04 Jan 2023 11:52:40	U	SMPL
HighStd - 1	HighStd	43255	9.6065	-	7470A	PPB	04 Jan 2023 11:54:54	U	SMPL
ChkStd - 1	ChkStd	28628	6.3693	-	7470A	PPB	04 Jan 2023 11:57:10	U	SMPL
PB150041BL - 1	PBW	-31	0.0265	-	7470A	PPB	04 Jan 2023 11:59:25	U	SMPL
PB150041BS - 1	LCSW	15321	3.4242	-	7470A	PPB	04 Jan 2023 12:01:42	U	SMPL
N6183-06 - 1	R-2	38	0.0418	-	7470A	PPB	04 Jan 2023 12:03:58	U	SMPL
N6183-06DUP - 1	R-2DUP	37	0.0416	-	7470A	PPB	04 Jan 2023 12:06:15	U	SMPL
N6183-06MS - 1	R-2MS	17281	3.8580	-	7470A	PPB	04 Jan 2023 12:11:23	U	SMPL
N6183-06MSD - 1	R-2MSD	17231	3.8469	-	7470A	PPB	04 Jan 2023 12:13:40	U	SMPL
CCV93 - 1	CCV93	23107	5.1474	-	7470A	PPB	04 Jan 2023 12:15:56	U	SMPL
CCB93 - 1	CCB93	31	0.0403	-	7470A	PPB	04 Jan 2023 12:18:11	U	SMPL
N6183-06LX5 - 1		32	0.0405	-	7470A	PPB	04 Jan 2023 12:21:23	U	SMPL
N6183-06A - 1		18746	4.1822	-	7470A	PPB	04 Jan 2023 12:23:38	U	SMPL
PB150041TB - 1	PB150000TB	-1	0.0332	-	7470A	PPB	04 Jan 2023 12:25:54	U	SMPL
CCV94 - 1	CCV94	23650	5.2676	-	7470A	PPB	04 Jan 2023 12:28:09	U	SMPL
CCB94 - 1	CCB94	-1	0.0332	-	7470A	PPB	04 Jan 2023 12:30:25	U	SMPL