


LB123560

7470A

INSTRUMENT 1D; CV 1

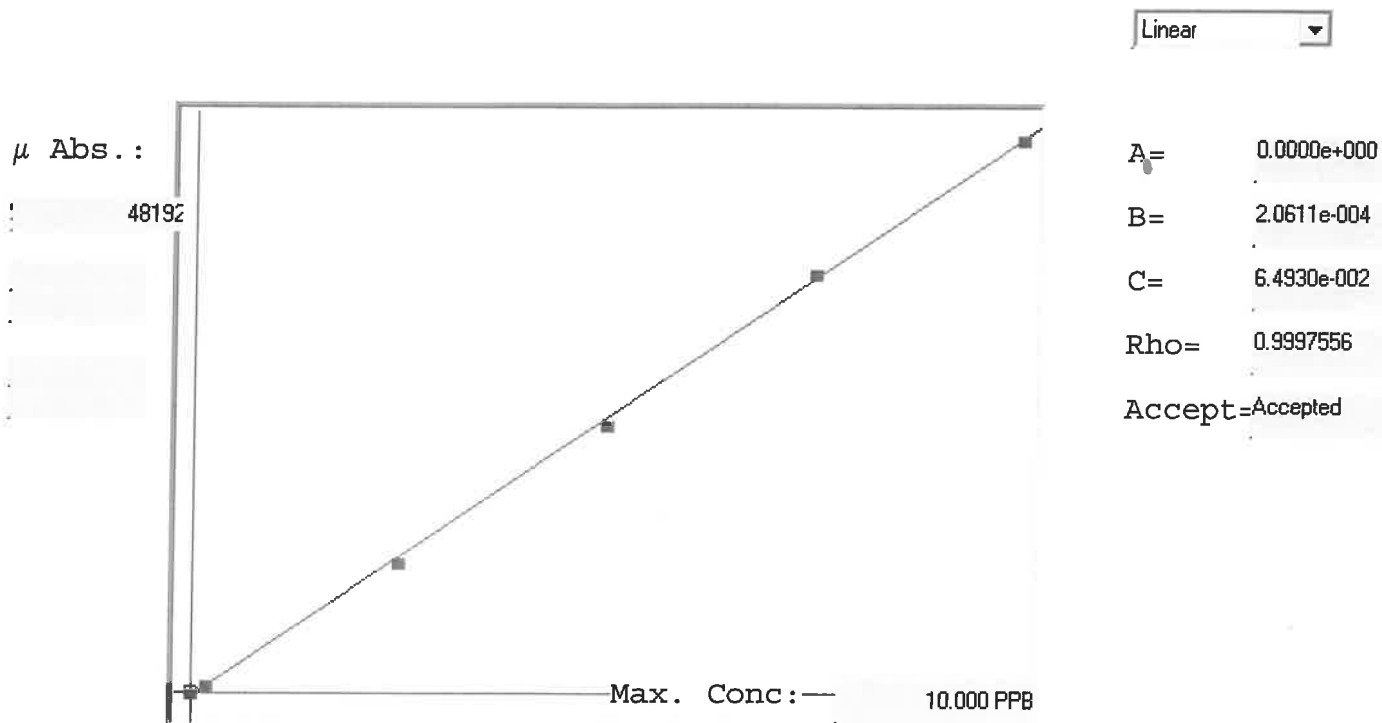

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.070	0.070	23	0.000	23					18
0.2	0.200	0.235	0.035	826	0.0 %	826					-4
2.5	2.500	2.411	-0.089	11384	0.0 %	11384					-2
5.0	5.000	4.879	-0.121	23359	0.0 %	23359					1
7.5	7.500	7.607	0.107	36592	0.0 %	36592					0
10.0	10.000	9.998	-0.002	48192	0.0 %	48192					

LB123560 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 06 Jan 2023 11:19:50

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	23	-	0.0000	7470A	PPB	06 Jan 2023 11:22:12	S	Std
0.2 - 1	50.2	826	-	0.2000	7470A	PPB	06 Jan 2023 11:24:29	S	Std
2.5 - 1	52.5	11384	-	2.5000	7470A	PPB	06 Jan 2023 11:26:46	S	Std
5.0 - 1	55	23359	-	5.0000	7470A	PPB	06 Jan 2023 11:29:04	S	Std
7.5 - 1	57.5	36592	-	7.5000	7470A	PPB	06 Jan 2023 11:31:20	S	Std
10.0 - 1	110	48192	-	10.0000	7470A	PPB	06 Jan 2023 11:33:36	S	Std
ICV93 - 1	ICV93	19352	4.0535	-	7470A	PPB	06 Jan 2023 11:36:30	U	SMPL
ICB93 - 1	ICB93	34	0.0719	-	7470A	PPB	06 Jan 2023 11:38:45	U	SMPL
CCV13 - 1	CCV13	23945	5.0002	-	7470A	PPB	06 Jan 2023 11:41:00	U	SMPL
CCB13 - 1	CCB13	45	0.0742	-	7470A	PPB	06 Jan 2023 11:43:15	U	SMPL
CRA - 1	CRA	842	0.2385	-	7470A	PPB	06 Jan 2023 11:45:30	U	SMPL
HighStd - 1	HighStd	48402	10.0410	-	7470A	PPB	06 Jan 2023 11:47:46	U	SMPL
ChkStd - 1	ChkStd	31999	6.6602	-	7470A	PPB	06 Jan 2023 11:50:01	U	SMPL
PB150044BL - 1	PBW	71	0.0796	-	7470A	PPB	06 Jan 2023 11:52:17	U	SMPL
PB150044BS - 1	LCSW	17026	3.5741	-	7470A	PPB	06 Jan 2023 11:54:33	U	SMPL
N6240-01 - 1	T4	179	0.1018	-	7470A	PPB	06 Jan 2023 11:56:50	U	SMPL
N6240-02 - 1	T5	186	0.1033	-	7470A	PPB	06 Jan 2023 11:59:06	U	SMPL
N6240-03 - 1	T6	110	0.0876	-	7470A	PPB	06 Jan 2023 12:01:23	U	SMPL
N6240-04 - 1	C1	58	0.0769	-	7470A	PPB	06 Jan 2023 12:03:40	U	SMPL
N6240-05 - 1	C2	28	0.0707	-	7470A	PPB	06 Jan 2023 12:05:56	U	SMPL
CCV14 - 1	CCV14	23934	4.9979	-	7470A	PPB	06 Jan 2023 12:08:11	U	SMPL
CCB14 - 1	CCB14	-83	0.0478	-	7470A	PPB	06 Jan 2023 12:10:27	U	SMPL
N6240-05DUP - 1	C2DUP	58	0.0769	-	7470A	PPB	06 Jan 2023 12:12:42	U	SMPL
N6240-05MSD - 1	C2MSD	18921	3.9647	-	7470A	PPB	06 Jan 2023 12:17:13	U	SMPL
PB150097BL - 1	PBW	-44	0.0559	-	7470A	PPB	06 Jan 2023 12:19:31	U	SMPL
PB150097BS - 1	LCSW	16743	3.5158	-	7470A	PPB	06 Jan 2023 12:21:46	U	SMPL
N6226-01 - 1	TWP01	3614	0.8098	-	7470A	PPB	06 Jan 2023 12:24:02	U	SMPL
N6226-02 - 1	TWP02	19250	4.0325	-	7470A	PPB	06 Jan 2023 12:26:19	U	SMPL
N6226-03 - 1	TWP01	-43	0.0561	-	7470A	PPB	06 Jan 2023 12:28:35	U	SMPL
N6226-04 - 1	TWP02	11	0.0672	-	7470A	PPB	06 Jan 2023 12:30:53	U	SMPL
N6232-01 - 1	MW-10	92	0.0839	-	7470A	PPB	06 Jan 2023 12:33:09	U	SMPL
CCV15 - 1	CCV15	24357	5.0851	-	7470A	PPB	06 Jan 2023 12:35:24	U	SMPL
CCB15 - 1	CCB15	-78	0.0489	-	7470A	PPB	06 Jan 2023 12:37:39	U	SMPL
N6232-02 - 1	MW-11	9	0.0668	-	7470A	PPB	06 Jan 2023 12:39:55	U	SMPL
N6232-03 - 1	MW-12	168	0.0996	-	7470A	PPB	06 Jan 2023 12:42:11	U	SMPL
N6232-04 - 1	MW-13	13	0.0676	-	7470A	PPB	06 Jan 2023 12:44:26	U	SMPL
O1006-01 - 1	33888	143	0.0944	-	7470A	PPB	06 Jan 2023 12:46:42	U	SMPL
O1006-02 - 1	33891-TOTE	83	0.0820	-	7470A	PPB	06 Jan 2023 12:48:57	U	SMPL
O1006-02DUP - 1	33891-TOTEDUP	51	0.0754	-	7470A	PPB	06 Jan 2023 12:51:14	U	SMPL
O1006-02MS - 1	33891-TOTEMS	16318	3.4282	-	7470A	PPB	06 Jan 2023 12:53:30	U	SMPL
O1006-02MSD - 1	33891-TOTEMSD	16897	3.5475	-	7470A	PPB	06 Jan 2023 12:55:47	U	SMPL
PB150023TB - 1	PB150023TB	2	0.0653	-	7470A	PPB	06 Jan 2023 12:58:04	U	SMPL
N6240-05MS - 1	C2MS	19136	4.0090	-	7470A	PPB	06 Jan 2023 13:00:19	U	SMPL
CCV16 - 1	CCV16	23944	5.0000	-	7470A	PPB	06 Jan 2023 13:02:35	U	SMPL
CCB16 - 1	CCB16	-22	0.0604	-	7470A	PPB	06 Jan 2023 13:04:50	U	SMPL
N6240-05LX5 - 1		31	0.0713	-	7470A	PPB	06 Jan 2023 13:07:06	U	SMPL
N6240-05A - 1		19869	4.1601	-	7470A	PPB	06 Jan 2023 13:09:21	U	SMPL
O1006-02LX5 - 1		27	0.0705	-	7470A	PPB	06 Jan 2023 13:11:37	U	SMPL
O1006-02A - 1		19962	4.1793	-	7470A	PPB	06 Jan 2023 13:13:52	U	SMPL
CCV17 - 1	CCV17	23991	5.0097	-	7470A	PPB	06 Jan 2023 13:16:08	U	SMPL
CCB17 - 1	CCB17	-37	0.0573	-	7470A	PPB	06 Jan 2023 13:18:24	U	SMPL