

LB123631

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

1/11/2023 11:34

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.009	0.0	0.108	
ICB1	0.000	0.0	0.011	
CCV1	1.007	0.0	0.108	
CCB1	0.001	0.0	0.011	
PB150181BL	-0.001	0.0	0.011	
PB150181BS	1.007	0.0	0.108	
O1094-01	-0.019	0.0	0.009	
O1094-01DUP	-0.018	0.0	0.009	
O1094-01MS	1.092	0.0	0.116	
O1094-01MSD	1.090	0.0	0.116	
O1094-03	-0.022	0.0	0.009	
CCV2	1.017	0.0	0.109	
CCB2	-0.003	0.0	0.011	

N	13
Mean	0.474
SD	0.5434
CV%	114.66

Aquakem v. 7.2AQ1

Results from time period:

Wed Jan 11 11:16:16 2023

Wed Jan 11 11:22:40 2023

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	-0.0022	mg/l	1/11/2023 9:46:04	
0.05PPM	A	Phenolics-	P	0.0537	mg/l	1/11/2023 9:46:05	
0.1PPM	A	Phenolics-	P	0.1073	mg/l	1/11/2023 9:46:06	
0.25PPM	A	Phenolics-	P	0.2542	mg/l	1/11/2023 9:46:07	
0.50PPM	A	Phenolics-	P	0.4996	mg/l	1/11/2023 9:46:08	
1.0PPM	A	Phenolics-	P	0.9765	mg/l	1/11/2023 9:46:09	
2.0PPM	A	Phenolics-	P	2.0109	mg/l	1/11/2023 9:46:10	
ICV1	S	Phenolics-	P	1.0091	mg/l	1/11/2023 11:16:16	
ICB1	S	Phenolics-	P	0.0001	mg/l	1/11/2023 11:16:19	
CCV1	S	Phenolics-	P	1.0074	mg/l	1/11/2023 11:16:20	
CCB1	S	Phenolics-	P	0.0009	mg/l	1/11/2023 11:16:23	
PB150181BL	S	Phenolics-	P	-0.0006	mg/l	1/11/2023 11:16:24	
PB150181BS	S	Phenolics-	P	1.0072	mg/l	1/11/2023 11:16:26	
O1094-01	S	Phenolics-	P	-0.019	mg/l	1/11/2023 11:22:34	
O1094-01DUP	S	Phenolics-	P	-0.0181	mg/l	1/11/2023 11:22:35	
O1094-01MS	S	Phenolics-	P	1.0924	mg/l	1/11/2023 11:22:36	
O1094-01MSD	S	Phenolics-	P	1.0897	mg/l	1/11/2023 11:22:37	
O1094-03	S	Phenolics-	P	-0.0222	mg/l	1/11/2023 11:22:38	
CCV2	S	Phenolics-	P	1.0166	mg/l	1/11/2023 11:22:39	
CCB2	S	Phenolics-	P	-0.0027	mg/l	1/11/2023 11:22:40	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

1/11/2023 9:46

Reviewed by : 12

Instrument ID : Konelab


Test Phenolics-

Accepted 1/11/2023 9:46

Factor 10.37
Bias 0.011

Coeff. of det. 0.999758

Errors

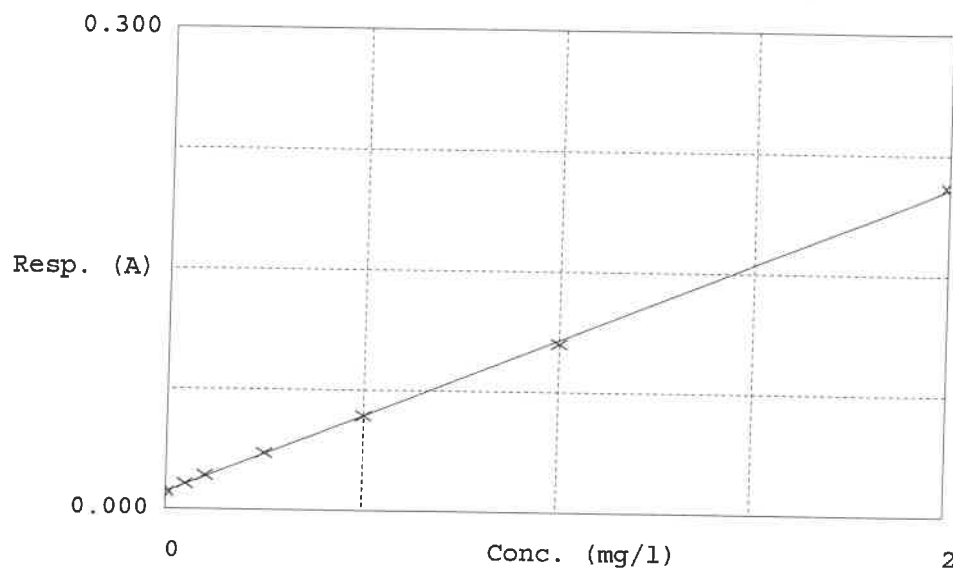

	Calibrator	Response	Calc. con.	Conc.	Re Errors
1	0.00PPM	0.011	-0.0022	0.0000	-
2	Phenol-2	0.016	0.0537	0.0500	7.4
3	Phenol-2	0.021	0.1073	0.1000	7.3
4	Phenol-2	0.035	0.2542	0.2500	1.7
5	Phenol-2	0.059	0.4996	0.5000	-2.1
6	Phenol-2	0.105	0.9765	1.0000	-2.4
7	Phenol-2	0.205	2.0109	2.0000	0.5

12/11/23