

LB 123723

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

1/18/2023 9:45

Test: CNEPA-NEW

Sample Id	Result	Dil. 1 +	Response	Errors
ICV0012ICV0012	98.318	0.0	0.096	
ICB0012ICB0012	0.748	0.0	0.009	
CCV0013CCV0013	248.241	0.0	0.230	
CCB0013CCB0013	0.620	0.0	0.009	
PB150309BL PBS309	0.923	0.0	0.009	
O1128-22 X3E37	197.089	0.0	0.185	
O1128-23 X3E37D	200.083	0.0	0.187	
O1128-24 X3E37S	290.606	0.0	0.268	
CCV0024CCV0024	253.310	0.0	0.235	
CCB0024CCB0024	0.403	0.0	0.009	

N 10
Mean 129.034
SD 121.2385
CV% 93.96

Aquakem v. 7.2AQ1

Results from time period:

Tue Jan 17 10:59:20 2023

Tue Jan 17 17:19:21 2023

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time
S0.0	A	CNEPA-NE\ P		-0.8596	µg/l	1/17/2023 10:59:20
S5.0	A	CNEPA-NE\ P		4.1166	µg/l	1/17/2023 10:59:21
S10.0	A	CNEPA-NE\ P		9.3529	µg/l	1/17/2023 10:59:22
S100.0	A	CNEPA-NE\ P		99.9705	µg/l	1/17/2023 10:59:23
S250.0	A	CNEPA-NE\ P		254.7838	µg/l	1/17/2023 10:59:24
S500.0	A	CNEPA-NE\ P		497.6358	µg/l	1/17/2023 10:59:25
ICV002 ICV002	S	CNEPA-NE\ P		98.3176	µg/l	1/17/2023 17:12:34
ICB002 ICB002	S	CNEPA-NE\ P		0.7483	µg/l	1/17/2023 17:12:37
CCV003 CCV003	S	CNEPA-NE\ P		248.2406	µg/l	1/17/2023 17:12:38
CCB003 CCB003	S	CNEPA-NE\ P		0.6198	µg/l	1/17/2023 17:12:40
PB150309BL PBS309	S	CNEPA-NE\ P		0.9228	µg/l	1/17/2023 17:12:43
O1128-22 X3E37	S	CNEPA-NE\ P		197.0891	µg/l	1/17/2023 17:19:13
O1128-23 X3E37D	S	CNEPA-NE\ P		200.0826	µg/l	1/17/2023 17:19:15
O1128-24 X3E37S	S	CNEPA-NE\ P		290.6056	µg/l	1/17/2023 17:19:17
CCV004 CCV004	S	CNEPA-NE\ P		253.3102	µg/l	1/17/2023 17:19:18
CCB004 CCB004	S	CNEPA-NE\ P		0.4026	µg/l	1/17/2023 17:19:21

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

1/17/2023 11:11


Test CNEPA-NEW

Accepted 1/17/2023 11:11

Factor slope 1119 0.000894
Bias % Intercept 0.009

Coeff. of det. 0.999846

Errors

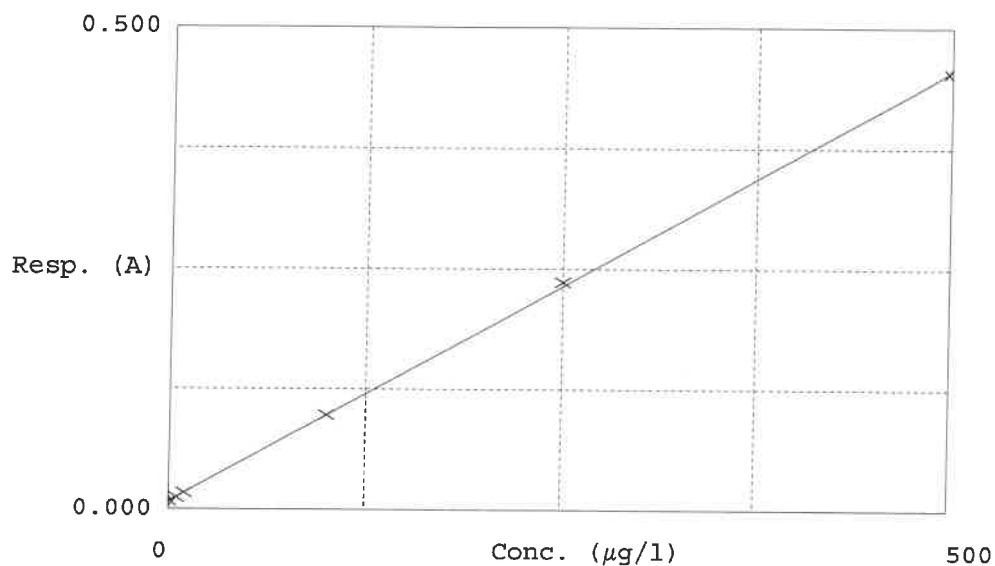

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN 50.0	0.008	-0.8596	0.0000	—
2	5.0PPBCN 550	0.012	4.1166	5.0000	-17.7
3	10PPBCN 510.0	0.017	9.3529	10.0000	-6.5
4	100PPBCN 5100.0	0.098	99.9705	100.0000	0.0
5	250PPBCN 5250.0	0.236	254.7838	250.0000	1.9
6	500PPBCN 5500.0	0.453	497.6358	500.0000	-0.5

12 1/17/23