

LB123868


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

39266

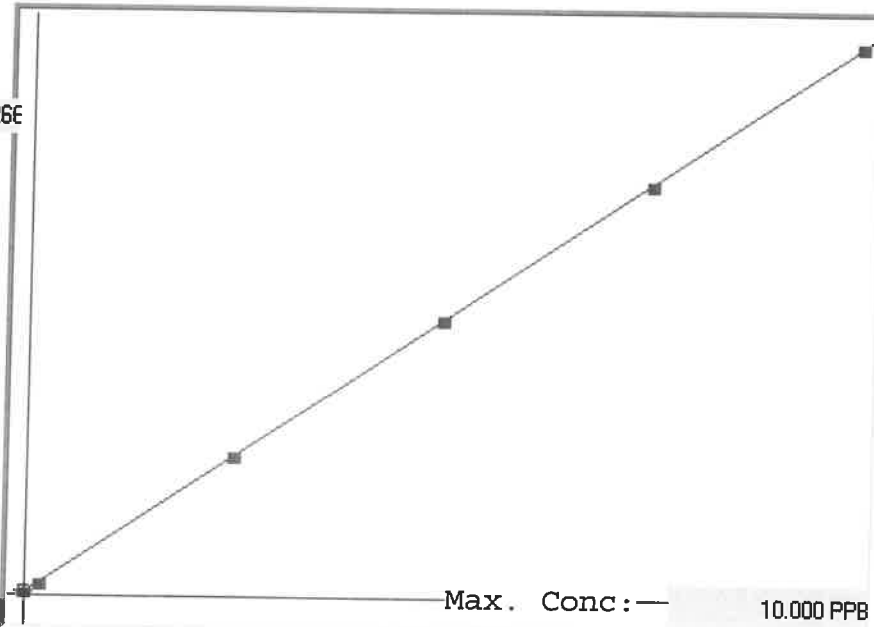

A= 0.0000e+000

B= 2.5632e-004

C= -5.7187e-002

Rho= 0.9999881

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/0/0
0.0	0.000	0.018	0.018	295	0.000	295					
0.2	0.200	0.175	-0.025	906	0.0 %	906					-13
2.5	2.500	2.503	0.003	9989	0.0 %	9989					0
5.0	5.000	5.019	0.019	19806	0.0 %	19806					0
7.5	7.500	7.477	-0.023	29393	0.0 %	29393					0
10.0	10.000	10.007	0.007	39266	0.0 %	39266					0

LB123868 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 31 Jan 2023 10:58:18

Sample ID	Extended ID	μ Abs.	Conc.	Std Cond	Method	Units	Date	Type	Type
0.0 - 1	50	295	-	0.0000	7470A	PPB	31 Jan 2023 11:06:34	S	Std
0.2 - 1	51.2	906	-	0.2000	7470A	PPB	31 Jan 2023 11:08:51	S	Std
2.5 - 1	52.5	9989	-	2.5000	7470A	PPB	31 Jan 2023 11:11:08	S	Std
5.0 - 1	55	19806	-	5.0000	7470A	PPB	31 Jan 2023 11:13:26	S	Std
7.5 - 1	57.5	29393	-	7.5000	7470A	PPB	31 Jan 2023 11:15:42	S	Std
10.0 - 1	510	39266	-	10.0000	7470A	PPB	31 Jan 2023 11:25:42	S	Std
ICV25 - 1	ICV25	15669	3.9590	-	7470A	PPB	31 Jan 2023 11:33:49	U	SMPL
ICB25 - 1	ICB25	10	-0.0546	-	7470A	PPB	31 Jan 2023 11:36:03	U	SMPL
CCV45 - 1	CCV45	19454	4.9292	-	7470A	PPB	31 Jan 2023 11:38:19	U	SMPL
CCB45 - 1	CCB45	-13	-0.0605	-	7470A	PPB	31 Jan 2023 11:40:34	U	SMPL
CRA - 1	CRA	955	0.1876	-	7470A	PPB	31 Jan 2023 11:45:23	U	SMPL
HighStd - 1	HighStd	39604	10.0939	-	7470A	PPB	31 Jan 2023 11:47:38	U	SMPL
ChkStd - 1	ChkStd	26665	6.7775	-	7470A	PPB	31 Jan 2023 11:49:53	U	SMPL
PB150552BL - 1	PBW	-76	-0.0767	-	7470A	PPB	31 Jan 2023 11:52:09	U	SMPL
PB150552BS - 1	LCSW	13749	3.4669	-	7470A	PPB	31 Jan 2023 11:54:26	U	SMPL
O1328-02 - 1	COMP-1-BORING-1-0-7	5	-0.0559	-	7470A	PPB	31 Jan 2023 11:56:43	U	SMPL
O1328-07 - 1	COMP-2-BORING-1-7-14	2	-0.0567	-	7470A	PPB	31 Jan 2023 11:59:00	U	SMPL
O1328-12 - 1	COMP-3-BORING-1-14-23	0	-0.0572	-	7470A	PPB	31 Jan 2023 12:01:17	U	SMPL
O1328-17 - 1	COMP-4-BORING-1-23-25	-8	-0.0592	-	7470A	PPB	31 Jan 2023 12:03:35	U	SMPL
O1328-22 - 1	COMP-5-BORING-2-0-7	39	-0.0472	-	7470A	PPB	31 Jan 2023 12:05:51	U	SMPL
CCV46 - 1	CCV46	20023	5.0750	-	7470A	PPB	31 Jan 2023 12:08:06	U	SMPL
CCB46 - 1	CCB46	-20	-0.0623	-	7470A	PPB	31 Jan 2023 12:10:21	U	SMPL
O1329-02 - 1	COMP-6-BORING-2-7-14	4	-0.0562	-	7470A	PPB	31 Jan 2023 12:12:37	U	SMPL
O1329-07 - 1	COMP-7-BORING-2-14-21	10	-0.0546	-	7470A	PPB	31 Jan 2023 12:14:52	U	SMPL
O1329-12 - 1	COMP-8-BORING-2-21-28	6	-0.0556	-	7470A	PPB	31 Jan 2023 12:17:08	U	SMPL
O1329-17 - 1	COMP-9-BORING-2-28-3	9	-0.0549	-	7470A	PPB	31 Jan 2023 12:19:24	U	SMPL
O1333-02 - 1	TP-I	24	-0.0510	-	7470A	PPB	31 Jan 2023 12:21:40	U	SMPL
O1333-05 - 1	MH-11	7	-0.0554	-	7470A	PPB	31 Jan 2023 12:23:56	U	SMPL
O1335-01 - 1	334-337	0	-0.0572	-	7470A	PPB	31 Jan 2023 12:26:13	U	SMPL
O1352-02 - 1	TP-2-WC	7	-0.0554	-	7470A	PPB	31 Jan 2023 12:28:30	U	SMPL
O1356-02 - 1	TP-J	23	-0.0513	-	7470A	PPB	31 Jan 2023 12:30:47	U	SMPL
O1356-02DUP - 1	TP-JDUP	10	-0.0546	-	7470A	PPB	31 Jan 2023 12:33:03	U	SMPL
CCV47 - 1	CCV47	20403	5.1724	-	7470A	PPB	31 Jan 2023 12:35:19	U	SMPL
CCB47 - 1	CCB47	-9	-0.0595	-	7470A	PPB	31 Jan 2023 12:37:34	U	SMPL
O1356-02MS - 1	TP-JMS	16072	4.0623	-	7470A	PPB	31 Jan 2023 12:45:15	U	SMPL
O1356-02MSD - 1	TP-JMSD	16150	4.0823	-	7470A	PPB	31 Jan 2023 12:50:05	U	SMPL
PB150553BL - 1	PBW	-37	-0.0667	-	7470A	PPB	31 Jan 2023 12:52:20	U	SMPL
PB150553BS - 1	LCSW	14664	3.7014	-	7470A	PPB	31 Jan 2023 12:54:36	U	SMPL
O1285-03 - 1	EB-2023-1-24	-20	-0.0623	-	7470A	PPB	31 Jan 2023 12:56:52	U	SMPL
O1320-01 - 1	TOTE-COMP-0126	2216	0.5108	-	7470A	PPB	31 Jan 2023 12:59:08	U	SMPL
O1327-01 - 1	N48965	4869	1.1908	-	7470A	PPB	31 Jan 2023 13:01:25	U	SMPL
O1327-01DUP - 1	N48965DUP	4700	1.1475	-	7470A	PPB	31 Jan 2023 13:03:42	U	SMPL
O1327-01MS - 1	N48965MS	19729	4.9997	-	7470A	PPB	31 Jan 2023 13:06:00	U	SMPL
O1327-01MSD - 1	N48965MSD	18694	4.7344	-	7470A	PPB	31 Jan 2023 13:08:16	U	SMPL
CCV48 - 1	CCV48	19613	4.9699	-	7470A	PPB	31 Jan 2023 13:10:32	U	SMPL
CCB48 - 1	CCB48	-81	-0.0779	-	7470A	PPB	31 Jan 2023 13:12:48	U	SMPL
PB150522TB - 1	PB150522TB	18	-0.0526	-	7470A	PPB	31 Jan 2023 13:15:04	U	SMPL
O1356-02LX5 - 1		20	-0.0521	-	7470A	PPB	31 Jan 2023 13:17:20	U	SMPL
O1356-02A - 1		16906	4.2761	-	7470A	PPB	31 Jan 2023 13:19:35	U	SMPL
O1327-01LX5 - 1		912	0.1766	-	7470A	PPB	31 Jan 2023 13:21:51	U	SMPL
O1327-01A - 1		18492	4.6826	-	7470A	PPB	31 Jan 2023 13:24:08	U	SMPL
CCV49 - 1	CCV49	19078	4.8328	-	7470A	PPB	31 Jan 2023 13:28:04	U	SMPL
CCB49 - 1	CCB49	-3	-0.0580	-	7470A	PPB	31 Jan 2023 13:30:20	U	SMPL