

LB123954


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

42351

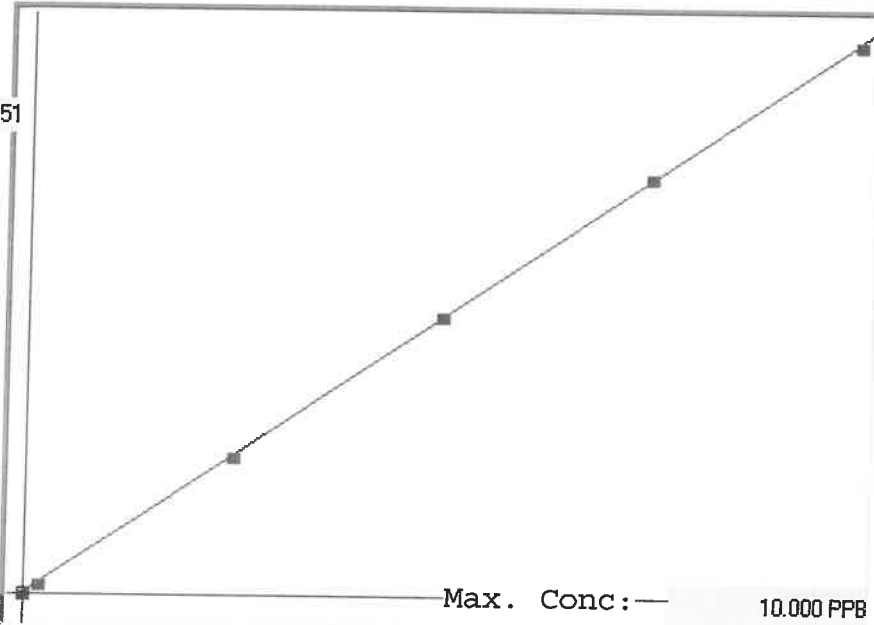

A= 0.0000e+000

B= 2.3528e-004

C= -2.2245e-002

Rho= 0.9999436

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	% (1)
0.0	0.000	0.002	0.002	103	0.000	103					
0.2	0.200	0.179	-0.021	855	0.0 %	855					-1)
2.5	2.500	2.478	-0.022	10626	0.0 %	10626					-1
5.0	5.000	5.046	0.046	21540	0.0 %	21540					1
7.5	7.500	7.553	0.053	32198	0.0 %	32198					1
10.0	10.000	9.942	-0.058	42351	0.0 %	42351					-1

LB123954 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 07 Feb 2023 09:27:14

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	103	-	0.0000	7470A	PPB	07 Feb 2023 10:37:24	S	Std
0.2 - 1	50.2	855	-	0.2000	7470A	PPB	07 Feb 2023 10:39:42	S	Std
2.5 - 1	52.5	10626	-	2.5000	7470A	PPB	07 Feb 2023 10:41:59	S	Std
5.0 - 1	55	21540	-	5.0000	7470A	PPB	07 Feb 2023 10:44:16	S	Std
7.5 - 1	57.5	32198	-	7.5000	7470A	PPB	07 Feb 2023 10:46:32	S	Std
10.0 - 1	510	42351	-	10.0000	7470A	PPB	07 Feb 2023 10:48:48	S	Std
ICV35 - 1	ICV35	17600	4.1187	-	7470A	PPB	07 Feb 2023 10:51:30	U	SMPL
ICB35 - 1	ICB35	18	-0.0180	-	7470A	PPB	07 Feb 2023 10:53:45	U	SMPL
CCV89 - 1	CCV89	21737	5.0921	-	7470A	PPB	07 Feb 2023 10:56:00	U	SMPL
CCB89 - 1	CCB89	1	-0.0220	-	7470A	PPB	07 Feb 2023 10:58:15	U	SMPL
CRA - 1	CRA	864	0.1810	-	7470A	PPB	07 Feb 2023 11:00:31	U	SMPL
HighStd - 1	HighStd	42826	10.0539	-	7470A	PPB	07 Feb 2023 11:02:46	U	SMPL
ChkStd - 1	ChkStd	29464	6.9101	-	7470A	PPB	07 Feb 2023 11:05:02	U	SMPL
PB150673BL - 1	PBW	-53	-0.0347	-	7470A	PPB	07 Feb 2023 11:07:18	U	SMPL
PB150673BS - 1	LCSW	17385	4.0681	-	7470A	PPB	07 Feb 2023 11:12:07	U	SMPL
O1402-01 - 1	20230201-H4-STOCKPILE	-6	-0.0237	-	7470A	PPB	07 Feb 2023 11:14:23	U	SMPL
O1406-01 - 1	5715	1341	0.2933	-	7470A	PPB	07 Feb 2023 11:16:39	U	SMPL
O1407-02 - 1	30987	-199	-0.0691	-	7470A	PPB	07 Feb 2023 11:18:57	U	SMPL
O1407-03 - 1	30988	-72	-0.0392	-	7470A	PPB	07 Feb 2023 11:21:18	U	SMPL
O1407-03DUP - 1	30988DUP	22	-0.0171	-	7470A	PPB	07 Feb 2023 11:23:35	U	SMPL
CCV90 - 1	CCV90	21681	5.0789	-	7470A	PPB	07 Feb 2023 11:25:52	U	SMPL
CCB90 - 1	CCB90	-22	-0.0274	-	7470A	PPB	07 Feb 2023 11:28:07	U	SMPL
O1407-03MS - 1	30988MS	16249	3.8008	-	7470A	PPB	07 Feb 2023 11:30:22	U	SMPL
O1407-03MSD - 1	30988MSD	17508	4.0971	-	7470A	PPB	07 Feb 2023 11:32:38	U	SMPL
PB150687BL - 1	PBW	27	-0.0159	-	7470A	PPB	07 Feb 2023 11:34:53	U	SMPL
PB150687BS - 1	LCSW	17537	4.1039	-	7470A	PPB	07 Feb 2023 11:37:08	U	SMPL
O1406-02 - 1	COMP1-0202	36	-0.0138	-	7470A	PPB	07 Feb 2023 11:39:24	U	SMPL
O1406-02DUP - 1	COMP1-0202DUP	174	0.0187	-	7470A	PPB	07 Feb 2023 11:41:41	U	SMPL
O1406-02MS - 1	COMP1-0202MS	16280	3.8081	-	7470A	PPB	07 Feb 2023 11:48:38	U	SMPL
O1406-02MSD - 1	COMP1-0202MSD	17417	4.0757	-	7470A	PPB	07 Feb 2023 11:50:55	U	SMPL
O1406-03 - 1	COMP2-0202	14	-0.0190	-	7470A	PPB	07 Feb 2023 11:53:15	U	SMPL
PB150701BL - 1	PBW	67	-0.0065	-	7470A	PPB	07 Feb 2023 11:55:31	U	SMPL
CCV91 - 1	CCV91	21466	5.0283	-	7470A	PPB	07 Feb 2023 11:57:46	U	SMPL
CCB91 - 1	CCB91	-54	-0.0349	-	7470A	PPB	07 Feb 2023 12:00:03	U	SMPL
PB150701BS - 1	LCSW	17544	4.1055	-	7470A	PPB	07 Feb 2023 12:02:18	U	SMPL
O1388-02 - 1	COMP	442	0.0817	-	7470A	PPB	07 Feb 2023 12:04:34	U	SMPL
O1407-05 - 1	30985	1360	0.2977	-	7470A	PPB	07 Feb 2023 12:06:49	U	SMPL
O1407-06 - 1	30986	4161	0.9568	-	7470A	PPB	07 Feb 2023 12:09:05	U	SMPL
O1416-03 - 1	EB-2023-2-2	-79	-0.0408	-	7470A	PPB	07 Feb 2023 12:11:21	U	SMPL
O1437-03 - 1	31956	795	0.1648	-	7470A	PPB	07 Feb 2023 12:13:37	U	SMPL
O1437-04 - 1	2423	1234	0.2681	-	7470A	PPB	07 Feb 2023 12:15:54	U	SMPL
O1440-01 - 1	MH-1	59	-0.0084	-	7470A	PPB	07 Feb 2023 12:18:11	U	SMPL
O1442-02 - 1	EB-2023-2-3	-23	-0.0277	-	7470A	PPB	07 Feb 2023 12:20:28	U	SMPL
O1447-01 - 1	T2	373	0.0655	-	7470A	PPB	07 Feb 2023 12:22:44	U	SMPL
CCV92 - 1	CCV92	20879	4.8902	-	7470A	PPB	07 Feb 2023 12:25:00	U	SMPL
CCB92 - 1	CCB92	36	-0.0138	-	7470A	PPB	07 Feb 2023 12:27:16	U	SMPL
O1447-01DUP - 1	T2DUP	227	0.0312	-	7470A	PPB	07 Feb 2023 12:32:17	U	SMPL
O1447-01MS - 1	T2MS	15528	3.6312	-	7470A	PPB	07 Feb 2023 12:34:33	U	SMPL
O1447-01MSD - 1	T2MSD	15145	3.5411	-	7470A	PPB	07 Feb 2023 12:36:48	U	SMPL
O1407-03LX5 - 1		-35	-0.0305	-	7470A	PPB	07 Feb 2023 12:39:04	U	SMPL
O1406-02LX5 - 1		-37	-0.0309	-	7470A	PPB	07 Feb 2023 12:43:37	U	SMPL
O1447-01LX5 - 1		29	-0.0154	-	7470A	PPB	07 Feb 2023 12:48:12	U	SMPL
O1447-01A - 1		14736	3.4449	-	7470A	PPB	07 Feb 2023 12:50:29	U	SMPL
O1407-03A - 1		17180	4.0199	-	7470A	PPB	07 Feb 2023 12:53:19	U	SMPL
O1406-02A - 1		16587	3.8804	-	7470A	PPB	07 Feb 2023 12:55:56	U	SMPL
CCV93 - 1	CCV93	19765	4.6281	-	7470A	PPB	07 Feb 2023 12:58:34	U	SMPL
CCB93 - 1	CCB93	17	-0.0182	-	7470A	PPB	07 Feb 2023 13:00:49	U	SMPL
PB150653TB - 1	PB150653TB	21	-0.0173	-	7470A	PPB	07 Feb 2023 13:03:05	U	SMPL
PB150649TB - 1	PB150649TB	3	-0.0215	-	7470A	PPB	07 Feb 2023 13:05:21	U	SMPL
CCV94 - 1	CCV94	19802	4.6368	-	7470A	PPB	07 Feb 2023 13:07:37	U	SMPL
CCB94 - 1	CCB94	-16	-0.0260	-	7470A	PPB	07 Feb 2023 13:09:53	U	SMPL