

Clear table

Instrument ID: IC-2											Analyst :	IZ	Method:	300.0 / 9056A		
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst					
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2023-01-19_	1/19/23 11:00		IZ/MA					
STD2	0.4880	0.6840	0.7060	2.3300	0.5760	1.0560	3.4740	2023-01-19_	1/19/23 11:31		IZ/MA					
STD3	0.7760	1.2150	1.2130	4.0420	1.0070	2.0000	6.0020	2023-01-19_	1/19/23 12:01		IZ/MA					
STD4	0.9450	1.5030	1.5180	5.0520	1.2780	2.5430	7.4510	2023-01-19_	1/19/23 12:32		IZ/MA					
STD5	1.8550	2.8760	2.8370	9.5070	2.3720	4.8860	14.5380	2023-01-19_	1/19/23 13:02		IZ/MA					
STD6	3.9270	5.9350	5.9150	19.6950	4.9230	9.9270	29.5160	2023-01-19_	1/19/23 13:33		IZ/MA					
STD7	5.0990	7.5870	7.6110	25.3740	6.3440	12.5880	38.0180	2023-01-19_	1/19/23 14:04		IZ/MA					
ICV	1.8290	2.9990	3.0090	9.9010	2.4740	4.7390	14.6300	2023-01-19_	1/19/23 15:07		IZ/MA					
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-01-19_	1/19/23 15:38		IZ/MA					
CCV	1.9980	2.9530	2.8690	9.8220	2.4350	5.3580	14.5790	2023-02-07_	2/7/23 10:28		IZ/MA					
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-02-07_	2/7/23 10:59		IZ/MA					
LB123983BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-02-07_	2/7/23 11:30		IZ/MA					
LB123983BSW	1.8340	2.7860	2.6430	9.2580	2.2950	4.7730	13.6780	2023-02-07_	2/7/23 12:00		IZ/MA					
O1468-01	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-02-07_	2/7/23 12:58		IZ/MA					
O1468-01MS	1.8790	2.9200	2.7960	9.6130	2.4390	4.8940	14.3500	2023-02-07_	2/7/23 13:29		IZ/MA					
O1468-01MSD	1.8710	2.8810	2.7820	9.4970	2.4160	4.9080	14.1360	2023-02-07_	2/7/23 14:00		IZ/MA					
CCV	1.8970	2.9810	2.8720	9.9170	2.4730	5.1610	14.6280	2023-02-07_	2/7/23 14:30		IZ/MA					
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-02-07_	2/7/23 15:01		IZ/MA					

Report date: 2/8/2023 1:35:33 PM
Printed by: wet


Ident: CCV
Analysis from: 2/7/2023 10:28:12 AM
File: _2023-02-07_

Last save: 2/7/2023 10:56:37 AM

Method: AnionsIC2-011923.mtw
Run operator: wet
Analysis number: 33222

Last save: 2/1/2023 10:37:

SAMPLE:
: IZ/MA
Vial number: 23
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

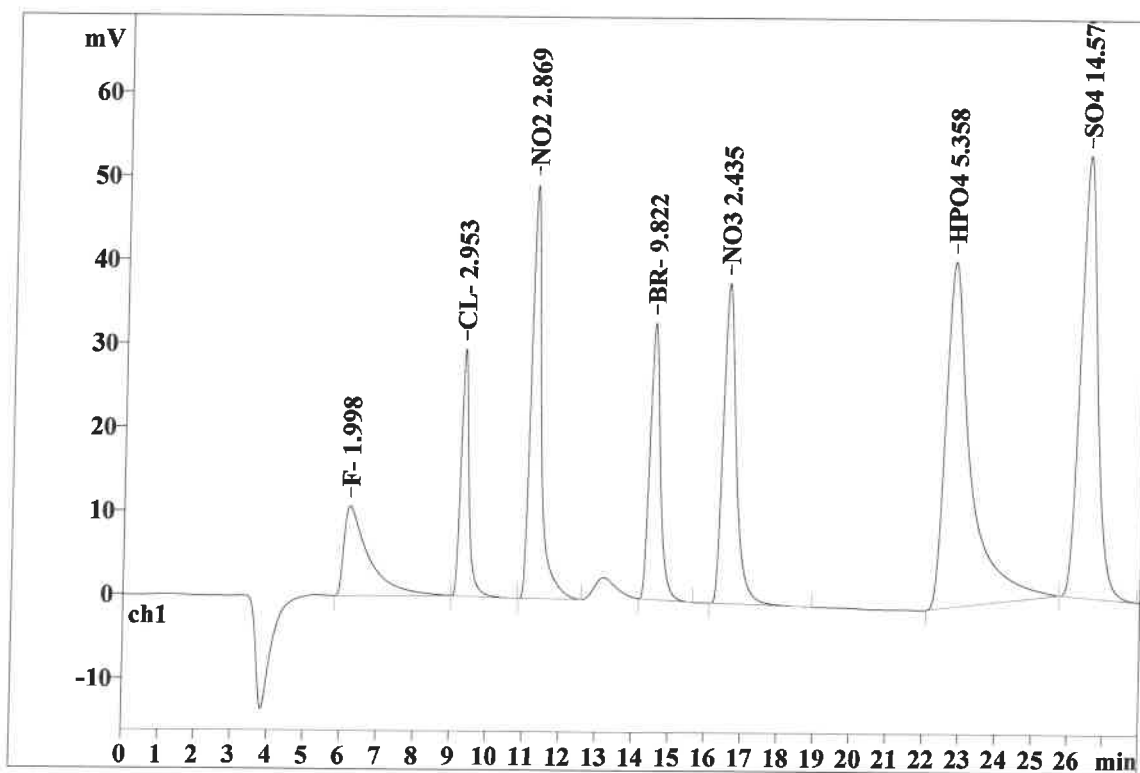

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.20	0.626	10.74	4.21	503.269	6.89
2	9.29	0.220	29.53	11.58	453.881	6.21
3	11.20	0.272	49.40	19.37	969.934	13.28
4	14.50	0.302	33.03	12.95	668.328	9.15
5	16.53	0.367	38.23	14.99	955.442	13.08
6	22.74	0.617	41.30	16.19	1990.269	27.25
7	26.43	0.505	52.81	20.71	1762.267	24.13
7	28.00	0.416	255.05	100.00	7303.390	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/8/2023 1:35:41 PM
Printed by: wet


Ident: CCB
Analysis from: 2/7/2023 10:59:26 AM
File: _2023-02-07_

Last save: 2/7/2023 11:27:26 AM

Method: AnionsIC2-011923.mtw
Run operator: wet
Analysis number: 33223

Last save: 2/1/2023 10:37:

SAMPLE:
:
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

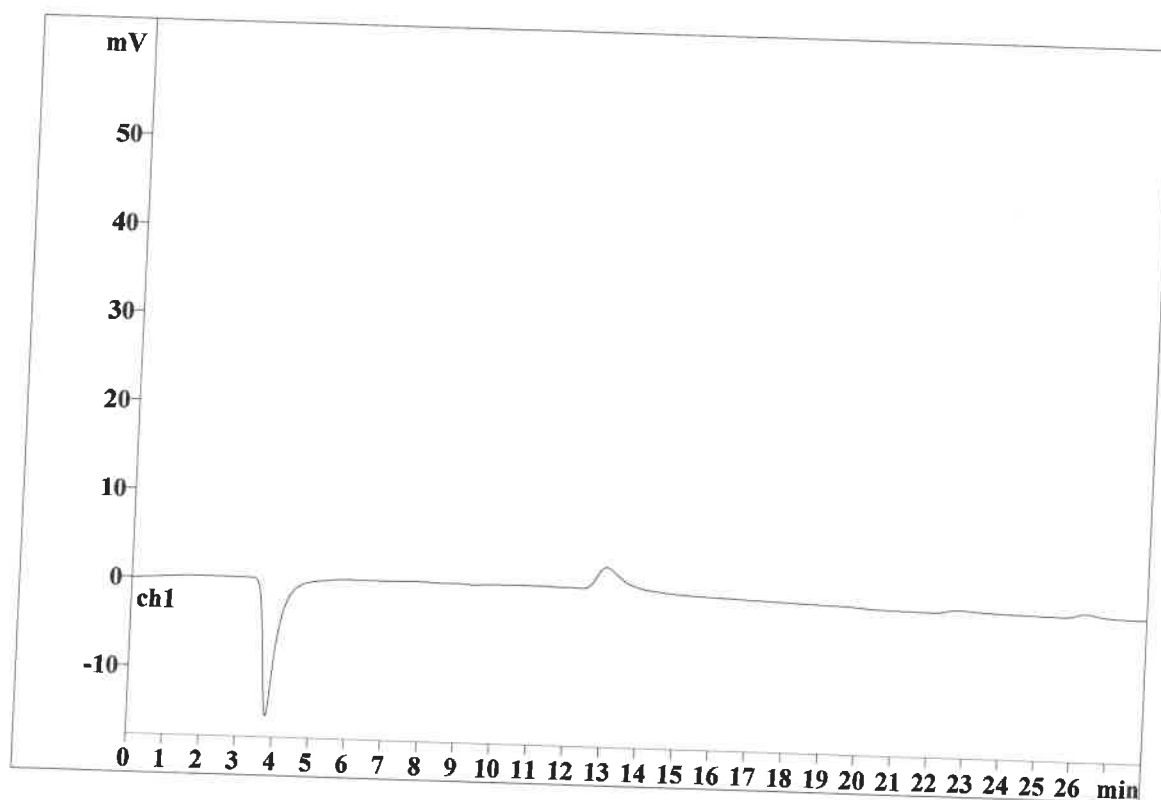

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 2/8/2023 1:35:48 PM
Printed by: wet


Ident: LB123983BLW
Analysis from: 2/7/2023 11:30:04 AM
File: _2023-02-07_

Last save: 2/8/2023 1:34:37 PM

Method: AnionsIC2-011923.mtw
Run operator: wet
Analysis number: 33224

Last save: 2/1/2023 10:37:

SAMPLE:
: IZ/MA
Vial number: 13
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

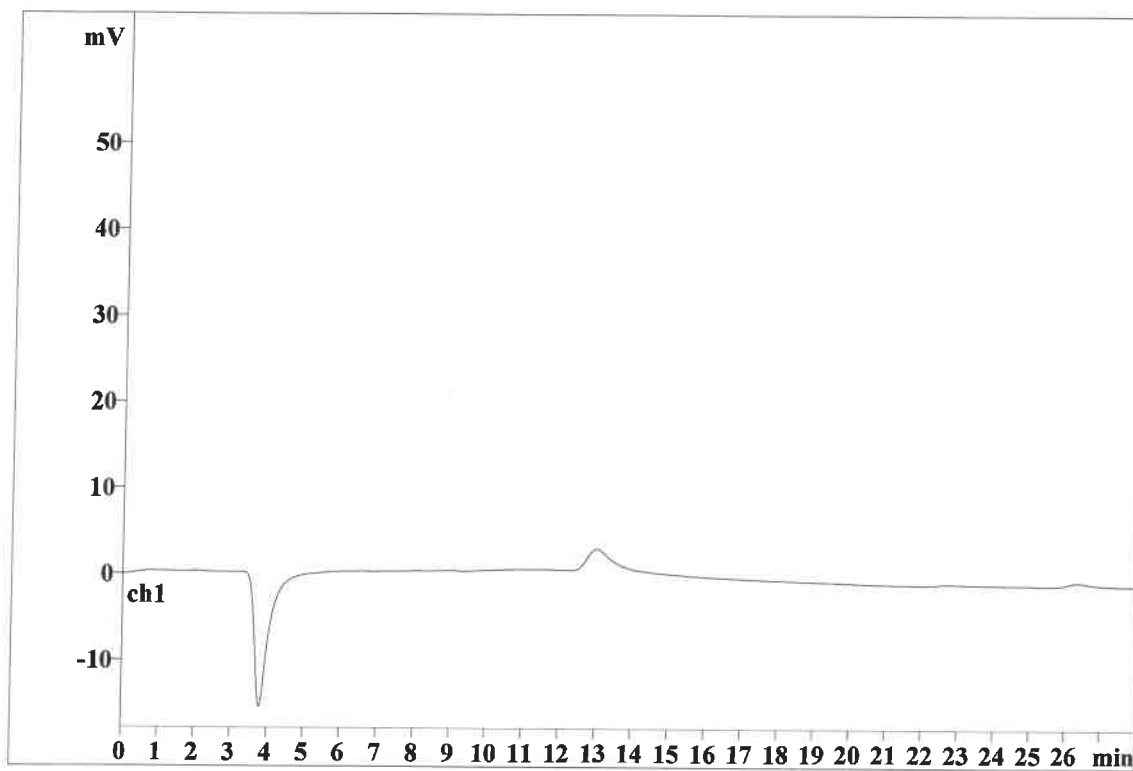

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 2/8/2023 1:37:48 PM
Printed by: wet


Ident: LB123983BSW
Analysis from: 2/7/2023 12:00:41 PM
File: _2023-02-07_

Last save: 2/8/2023 1:34:37 PM

Method: AnionsIC2-011923.mtw
Run operator: wet
Analysis number: 33225

Last save: 2/1/2023 10:37:

SAMPLE:
: IZ/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

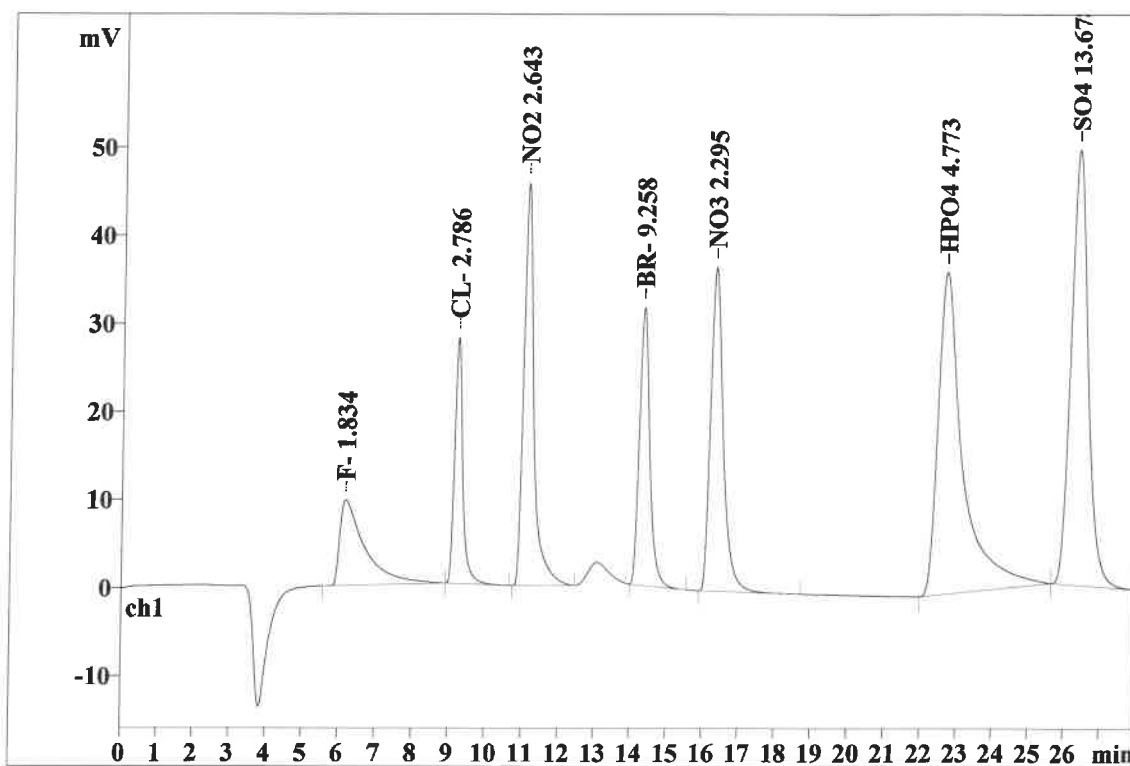

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.17	0.627	9.69	4.08	457.645	6.84
2	9.21	0.218	27.99	11.78	426.573	6.37
3	11.08	0.268	45.68	19.22	885.949	13.24
4	14.31	0.296	31.52	13.26	626.660	9.36
5	16.29	0.359	36.79	15.48	896.638	13.40
6	22.65	0.615	36.57	15.38	1753.501	26.20
7	26.32	0.504	49.45	20.80	1645.874	24.59
7	28.00	0.412	237.69	100.00	6692.840	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/8/2023 1:38:17 PM
Printed by: wet


Ident: 01468-01
Analysis from: 2/7/2023 12:58:49 PM
File: _2023-02-07_

Last save: 2/8/2023 1:38:16 PM

Method: AnionsIC2-011923.mtw
Run operator: wet
Analysis number: 33226

Last save: 2/1/2023 10:37:

SAMPLE:
: IZ/MA
Vial number: 28
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

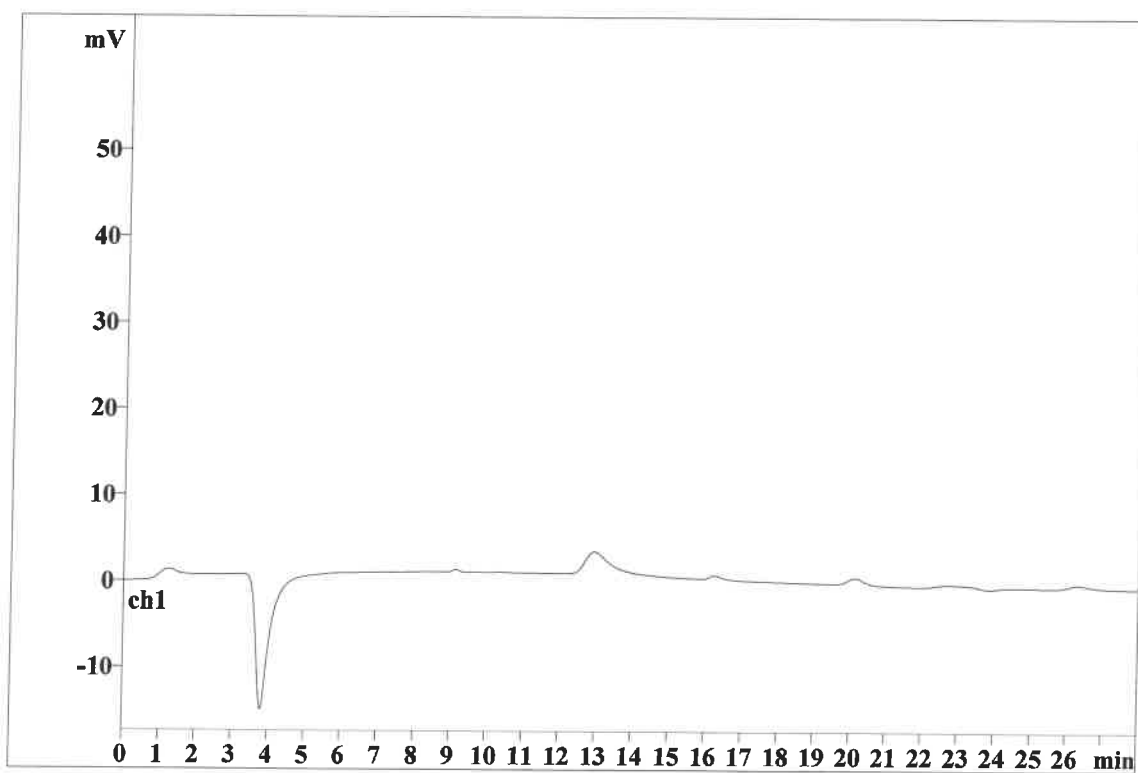

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 2/8/2023 1:38:23 PM
Printed by: wet


Ident: 01468-01MS
Analysis from: 2/7/2023 1:29:27 PM
File: _2023-02-07_

Last save: 2/7/2023 1:57:27 PM

Method: AnionsIC2-011923.mtw
Run operator: wet
Analysis number: 33227

Last save: 2/1/2023 10:37:

SAMPLE:
: IZ/MA
Vial number: 29
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

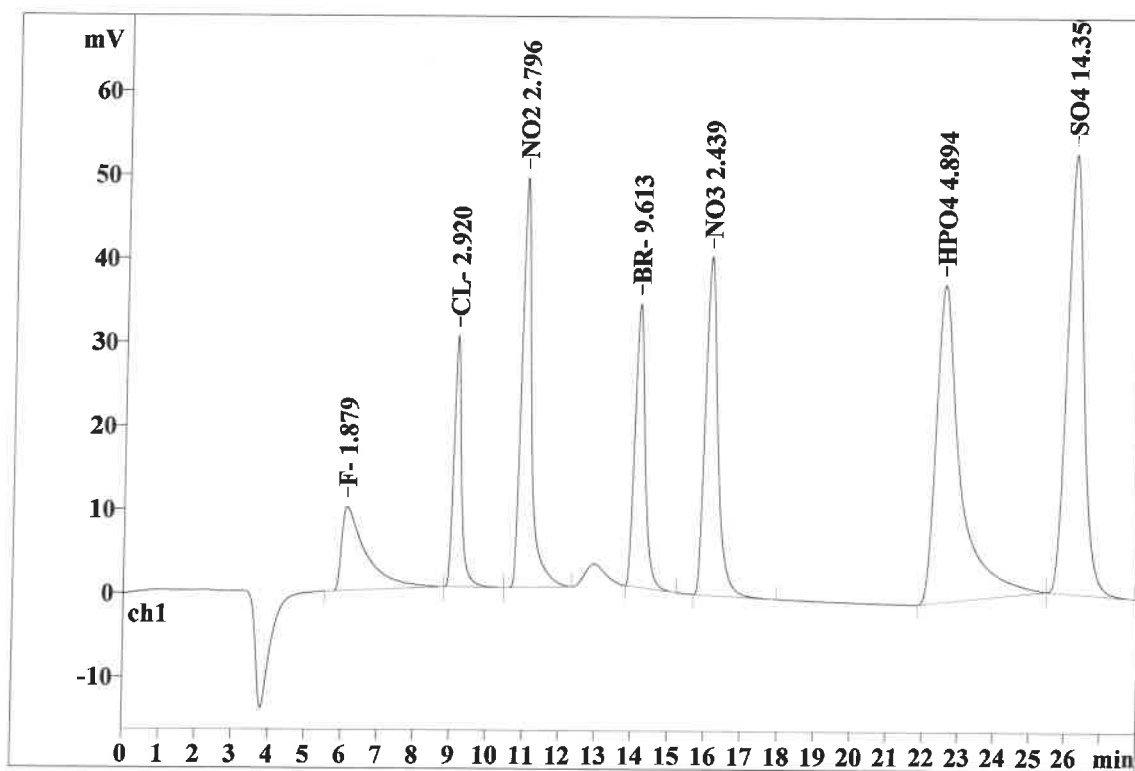

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.10	0.617	10.03	3.95	470.185	6.71
2	9.10	0.214	30.03	11.84	448.408	6.40
3	10.95	0.266	48.92	19.28	942.874	13.46
4	14.11	0.288	33.84	13.34	652.853	9.32
5	16.04	0.349	40.43	15.94	957.430	13.66
6	22.50	0.608	37.93	14.95	1802.684	25.73
7	26.15	0.498	52.54	20.71	1732.714	24.73
7	28.00	0.406	253.73	100.00	7007.148	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/8/2023 1:38:30 PM
Printed by: wet


Ident: 01468-01MSD
Analysis from: 2/7/2023 2:00:04 PM
File: _2023-02-07_

Last save: 2/7/2023 2:28:04 PM

Method: AnionsIC2-011923.mtw
Run operator: wet
Analysis number: 33228

Last save: 2/1/2023 10:37:

SAMPLE:
: IZ/MA
Vial number: 30
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

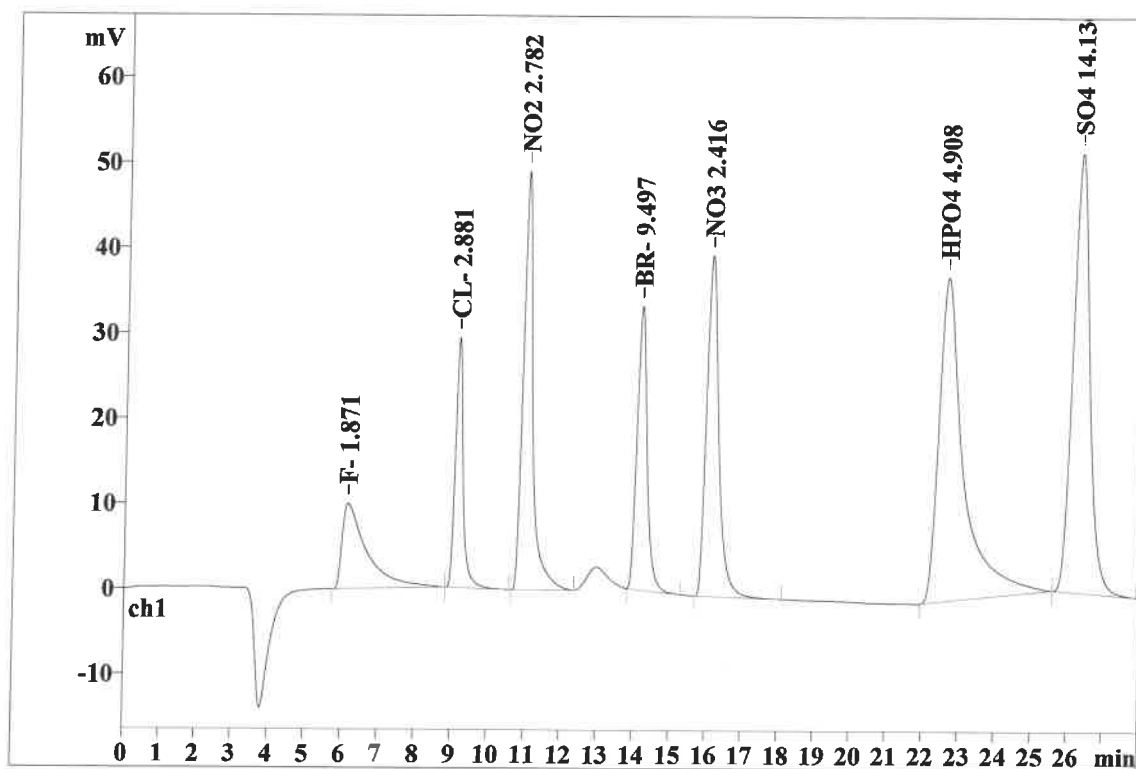

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.14	0.621	10.00	3.98	467.909	6.73
2	9.13	0.215	29.39	11.69	442.137	6.36
3	10.97	0.264	49.12	19.54	937.368	13.48
4	14.14	0.288	33.32	13.25	644.307	9.27
5	16.06	0.349	40.00	15.91	947.775	13.63
6	22.59	0.608	38.01	15.12	1808.138	26.01
7	26.26	0.500	51.56	20.51	1705.062	24.52
7	28.00	0.406	251.40	100.00	6952.696	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/8/2023 1:38:37 PM
Printed by: wet


Ident: CCV
Analysis from: 2/7/2023 2:30:45 PM
File: _2023-02-07_

Last save: 2/7/2023 3:28:27 PM

Method: AnionsIC2-011923.mtw
Run operator: wet
Analysis number: 33229

Last save: 2/1/2023 10:37:

SAMPLE:
: IZ/MA
Vial number: 23
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

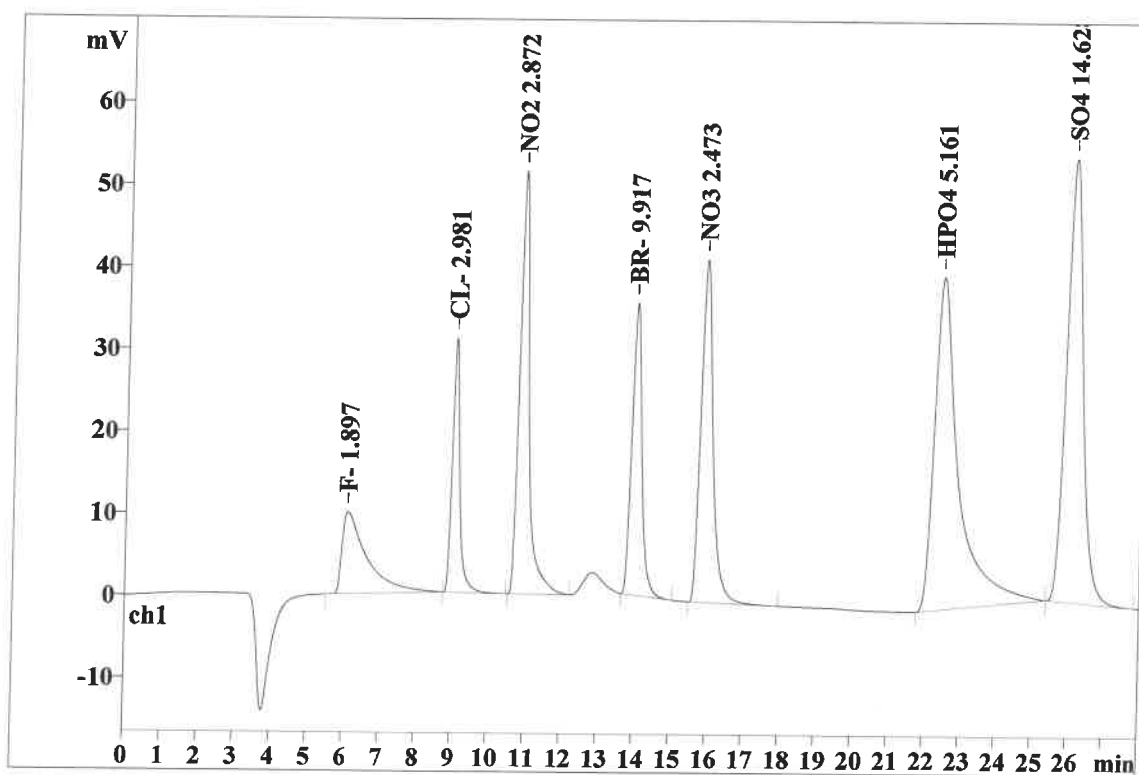

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.09	0.636	9.96	3.77	474.940	6.57
2	9.04	0.212	30.92	11.71	458.410	6.34
3	10.86	0.261	51.45	19.49	970.794	13.43
4	13.98	0.283	35.55	13.47	675.270	9.34
5	15.88	0.343	41.67	15.79	971.475	13.44
6	22.43	0.604	40.47	15.33	1910.397	26.42
7	26.07	0.496	53.95	20.44	1768.665	24.46
7	28.00	0.405	263.99	100.00	7229.952	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/8/2023 1:38:45 PM
Printed by: wet


Ident: CCB
Analysis from: 2/7/2023 3:01:27 PM
File: _2023-02-07_

Last save: 2/7/2023 3:29:28 PM

Method: AnionsIC2-011923.mtw
Run operator: wet
Analysis number: 33230

Last save: 2/1/2023 10:37:

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

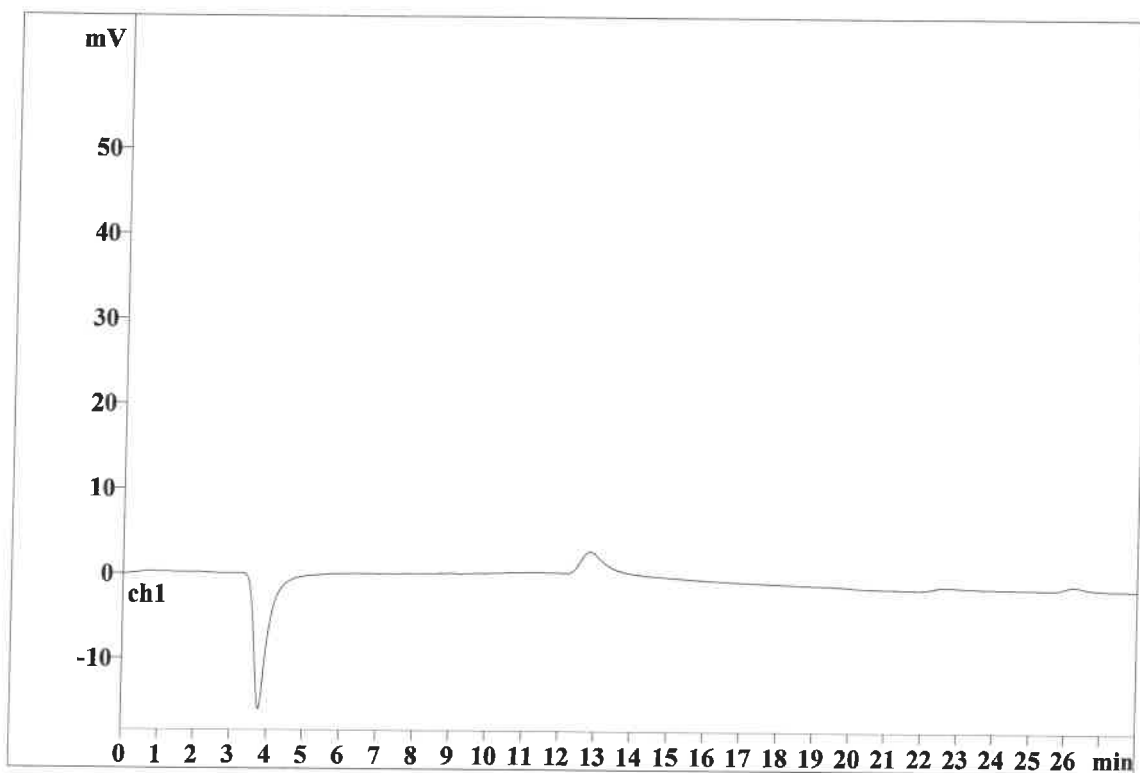

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD