


LB124015

7471B INSTRUMENT ID: CVA

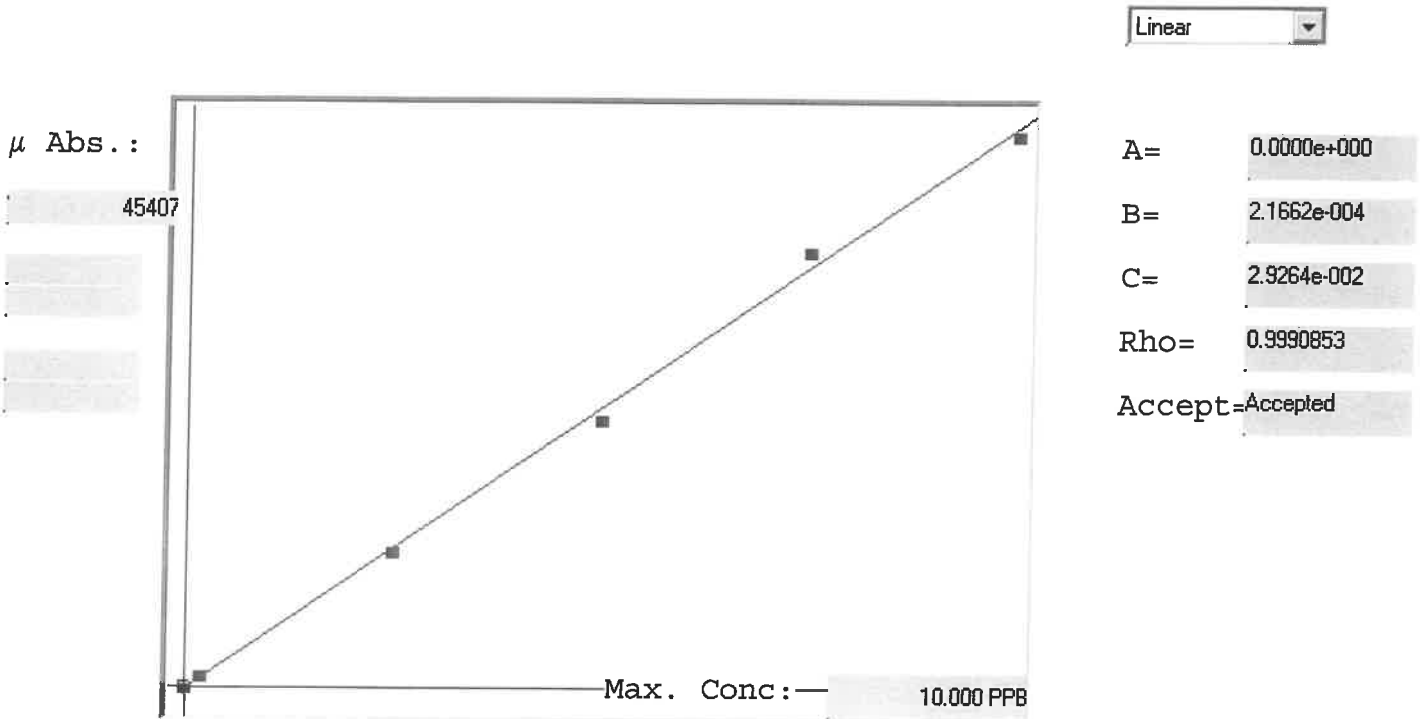

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0100
0.0	0.000	0.035	0.035	27	0.000	27					-
0.2	0.200	0.238	0.038	964	0.0 %	964					19
2.5	2.500	2.448	-0.052	11166	0.0 %	11166					-2
5.0	5.000	4.812	-0.188	22081	0.0 %	22081					-4
7.5	7.500	7.801	0.301	35878	0.0 %	35878					-4
10.0	10.000	9.865	-0.135	45407	0.0 %	45407					-1

LB124015 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 10 Feb 2023 11:30:03

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	27	-	0.0000	7471B	PPB	10 Feb 2023 11:31:04	S	Std
0.2 - 1	52.2	964	-	0.2000	7471B	PPB	10 Feb 2023 11:33:21	S	Std
2.5 - 1	52.5	11166	-	2.5000	7471B	PPB	10 Feb 2023 11:35:39	S	Std
5.0 - 1	55	22081	-	5.0000	7471B	PPB	10 Feb 2023 11:37:56	S	Std
7.5 - 1	57.5	35878	-	7.5000	7471B	PPB	10 Feb 2023 11:40:16	S	Std
10.0 - 1	510	45407	-	10.0000	7471B	PPB	10 Feb 2023 11:42:32	S	Std
ICV41 - 1	ICV41	18220	3.9761	-	7471B	PPB	10 Feb 2023 11:47:58	U	SMPL
ICB41 - 1	ICB41	68	0.0440	-	7471B	PPB	10 Feb 2023 11:50:13	U	SMPL
CCV12 - 1	CCV12	22120	4.8209	-	7471B	PPB	10 Feb 2023 11:52:29	U	SMPL
CCB12 - 1	CCB12	48	0.0397	-	7471B	PPB	10 Feb 2023 11:54:44	U	SMPL
CRA - 1	CRA	946	0.2342	-	7471B	PPB	10 Feb 2023 11:57:00	U	SMPL
HighStd - 1	HighStd	45271	9.8358	-	7471B	PPB	10 Feb 2023 11:59:15	U	SMPL
ChkStd - 1	ChkStd	33236	7.2288	-	7471B	PPB	10 Feb 2023 12:01:31	U	SMPL
PB150761BL - 1	PBS	3	0.0299	-	7471B	PPB	10 Feb 2023 12:03:47	U	SMPL
PB150761BS - 1	LCSS	17634	3.8491	-	7471B	PPB	10 Feb 2023 12:06:03	U	SMPL
O1504-01 - 1	COMP-1	1588	0.3733	-	7471B	PPB	10 Feb 2023 12:08:19	U	SMPL
O1504-01DUP - 1	COMP-1DUP	1400	0.3325	-	7471B	PPB	10 Feb 2023 12:10:36	U	SMPL
O1504-01MS - 1	COMP-1MS	20069	4.3766	-	7471B	PPB	10 Feb 2023 12:12:53	U	SMPL
O1504-01MSD - 1	COMP-1MSD	18817	4.1054	-	7471B	PPB	10 Feb 2023 12:15:11	U	SMPL
O1510-03 - 1	TWM-TP14-020823	14172	3.0992	-	7471B	PPB	10 Feb 2023 12:17:26	U	SMPL
CCV13 - 1	CCV13	21872	4.7671	-	7471B	PPB	10 Feb 2023 12:19:42	U	SMPL
CCB13 - 1	CCB13	-1	0.0290	-	7471B	PPB	10 Feb 2023 12:21:57	U	SMPL
O1510-07 - 1	JPP-51B-020823	35515	7.7225	-	7471B	PPB	10 Feb 2023 12:24:12	U	SMPL
O1510-11 - 1	JPP-55-020823	32331	7.0328	-	7471B	PPB	10 Feb 2023 12:26:27	U	SMPL
O1510-15 - 1	JPP-59-020823	75020	16.2800	-	7471B	PPB	10 Feb 2023 12:28:43	U	SMPL
O1513-02 - 1	VNJ-208	1706	0.3988	-	7471B	PPB	10 Feb 2023 12:30:59	U	SMPL
O1504-01LX5 - 1		304	0.0951	-	7471B	PPB	10 Feb 2023 12:33:18	U	SMPL
O1504-01A - 1		8055	1.7741	-	7471B	PPB	10 Feb 2023 12:35:35	U	SMPL
O1510-15DX5 - 1		15622	3.4133	-	7471B	PPB	10 Feb 2023 12:37:52	U	SMPL
CCV14 - 1	CCV14	21841	4.7604	-	7471B	PPB	10 Feb 2023 12:40:09	U	SMPL
CCB14 - 1	CCB14	-30	0.0228	-	7471B	PPB	10 Feb 2023 12:42:27	U	SMPL