

LIB124054

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

2/13/2023 13:01

Test: Phenolics-

Sample Id	^{m/L} Result	Dil. 1 +	Response	Errors
ICV1	0.965	0.0	0.114	
ICB1	-0.009	0.0	0.011	
CCV1	0.974	0.0	0.115	
CCB1	-0.009	0.0	0.012	
PB150850BL	-0.008	0.0	0.012	
PB150820BS	0.963	0.0	0.114	
O1375-01	0.006	0.0	0.013	
O1375-01DUP	0.003	0.0	0.013	
O1375-01MS	1.028	0.0	0.121	
O1375-01MSD	1.036	0.0	0.121	
CCV2	0.967	0.0	0.114	
CCB2	-0.011	0.0	0.011	

N 12
Mean 0.492
SD 0.5194
CV% 105.54

Aquakem v. 7.2AQ1

Results from time period:

Mon Feb 13 12:12:58 2023

Mon Feb 13 12:55:45 2023

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	-0.0084	mg/l	2/13/2023 12:12:58	
0.05PPM	A	Phenolics-	P	0.0502	mg/l	2/13/2023 12:12:59	
0.1PPM	A	Phenolics-	P	0.1032	mg/l	2/13/2023 12:13:00	
0.25PPM	A	Phenolics-	P	0.2506	mg/l	2/13/2023 12:13:01	
0.50PPM	A	Phenolics-	P	0.4897	mg/l	2/13/2023 12:13:02	
1.0PPM	A	Phenolics-	P	1.0247	mg/l	2/13/2023 12:13:03	
2.0PPM	A	Phenolics-	P	1.99	mg/l	2/13/2023 12:13:04	
ICV1	S	Phenolics-	P	0.9651	mg/l	2/13/2023 12:45:32	
ICB1	S	Phenolics-	P	-0.0094	mg/l	2/13/2023 12:45:34	
CCV1	S	Phenolics-	P	0.9745	mg/l	2/13/2023 12:45:36	
CCB1	S	Phenolics-	P	-0.0088	mg/l	2/13/2023 12:45:38	
PB150850BL	S	Phenolics-	P	-0.0081	mg/l	2/13/2023 12:45:40	
PB150820BS	S	Phenolics-	P	0.963	mg/l	2/13/2023 12:45:43	
O1375-01	S	Phenolics-	P	0.0064	mg/l	2/13/2023 12:55:34	
O1375-01DUP	S	Phenolics-	P	0.0033	mg/l	2/13/2023 12:55:36	
O1375-01MS	S	Phenolics-	P	1.0282	mg/l	2/13/2023 12:55:39	
O1375-01MSD	S	Phenolics-	P	1.0356	mg/l	2/13/2023 12:55:40	
CCV2	S	Phenolics-	P	0.9668	mg/l	2/13/2023 12:55:42	
CCB2	S	Phenolics-	P	-0.0114	mg/l	2/13/2023 12:55:45	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

2/13/2023 12:20


Test Phenolics-

Accepted 2/13/2023 12:20

Factor 9.508
Bias 0.012

Coeff. of det. 0.999716

Errors

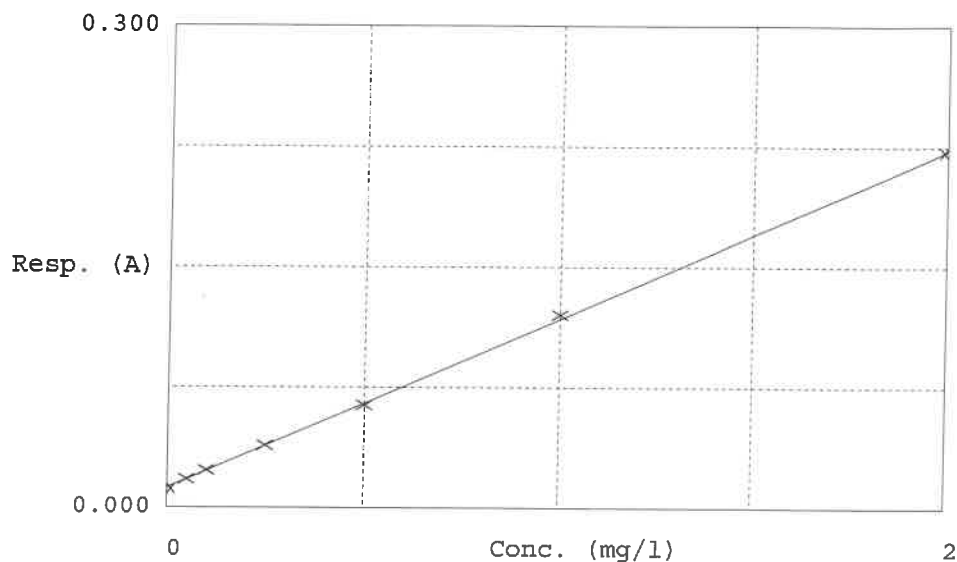

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.012	-0.0084	0.0000	-
2	Phenol-2	0.018	0.0502	0.0500	0.4
3	Phenol-2	0.023	0.1032	0.1000	3.2
4	Phenol-2	0.039	0.2506	0.2500	0.2
5	Phenol-2	0.064	0.4897	0.5000	-2.1
6	Phenol-2	0.120	1.0247	1.0000	2.5
7	Phenol-2	0.222	1.9900	2.0000	-0.5

12
2/13/23