

LB 12414p

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

2/20/2023 12:02

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.002	0.0	0.106	
ICB1	-0.007	0.0	0.011	
CCV1	0.923	0.0	0.099	
CCB1	-0.002	0.0	0.012	
PB150945BL	-0.005	0.0	0.011	
PB150945BS	1.005	0.0	0.106	
O1553-05	-0.229	0.0	-0.010	
O1553-05DUP	-0.317	0.0	-0.018	
O1553-05MS	0.109	0.0	0.022	
O1553-05MSD	0.103	0.0	0.022	
CCV2	0.921	0.0	0.098	
CCB2	-0.004	0.0	0.012	

N	12
Mean	0.291
SD	0.5109
CV%	175.26

Aquakem v. 7.2AQ1

Results from time period:

Mon Feb 20 10:26:28 2023

Mon Feb 20 12:00:31 2023

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	-0.006	mg/l	2/20/2023 10:26:28	
0.05PPM	A	Phenolics-	P	0.048	mg/l	2/20/2023 10:26:29	
0.1PPM	A	Phenolics-	P	0.1019	mg/l	2/20/2023 10:26:30	
0.25PPM	A	Phenolics-	P	0.2563	mg/l	2/20/2023 10:26:31	
0.50PPM	A	Phenolics-	P	0.4973	mg/l	2/20/2023 10:26:32	
1.0PPM	A	Phenolics-	P	1.0055	mg/l	2/20/2023 10:26:33	
2.0PPM	A	Phenolics-	P	1.9971	mg/l	2/20/2023 10:26:34	
ICV1	S	Phenolics-	P	1.0023	mg/l	2/20/2023 11:30:04	
ICB1	S	Phenolics-	P	-0.007	mg/l	2/20/2023 11:30:06	
CCV1	S	Phenolics-	P	0.9229	mg/l	2/20/2023 11:30:08	
CCB1	S	Phenolics-	P	-0.0024	mg/l	2/20/2023 11:30:10	
PB150945BL	S	Phenolics-	P	-0.0052	mg/l	2/20/2023 11:30:12	
PB150945BS	S	Phenolics-	P	1.0052	mg/l	2/20/2023 11:30:15	
O1553-05	S	Phenolics-	P	-0.2293	mg/l	2/20/2023 11:40:07	
O1553-05DUP	S	Phenolics-	P	-0.3168	mg/l	2/20/2023 11:40:09	
O1553-05MS	S	Phenolics-	P	0.1085	mg/l	2/20/2023 11:40:10	
O1553-05MSD	S	Phenolics-	P	0.1031	mg/l	2/20/2023 11:40:11	
CCV2	S	Phenolics-	P	0.921	mg/l	2/20/2023 11:40:14	
CCB2	S	Phenolics-	P	-0.0043	mg/l	2/20/2023 11:40:16	

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

2/20/2023 10:44

Test Phenolics-


Accepted 2/20/2023 10:44

Factor 10.66

Bias 0.012

Coeff. of det. 0.999959

Errors

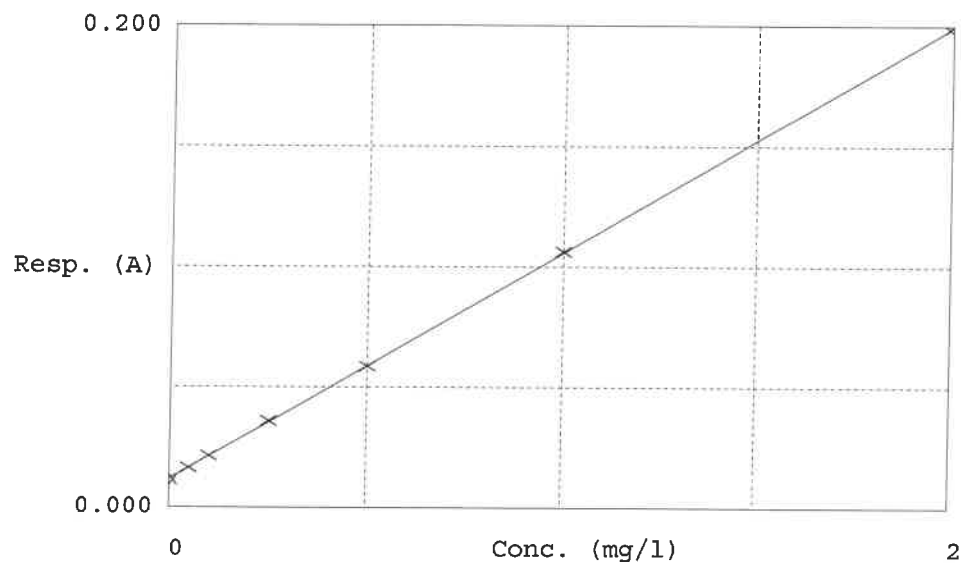

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.011	-0.0060	0.0000	
2	Phenol-2	0.016	0.0480	0.0500	-4.0
3	Phenol-2	0.021	0.1019	0.1000	1.9
4	Phenol-2	0.036	0.2563	0.2500	2.5
5	Phenol-2	0.059	0.4973	0.5000	-0.5
6	Phenol-2	0.106	1.0055	1.0000	0.6
7	Phenol-2	0.199	1.9971	2.0000	-0.1

12
2/20/23