

L11324346

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

3/2/2023 14:11

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.092	0.0	0.104	
ICB1	0.006	0.0	0.012	
CCV1	1.014	0.0	0.098	
CCB1	0.008	0.0	0.012	
PB151170BL	0.009	0.0	0.012	
PB151170BS	1.086	0.0	0.104	
O1627-10	0.033	0.0	0.014	
O1627-11	0.057	0.0	0.016	
O1759-01	0.072	0.0	0.017	
O1759-01DUP	0.096	0.0	0.019	
O1759-01MS	1.223	0.0	0.115	
O1759-01MSD	1.203	0.0	0.114	
O1759-03	0.049	0.0	0.015	
CCV2	1.033	0.0	0.099	
CCB2	0.008	0.0	0.012	

N 15
Mean 0.466
SD 0.5463
CV% 117.21

Aquakem v. 7.2AQ1

Results from time period:

Thu Mar 02 11:37:08 2023

Thu Mar 02 14:00:28 2023

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0025	mg/l	3/2/2023 11:37:08	
0.05PPM	A	Phenolics-	P	0.0604	mg/l	3/2/2023 11:37:09	
0.1PPM	A	Phenolics-	P	0.1092	mg/l	3/2/2023 11:37:10	
0.25PPM	A	Phenolics-	P	0.2476	mg/l	3/2/2023 11:37:11	
0.50PPM	A	Phenolics-	P	0.4973	mg/l	3/2/2023 11:37:12	
1.0PPM	A	Phenolics-	P	0.9655	mg/l	3/2/2023 11:37:13	
2.0PPM	A	Phenolics-	P	2.0175	mg/l	3/2/2023 11:37:14	
ICV1	S	Phenolics-	P	1.0921	mg/l	3/2/2023 13:25:54	
ICB1	S	Phenolics-	P	0.0062	mg/l	3/2/2023 13:25:55	
CCV1	S	Phenolics-	P	1.0144	mg/l	3/2/2023 13:25:57	
CCB1	S	Phenolics-	P	0.008	mg/l	3/2/2023 13:25:59	
PB151170BL	S	Phenolics-	P	0.0086	mg/l	3/2/2023 13:26:01	
PB151170BS	S	Phenolics-	P	1.0863	mg/l	3/2/2023 13:26:04	
O1627-10	S	Phenolics-	P	0.0326	mg/l	3/2/2023 14:00:19	
O1627-11	S	Phenolics-	P	0.0571	mg/l	3/2/2023 14:00:20	
O1759-01	S	Phenolics-	P	0.0719	mg/l	3/2/2023 14:00:22	
O1759-01DUP	S	Phenolics-	P	0.0963	mg/l	3/2/2023 14:00:23	
O1759-01MS	S	Phenolics-	P	1.2234	mg/l	3/2/2023 14:00:24	
O1759-01MSD	S	Phenolics-	P	1.2034	mg/l	3/2/2023 14:00:25	
O1759-03	S	Phenolics-	P	0.049	mg/l	3/2/2023 14:00:26	
CCV2	S	Phenolics-	P	1.0332	mg/l	3/2/2023 14:00:27	
CCB2	S	Phenolics-	P	0.0082	mg/l	3/2/2023 14:00:28	

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

3/2/2023 11:39


Test Phenolics-

Accepted 3/2/2023 11:39

Factor 11.73
Bias 0.011

Coeff. of det. 0.999459

Errors

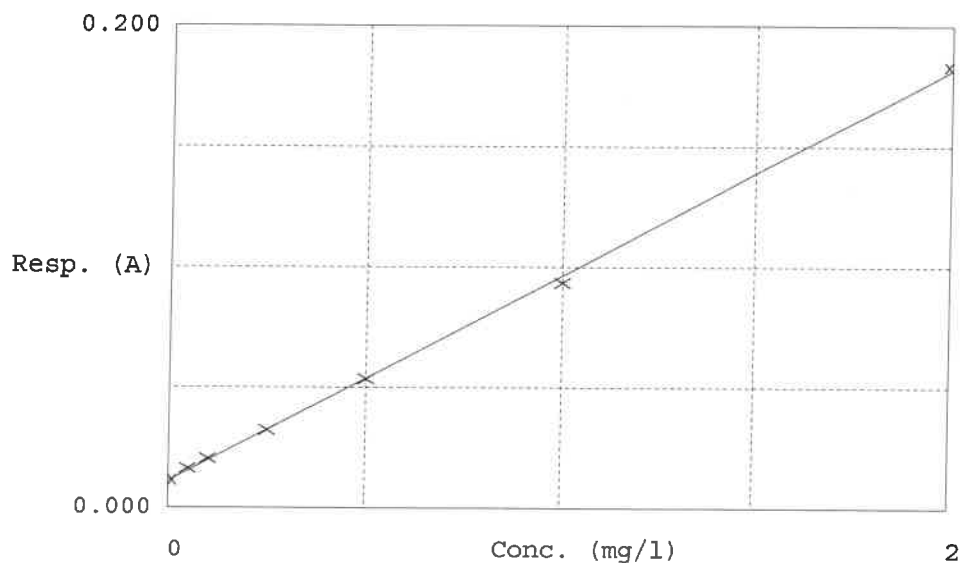

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.011	0.0025	0.0000	-
2	Phenol-2	0.016	0.0604	0.0500	20.8
3	Phenol-2	0.020	0.1092	0.1000	9.2
4	Phenol-2	0.032	0.2476	0.2500	-1.0
5	Phenol-2	0.054	0.4973	0.5000	-0.5
6	Phenol-2	0.093	0.9655	1.0000	-3.5
7	Phenol-2	0.183	2.0175	2.0000	0.9

12
3/2/23