

LB124421


7470A

INSTRUMENT ID: EV2

Linear

 μ Abs.:

44581

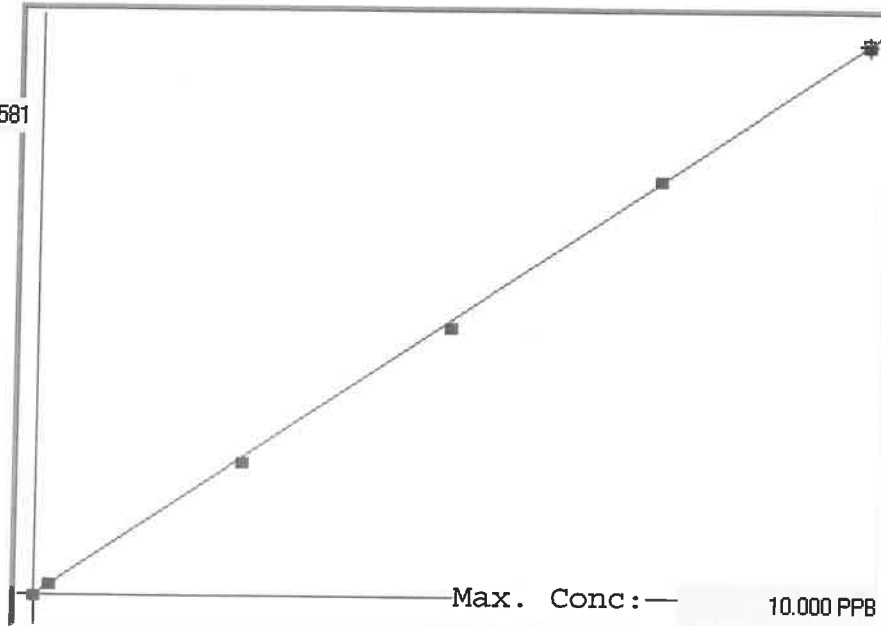

A= 0.0000e+000

B= 2.2427e-004

C= 8.3161e-003

Rho= 0.9998756

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.032	0.032	106	0.000	106					
0.2	0.200	0.240	0.040	1031	0.0 %	1031					20
2.5	2.500	2.452	-0.048	10898	0.0 %	10898					2
5.0	5.000	4.898	-0.102	21803	0.0 %	21803					2
7.5	7.500	7.571	0.071	33721	0.0 %	33721					1
10.0	10.000	10.007	0.007	44581	0.0 %	44581					0

LB124421 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 09 Mar 2023 10:26:24

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	56	106	-	0.0000	7470A	PPB	09 Mar 2023 10:37:48	S	Std
0.2 - 1	56.2	1031	-	0.2000	7470A	PPB	09 Mar 2023 10:40:06	S	Std
2.5 - 1	52.5	10898	-	2.5000	7470A	PPB	09 Mar 2023 10:42:24	S	Std
5.0 - 1	53	21803	-	5.0000	7470A	PPB	09 Mar 2023 10:44:41	S	Std
7.5 - 1	57.5	33721	-	7.5000	7470A	PPB	09 Mar 2023 10:49:35	S	Std
10.0 - 1	57.8	44581	-	10.0000	7470A	PPB	09 Mar 2023 10:51:52	S	Std
ICV76 - 1	ICV76	17493	3.9315	-	7470A	PPB	09 Mar 2023 10:54:52	U	SMPL
ICB76 - 1	ICB76	-40	-0.0007	-	7470A	PPB	09 Mar 2023 10:57:07	U	SMPL
CCV43 - 1	CCV43	21817	4.9013	-	7470A	PPB	09 Mar 2023 11:01:11	U	SMPL
CCB43 - 1	CCB43	-48	-0.0024	-	7470A	PPB	09 Mar 2023 11:03:26	U	SMPL
CRA - 1	CRA	980	0.2281	-	7470A	PPB	09 Mar 2023 11:05:41	U	SMPL
HighStd - 1	HighStd	43886	9.8508	-	7470A	PPB	09 Mar 2023 11:07:55	U	SMPL
ChkStd - 1	ChkStd	32511	7.2997	-	7470A	PPB	09 Mar 2023 11:10:11	U	SMPL
PB151320BL - 1	PBW	-88	-0.0114	-	7470A	PPB	09 Mar 2023 11:12:28	U	SMPL
PB151320BS - 1	LCSW	15039	3.3812	-	7470A	PPB	09 Mar 2023 11:14:45	U	SMPL
O1833-02 - 1	46	-28	0.0020	-	7470A	PPB	09 Mar 2023 11:17:02	U	SMPL
O1833-05 - 1	42	23	0.0135	-	7470A	PPB	09 Mar 2023 11:19:18	U	SMPL
O1833-08 - 1	11	21	0.0130	-	7470A	PPB	09 Mar 2023 11:21:35	U	SMPL
O1833-08DUP - 1	11DUP	32	0.0155	-	7470A	PPB	09 Mar 2023 11:23:52	U	SMPL
O1833-08MS - 1	11MS	16934	3.8062	-	7470A	PPB	09 Mar 2023 11:26:08	U	SMPL
CCV44 - 1	CCV44	21463	4.8219	-	7470A	PPB	09 Mar 2023 11:28:23	U	SMPL
CCB44 - 1	CCB44	-34	0.0007	-	7470A	PPB	09 Mar 2023 11:30:39	U	SMPL
O1833-08MSD - 1	11MSD	16873	3.7925	-	7470A	PPB	09 Mar 2023 11:32:55	U	SMPL
PB151294TB - 1	PB151294TB	-38	-0.0002	-	7470A	PPB	09 Mar 2023 11:35:10	U	SMPL
O1833-08LX5 - 1		-7	0.0067	-	7470A	PPB	09 Mar 2023 11:37:26	U	SMPL
O1833-08A - 1		17984	4.0417	-	7470A	PPB	09 Mar 2023 11:39:42	U	SMPL
CCV45 - 1	CCV45	21722	4.8800	-	7470A	PPB	09 Mar 2023 11:41:58	U	SMPL
CCB45 - 1	CCB45	-32	0.0011	-	7470A	PPB	09 Mar 2023 11:44:15	U	SMPL