


LB124424

7471B

INSTRUMENT ID: CV4

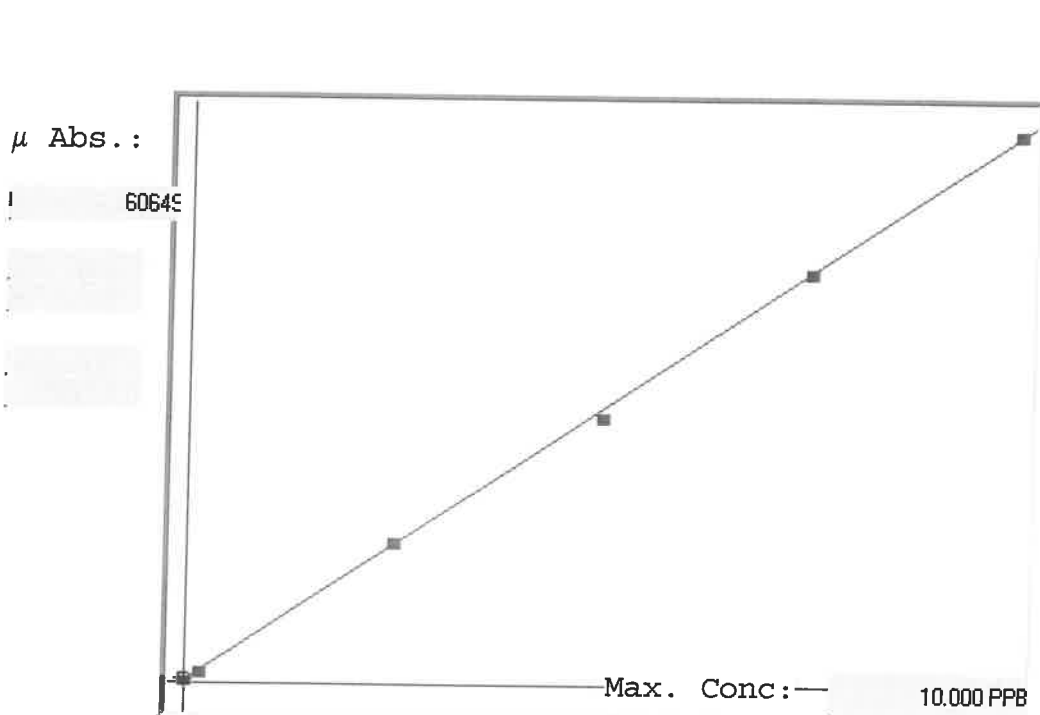

Linear

A= 0.0000e+000

B= 1.6611e-004

C= -3.6662e-002

Rho= 0.9998291

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.043	0.043	480	0.000	480					1
0.2	0.200	0.185	-0.015	1336	0.0 %	1336					1
2.5	2.500	2.554	0.054	15594	0.0 %	15594					2
5.0	5.000	4.855	-0.145	29451	0.0 %	29451					1
7.5	7.500	7.525	0.025	45525	0.0 %	45525					3
10.0	10.000	10.037	0.037	60649	0.0 %	60649					0

LB124424 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 09 Mar 2023 13:08:13

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	480	-	0.0000	7471B	PPB	09 Mar 2023 13:11:26	S	Std
0.2 - 1	50.2	1336	-	0.2000	7471B	PPB	09 Mar 2023 13:13:44	S	Std
2.5 - 1	52.5	15594	-	2.5000	7471B	PPB	09 Mar 2023 13:16:01	S	Std
5.0 - 1	55	29451	-	5.0000	7471B	PPB	09 Mar 2023 13:18:18	S	Std
7.5 - 1	57.5	45525	-	7.5000	7471B	PPB	09 Mar 2023 13:20:35	S	Std
10.0 - 1	58	60649	-	10.0000	7471B	PPB	09 Mar 2023 13:25:32	S	Std
ICV77 - 1	ICV77	24927	4.1039	-	7471B	PPB	09 Mar 2023 13:28:14	U	SMPL
ICB77 - 1	ICB77	-26	-0.0410	-	7471B	PPB	09 Mar 2023 13:30:29	U	SMPL
CCV46 - 1	CCV46	32898	5.4279	-	7471B	PPB	09 Mar 2023 13:32:45	U	SMPL
CCB46 - 1	CCB46	4	-0.0360	-	7471B	PPB	09 Mar 2023 13:35:01	U	SMPL
CRA - 1	CRA	1241	0.1695	-	7471B	PPB	09 Mar 2023 13:37:17	U	SMPL
HighStd - 1	HighStd	60348	9.9875	-	7471B	PPB	09 Mar 2023 13:39:32	U	SMPL
ChkStd - 1	ChkStd	41779	6.9031	-	7471B	PPB	09 Mar 2023 13:41:47	U	SMPL
PB151325BL - 1	PB151325BL	-142	-0.0602	-	7471B	PPB	09 Mar 2023 13:44:05	U	SMPL
PB151325BS - 1	PB151325BS	19621	3.2225	-	7471B	PPB	09 Mar 2023 13:46:22	U	SMPL
O1842-01 - 1	VNJ-228	9196	1.4908	-	7471B	PPB	09 Mar 2023 13:48:39	U	SMPL
O1842-01DUP - 1	VNJ-228DUP	9161	1.4850	-	7471B	PPB	09 Mar 2023 13:50:56	U	SMPL
O1842-01MS - 1	VNJ-228MS	32510	5.3634	-	7471B	PPB	09 Mar 2023 13:53:13	U	SMPL
O1842-01MSD - 1	VNJ-228MSD	29979	4.9430	-	7471B	PPB	09 Mar 2023 13:55:30	U	SMPL
O1846-02 - 1	TP-3	131660	21.8328	-	7471B	PPB	09 Mar 2023 13:57:47	U	SMPL
CCV47 - 1	CCV47	31994	5.2777	-	7471B	PPB	09 Mar 2023 14:00:04	U	SMPL
CCB47 - 1	CCB47	-124	-0.0573	-	7471B	PPB	09 Mar 2023 14:02:22	U	SMPL
O1846-04 - 1	TP-4	4219	0.6641	-	7471B	PPB	09 Mar 2023 14:04:38	U	SMPL
O1847-01 - 1	TR-05-030823	3445	0.5356	-	7471B	PPB	09 Mar 2023 14:06:53	U	SMPL
O1848-01 - 1	OR-02-03082023	2643	0.4024	-	7471B	PPB	09 Mar 2023 14:09:09	U	SMPL
O1842-01LX5 - 1		1736	0.2517	-	7471B	PPB	09 Mar 2023 14:15:01	U	SMPL
O1842-01A - 1		31718	5.2319	-	7471B	PPB	09 Mar 2023 14:17:16	U	SMPL
O1833-07 - 1	11	3659	0.5711	-	7471B	PPB	09 Mar 2023 14:19:33	U	SMPL
O1833-07DUP - 1	11DUP	3700	0.5779	-	7471B	PPB	09 Mar 2023 14:21:50	U	SMPL
O1833-07MS - 1	11MS	28122	4.6346	-	7471B	PPB	09 Mar 2023 14:24:07	U	SMPL
O1833-07MSD - 1	11MSD	28216	4.6502	-	7471B	PPB	09 Mar 2023 14:26:24	U	SMPL
O1846-02DLX5 - 1		23407	3.8514	-	7471B	PPB	09 Mar 2023 14:28:40	U	SMPL
CCV48 - 1	CCV48	30088	4.9611	-	7471B	PPB	09 Mar 2023 14:30:57	U	SMPL
CCB48 - 1	CCB48	-86	-0.0509	-	7471B	PPB	09 Mar 2023 14:33:13	U	SMPL
O1833-07LX5 - 1		635	0.0688	-	7471B	PPB	09 Mar 2023 14:35:30	U	SMPL
O1833-07A - 1		28092	4.6296	-	7471B	PPB	09 Mar 2023 14:37:46	U	SMPL
O1829-01 - 1	SS-01-20230306	3916	0.6138	-	7471B	PPB	09 Mar 2023 14:40:01	U	SMPL
O1829-10 - 1	SS-10-20230306	4374	0.6899	-	7471B	PPB	09 Mar 2023 14:42:18	U	SMPL
O1829-10DUP - 1	SS-10-20230306DUP	4314	0.6799	-	7471B	PPB	09 Mar 2023 14:44:34	U	SMPL
O1829-11 - 1	O1829-10MS	26230	4.3203	-	7471B	PPB	09 Mar 2023 14:49:44	U	SMPL
O1829-12 - 1	O1829-10MSD	27139	4.4713	-	7471B	PPB	09 Mar 2023 14:52:01	U	SMPL
O1829-10LX5 - 1		780	0.0929	-	7471B	PPB	09 Mar 2023 14:54:19	U	SMPL
O1829-10A - 1		26553	4.3739	-	7471B	PPB	09 Mar 2023 14:56:37	U	SMPL
CCV49 - 1	CCV49	29801	4.9135	-	7471B	PPB	09 Mar 2023 14:58:53	U	SMPL
CCB49 - 1	CCB49	-86	-0.0509	-	7471B	PPB	09 Mar 2023 15:01:10	U	SMPL