

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

3/15/2023 14:26

Reviewed by : 12

Instrument ID : Konelab

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.072	0.0	0.086	
ICB1	0.003	0.0	0.008	
CCV1	1.068	0.0	0.086	
CCB1	-0.007	0.0	0.007	
PB151446BL	-0.007	0.0	0.007	
PB151446BS	1.063	0.0	0.086	
PB151447BL	-0.001	0.0	0.008	
PB151447BS	1.069	0.0	0.086	
O1627-09	0.026	0.0	0.010	
O1627-03	0.021	0.0	0.009	
CCV2	1.077	0.0	0.087	
CCB2	-0.005	0.0	0.007	

N	12
Mean	0.448
SD	0.5487
CV%	122.43

Aquakem v. 7.2AQ1

Results from time period:

Wed Mar 15 12:16:03 2023

Wed Mar 15 14:24:01 2023

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.001	mg/l	3/15/2023 12:37:45	
0.05PPM	A	Phenolics-	P	0.0523	mg/l	3/15/2023 12:37:46	
0.1PPM	A	Phenolics-	P	0.1038	mg/l	3/15/2023 12:37:47	
0.25PPM	A	Phenolics-	P	0.2512	mg/l	3/15/2023 12:37:48	
0.50PPM	A	Phenolics-	P	0.502	mg/l	3/15/2023 12:37:49	
1.0PPM	A	Phenolics-	P	0.9811	mg/l	3/15/2023 12:37:50	
2.0PPM	A	Phenolics-	P	2.0085	mg/l	3/15/2023 12:37:51	
ICV1	S	Phenolics-	P	1.0721	mg/l	3/15/2023 13:50:28	
ICB1	S	Phenolics-	P	0.0031	mg/l	3/15/2023 13:50:29	
CCV1	S	Phenolics-	P	1.0677	mg/l	3/15/2023 13:50:32	
CCB1	S	Phenolics-	P	-0.0065	mg/l	3/15/2023 13:50:33	
PB151446BL	S	Phenolics-	P	-0.007	mg/l	3/15/2023 13:50:35	
PB151446BS	S	Phenolics-	P	1.0633	mg/l	3/15/2023 13:50:38	
PB151447BL	S	Phenolics-	P	-0.0011	mg/l	3/15/2023 14:00:31	
PB151447BS	S	Phenolics-	P	1.0692	mg/l	3/15/2023 14:00:34	
O1627-09	S	Phenolics-	P	0.0259	mg/l	3/15/2023 14:23:57	
O1627-03	S	Phenolics-	P	0.0209	mg/l	3/15/2023 14:23:58	
CCV2	S	Phenolics-	P	1.0765	mg/l	3/15/2023 14:24:00	
CCB2	S	Phenolics-	P	-0.0053	mg/l	3/15/2023 14:24:01	

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

3/15/2023 12:57

Test Phenolics-


Accepted 3/15/2023 12:57

Factor 13.64

Bias 0.008

Coeff. of det. 0.999856

Errors

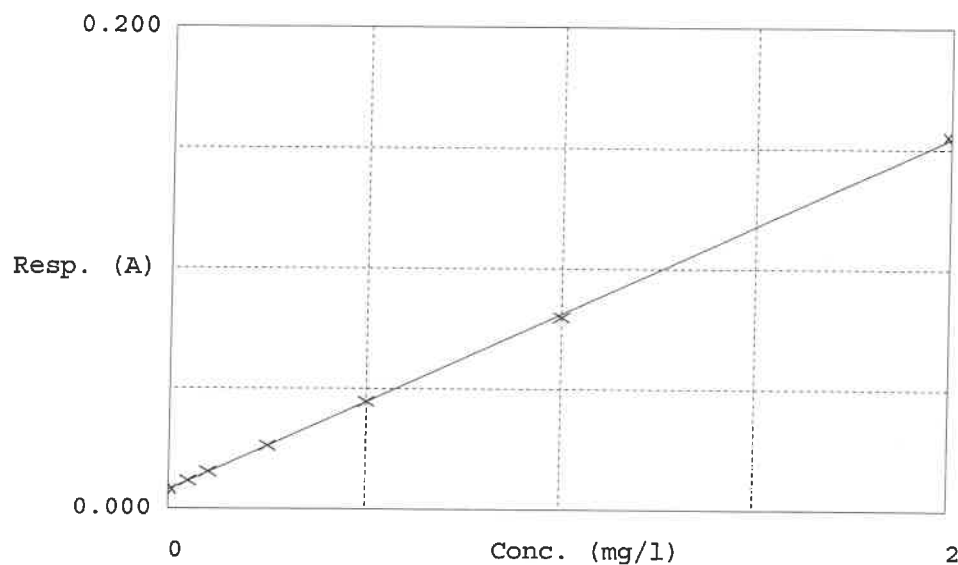

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.008	0.0010	0.0000	-
2	Phenol-2	0.012	0.0523	0.0500	4.6
3	Phenol-2	0.015	0.1038	0.1000	3.8
4	Phenol-2	0.026	0.2512	0.2500	0.5
5	Phenol-2	0.045	0.5020	0.5000	0.4
6	Phenol-2	0.080	0.9811	1.0000	-1.8
7	Phenol-2	0.155	2.0085	2.0000	0.4

12
3/15/23