

213124579

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

3/16/2023 11:12

Reviewed by : 12

Instrument ID : Konelab

Test: Phenolics-

Sample Id	<i>mpl</i> Result	Dil. 1 +	Response	Errors
ICV1	1.029	0.0	0.081	
ICB1	0.003	0.0	0.007	
CCV1	1.022	0.0	0.081	
CCB1	0.004	0.0	0.007	
PB151436BL	0.004	0.0	0.007	
PB151436BS	1.024	0.0	0.081	
O1627-12	0.030	0.0	0.009	
O1923-01	-0.022	0.0	0.005	
O1923-01DUP	-0.025	0.0	0.005	
O1923-01MS	0.992	0.0	0.079	
O1923-01MSD	0.981	0.0	0.078	
CCV2	1.037	0.0	0.082	
CCB2	0.001	0.0	0.007	

N 13
Mean 0.468
SD 0.5270
CV% 112.68

Aquakem v. 7.2AQ1

Results from time period:

Thu Mar 16 10:04:13 2023

Thu Mar 16 11:11:12 2023

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0024	mg/l	3/16/2023 10:04:13	
0.05PPM	A	Phenolics-	P	0.0563	mg/l	3/16/2023 10:04:14	
0.1PPM	A	Phenolics-	P	0.1029	mg/l	3/16/2023 10:04:15	
0.25PPM	A	Phenolics-	P	0.2493	mg/l	3/16/2023 10:04:16	
0.50PPM	A	Phenolics-	P	0.4988	mg/l	3/16/2023 10:04:17	
1.0PPM	A	Phenolics-	P	0.9807	mg/l	3/16/2023 10:04:18	
2.0PPM	A	Phenolics-	P	2.0097	mg/l	3/16/2023 10:04:19	
ICV1	S	Phenolics-	P	1.0287	mg/l	3/16/2023 10:39:43	
ICB1	S	Phenolics-	P	0.0029	mg/l	3/16/2023 10:39:44	
CCV1	S	Phenolics-	P	1.0224	mg/l	3/16/2023 10:39:47	
CCB1	S	Phenolics-	P	0.0041	mg/l	3/16/2023 10:39:49	
PB151436BL	S	Phenolics-	P	0.0036	mg/l	3/16/2023 10:39:51	
PB151436BS	S	Phenolics-	P	1.0243	mg/l	3/16/2023 10:39:52	
O1627-12	S	Phenolics-	P	0.0302	mg/l	3/16/2023 10:49:45	
O1923-01	S	Phenolics-	P	-0.0217	mg/l	3/16/2023 10:49:47	
O1923-01DUP	S	Phenolics-	P	-0.0248	mg/l	3/16/2023 10:49:48	
O1923-01MS	S	Phenolics-	P	0.9918	mg/l	3/16/2023 11:11:06	
O1923-01MSD	S	Phenolics-	P	0.9806	mg/l	3/16/2023 11:11:07	
CCV2	S	Phenolics-	P	1.0375	mg/l	3/16/2023 11:11:09	
CCB2	S	Phenolics-	P	0.0007	mg/l	3/16/2023 11:11:12	

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

3/16/2023 10:07

Test Phenolics-


Accepted 3/16/2023 10:07

Factor 13.81

Bias 0.007

Coeff. of det. 0.999834

Errors

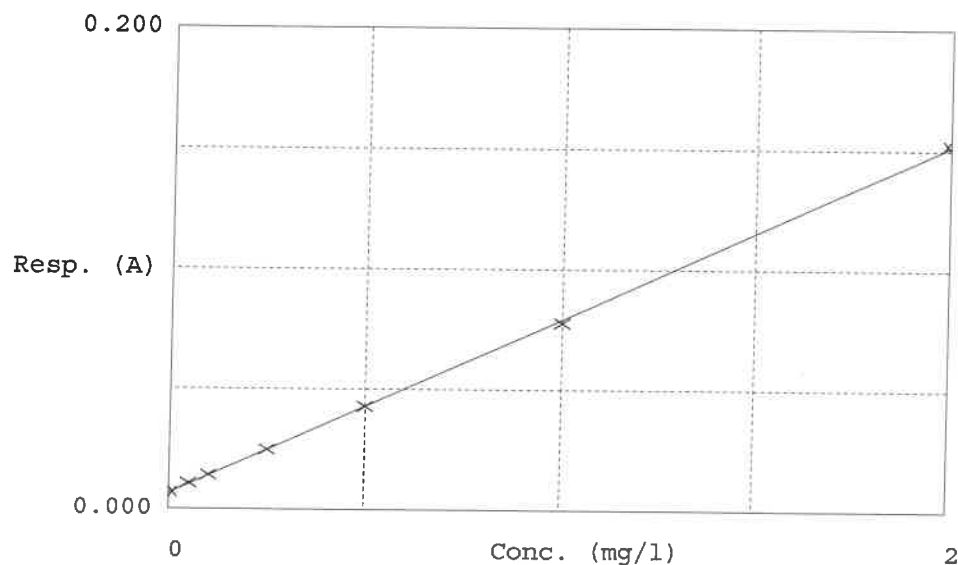

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.007	0.0024	0.0000	-
2	Phenol-2	0.011	0.0563	0.0500	12.8
3	Phenol-2	0.014	0.1029	0.1000	2.8
4	Phenol-2	0.025	0.2493	0.2500	-0.3
5	Phenol-2	0.043	0.4988	0.5000	-0.2
6	Phenol-2	0.078	0.9807	1.0000	-1.9
7	Phenol-2	0.152	2.0097	2.0000	0.5

12
3/16/23