

Clear table


Instrument ID: IC-2										Analyst :		IZ		Method:		300.0 / 9056A	
ident	concentra tion F-	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio on HPO4	concentratio on SO4	file name	date time	Initial wt/ Final Vol	Analyst						
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-02-21_	2/21/23 10:44		IZ/MA						
STD2	0.4920	0.6780	0.7170	2.3360	0.5860	1.2450	3.5390	2023-02-21_	2/21/23 11:16		IZ/MA						
STD3	0.8220	1.2480	1.2550	4.1190	1.0260	2.0990	6.2150	2023-02-21_	2/21/23 11:48		IZ/MA						
STD4	0.9980	1.4880	1.4540	4.9470	1.2430	2.2960	7.4400	2023-02-21_	2/21/23 13:37		IZ/MA						
STD5	1.8430	2.8780	2.8510	9.5750	2.3920	4.8400	14.2760	2023-02-21_	2/21/23 14:09		IZ/MA						
STD6	3.8900	5.8880	5.9030	19.5900	4.8850	9.8330	29.2840	2023-02-21_	2/21/23 14:40		IZ/MA						
STD7	5.1240	7.6200	7.6200	25.4430	6.3680	12.6870	38.2450	2023-02-21_	2/21/23 15:12		IZ/MA						
ICV	1.8340	2.9800	3.0180	9.9890	2.4670	4.8900	14.7310	2023-02-21_	2/21/23 17:02		IZ/MA						
ICB	0.0000	0.0000	0.0000	10.0880	0.0000	0.0000	0.0000	2023-02-21_	2/21/23 18:03		IZ/MA						
CCV	1.9640	2.9780	3.0030	0.0000	2.4860	5.1070	14.7260	2023-03-16_	3/16/23 10:02		IZ/MA						
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-03-16_	3/16/23 10:34		IZ/MA						
LB124536BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-03-16_	3/16/23 11:06		IZ/MA						
LB124536BSW	1.9270	3.0210	3.0220	10.1840	2.5150	4.9740	14.8790	2023-03-16_	3/16/23 11:37		IZ/MA						
O1923-01	0.4430	14.4400	0.1510	0.0000	0.1340	0.5210	197.2180	2023-03-16_	3/16/23 12:10		IZ/MA						
O1923-01MS	3.0590	17.5640	3.1680	10.2210	2.6590	8.1090	206.2900	2023-03-16_	3/16/23 12:41		IZ/MA						
O1923-01MSD	2.9300	17.5520	3.1580	10.0470	2.6160	8.2170	206.0210	2023-03-16_	3/16/23 13:13		IZ/MA						
O1935-02	18.4350	235.8350	0.0000	0.0000	4.4260	6.7490	0.0000	2023-03-16_	3/16/23 14:17		IZ/MA						
O1935-02DLX5	3.4360	39.2550	0.0000	0.0000	0.7030	0.5490	3.0720	2023-03-16_	3/16/23 14:48		IZ/MA						
CCV	1.8180	3.0580	3.1250	10.2610	2.5170	4.2890	15.0540	2023-03-16_	3/16/23 18:29		IZ/MA						
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-03-16_	3/16/23 19:01		IZ/MA						

Clear table

Instrument ID: IC-2									
Analyst :				IZ		Method:		300.0 / 9056A	
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time
Initial wt/ Final Vol									
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-02-21_	2/21/23 10:44
STD2	0.4920	0.6780	0.7170	2.3360	0.5860	1.2450	3.5390	2023-02-21_	2/21/23 11:16
STD3	0.8220	1.2480	1.2550	4.1190	1.0260	2.0990	6.2150	2023-02-21_	2/21/23 11:48
STD4	0.9980	1.4880	1.4540	4.9470	1.2430	2.2960	7.4400	2023-02-21_	2/21/23 13:37
STD5	1.8430	2.8780	2.8510	9.5750	2.3920	4.8400	14.2760	2023-02-21_	2/21/23 14:09
STD6	3.8900	5.8880	5.9030	19.5800	4.8850	9.8330	29.2840	2023-02-21_	2/21/23 14:40
STD7	5.1240	7.6200	7.6200	25.4430	6.3680	12.6870	38.2450	2023-02-21_	2/21/23 15:12
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4		
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000		
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000		
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000		
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000		
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000		
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000		
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000		
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4		
STD1									
STD2	23.0000	13.0000	19.5000	16.8000	17.2000	24.5000	17.9667		
STD3	2.7500	4.0000	4.5833	2.9750	2.6000	4.9500	3.5833		
STD4	-0.2000	-0.8000	-3.0667	-1.0600	-0.5600	-8.1600	-0.8000		
STD5	-7.8500	-4.0667	-4.9667	-4.2500	-4.3200	-3.2000	-4.8267		
STD6	-2.7500	-1.8667	-1.6167	-2.1000	-2.3000	-1.6700	-2.3867		
STD7	2.4800	1.6000	1.6000	1.7720	1.8880	1.4960	3.3649		

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-022123.mtw
 Equation: $Q = 0.0749918 \cdot A + 4.34204$
 RSD: 5.920 %
 Correlation coefficient: 0.998088

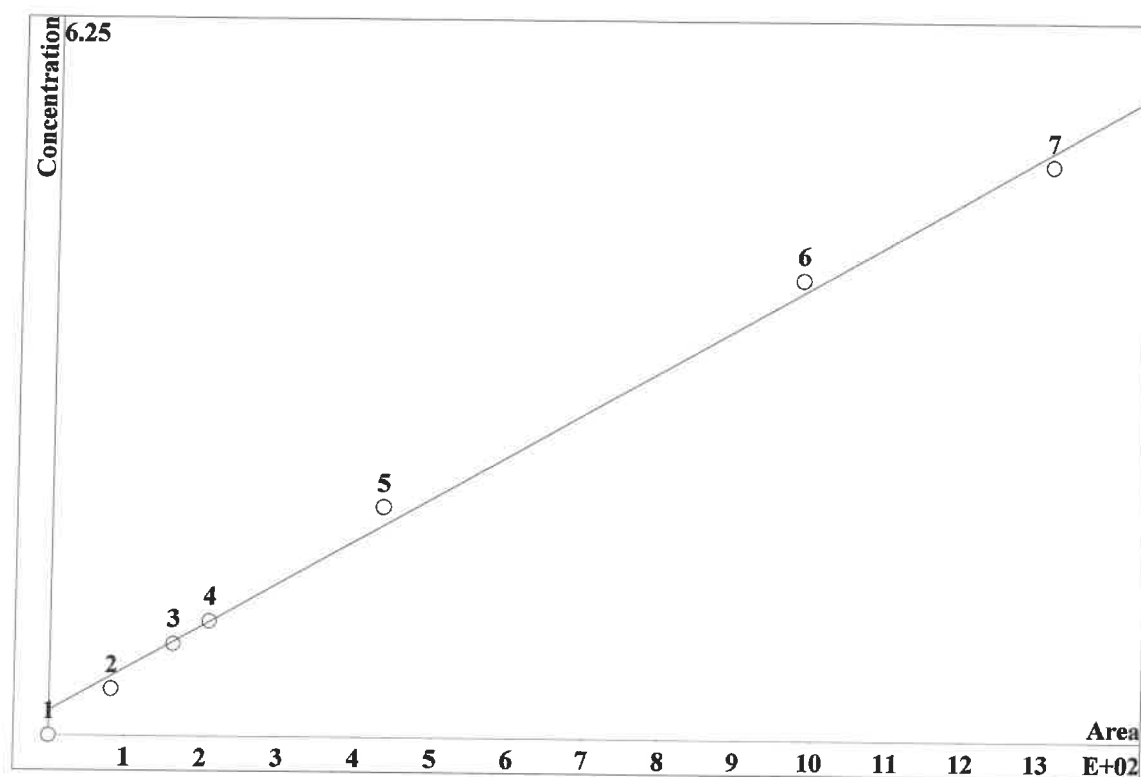


K3 = 0 K2 = 0 K1 = 0.0749918 K0 = 4.34204
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	1.369	81.6	0.4	20	6.113		
3	3.148	161.3	0.8	20	6.113		
4	4.373	208.2	1	20	6.113		
5	8.63	433.6	2	20	6.113		
6	20.89	979.5	4	20	6.113		
7	27.03	1309	5	20	6.113		

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-022123.mtw
 Equation: $Q = 0.126762 \cdot A + 3.40502$
 RSD: 3.398 %
 Correlation coefficient: 0.999370

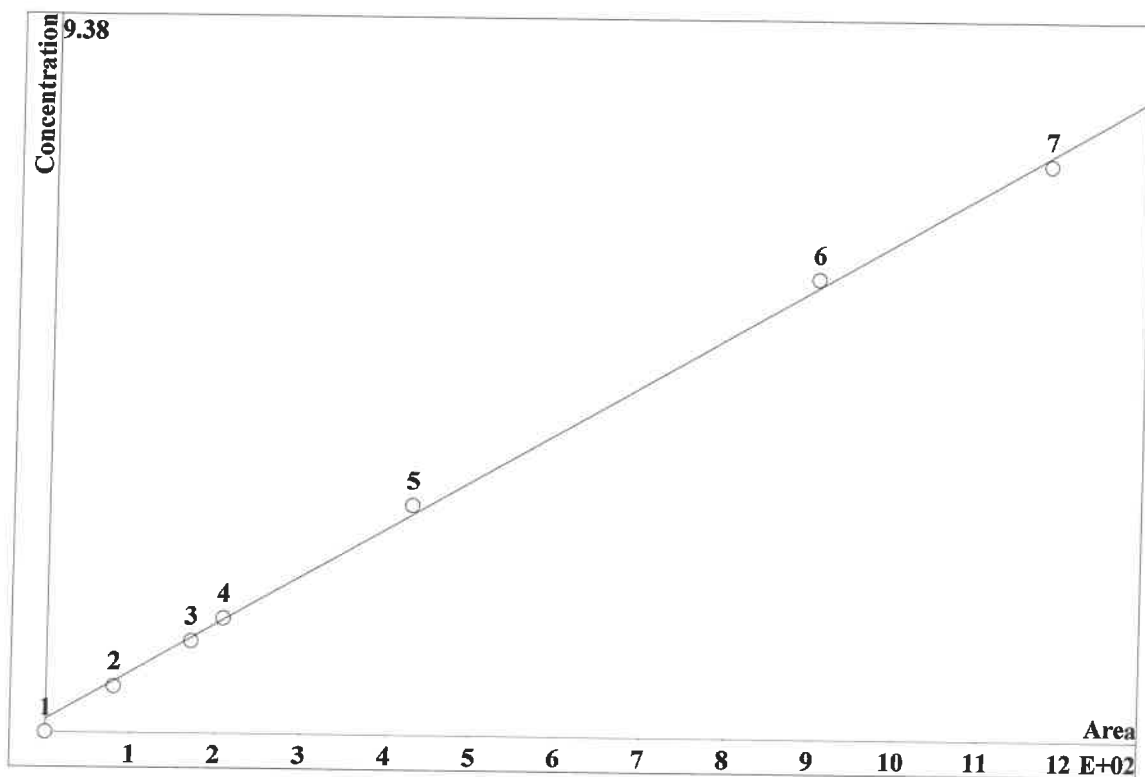


K3 = 0 K2 = 0 K1 = 0.126762 K0 = 3.40502
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	4.987	80.06	0.6	20	9.089		
3	10.35	170	1.2	20	9.089		
4	12.75	207.9	1.5	20	9.089		
5	26.5	427.3	3	20	9.089		
6	56.44	902.1	6	20	9.089		
7	73.41	1175	7.5	20	9.089		

1.□

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-022123.mtw
 Equation: $Q = 0.0557567 \cdot A + 5.76076$
 RSD: 3.856 %
 Correlation coefficient: 0.999189

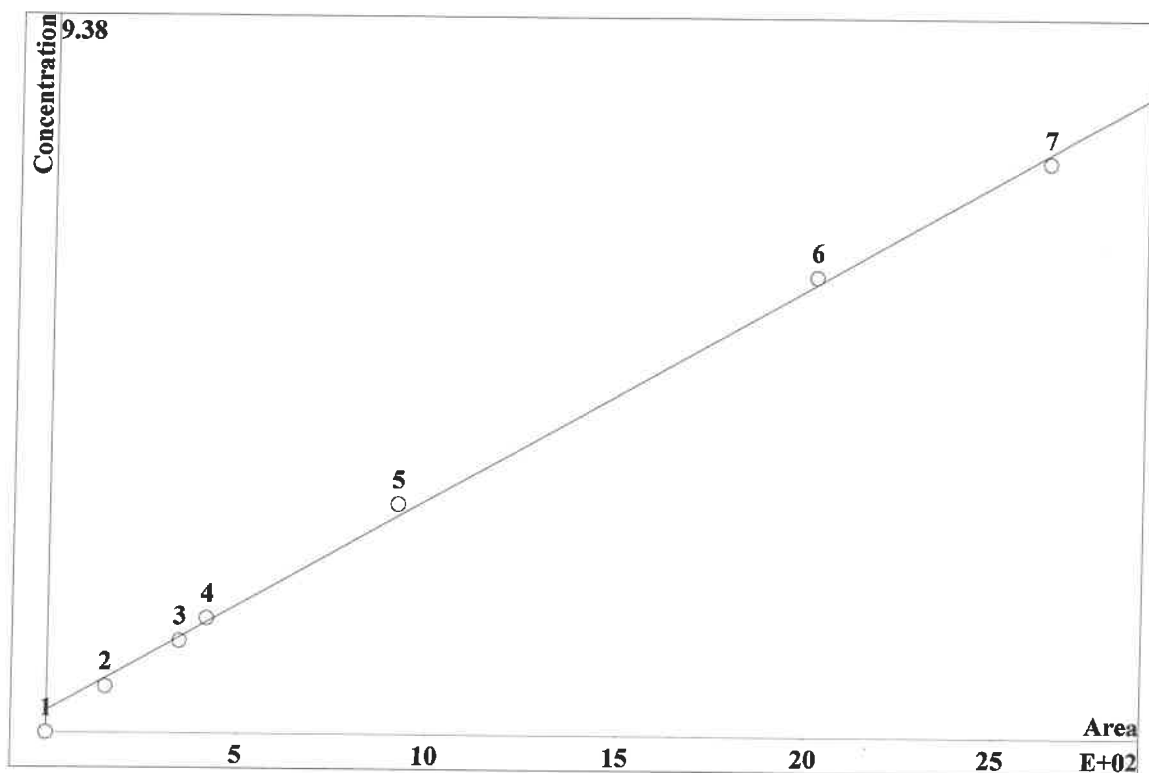


K3 = 0 K2 = 0 K1 = 0.0557567 K0 = 5.76076
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	7.543	153.9	0.6	20	10.92		
3	16.86	346.9	1.2	20	10.92		
4	20.85	418.2	1.5	20	10.92		
5	45.79	919.5	3	20	10.92		
6	98.56	2014	6	20	10.92		
7	128	2630	7.5	20	10.92		

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-022123.mtw
 Equation: $Q = 0.281656 \cdot A + 14.8485$
 RSD: 3.758 %
 Correlation coefficient: 0.999230

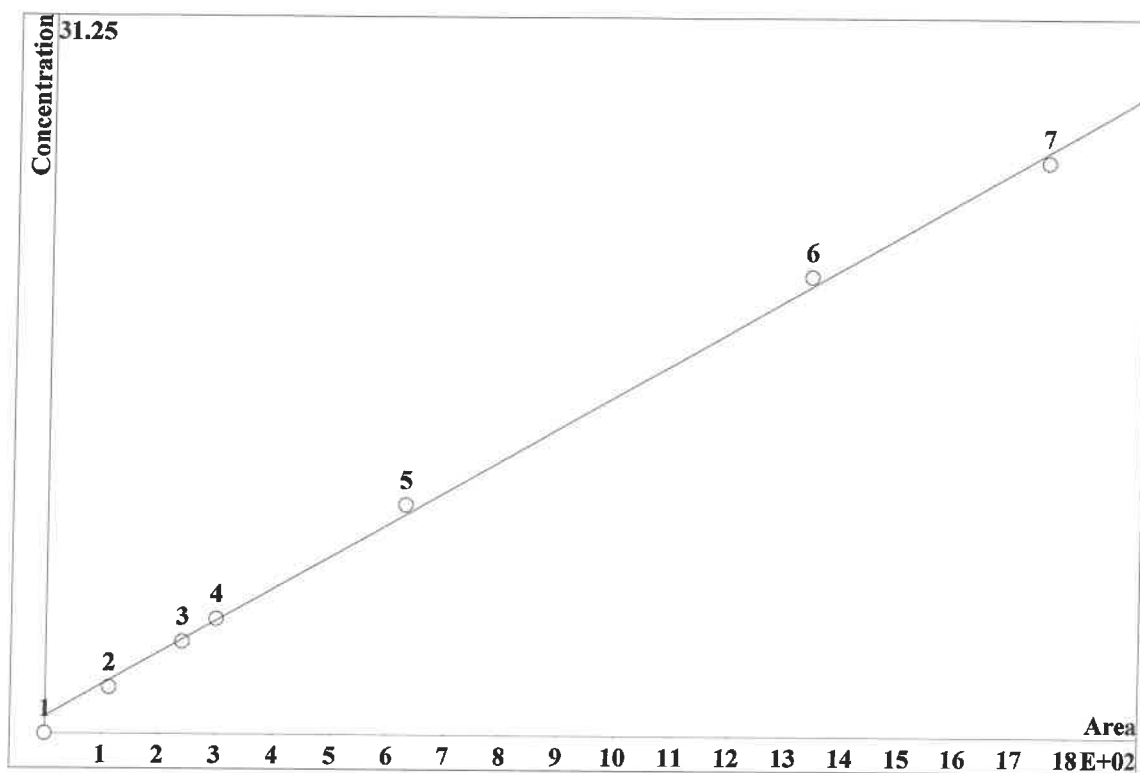


K3 = 0 K2 = 0 K1 = 0.281656 K0 = 14.8485
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	5.403	113.2	2	20	14.05		
3	11.55	239.8	4	20	14.05		
4	14.44	298.5	5	20	14.05		
5	30.61	627.2	10	20	14.05		
6	65.85	1338	20	20	14.05		
7	86.08	1754	25	20	14.05		

1. □

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-022123.mtw
 Equation: $Q = 0.0491063 \cdot A + 3.24923$
 RSD: 3.939 %
 Correlation coefficient: 0.999154

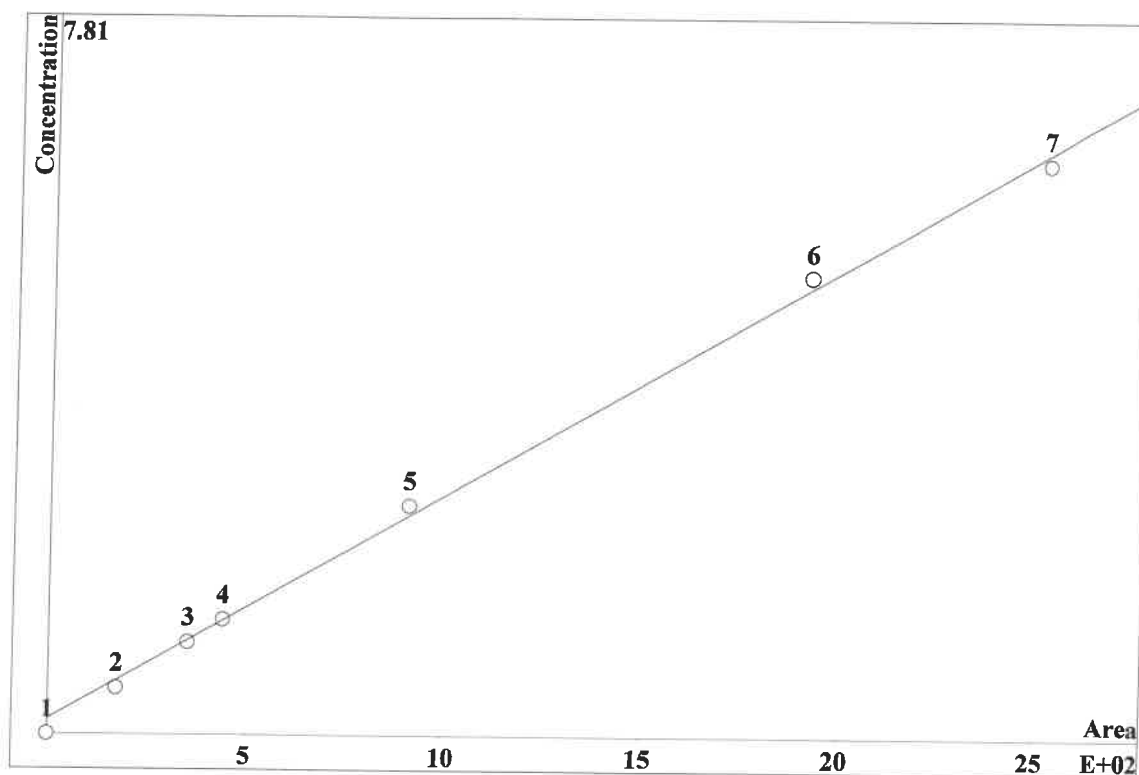


K3 = 0 K2 = 0 K1 = 0.0491063 K0 = 3.24923
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.522	172.4	0.5	20	15.97		
3	13.59	351.7	1	20	15.97		
4	17.08	440.1	1.25	20	15.97		
5	35.76	908.2	2.5	20	15.97		
6	77.05	1923	5	20	15.97		
7	101.6	2527	6.25	20	15.97		

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-022123.mtw
 Equation: $Q = 0.0553071 \cdot A + 13.4923$
 RSD: 4.068 %
 Correlation coefficient: 0.999097

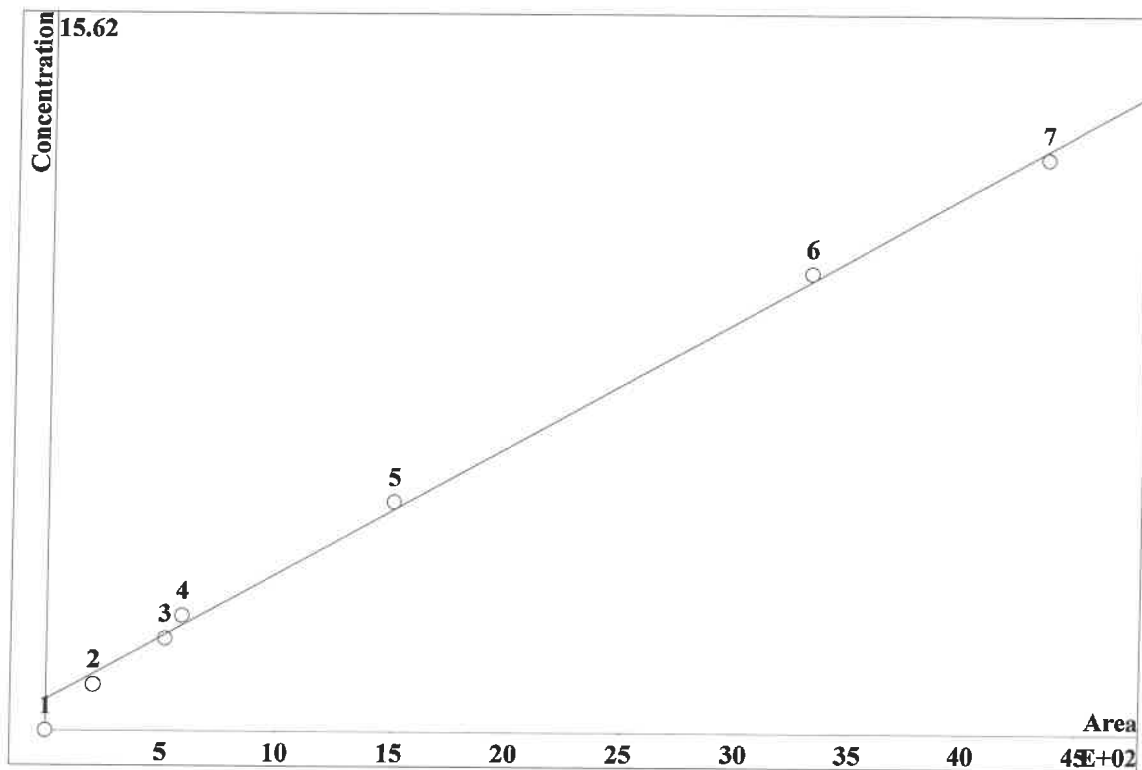

K3 = 0 K2 = 0 K1 = 0.0553071 K0 = 13.4923

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		
2	3.872	206.4	1	20	22.61		
3	9.929	515	2	20	22.61		
4	10.64	586.4	2.5	20	22.61		
5	30.45	1506	5	20	22.61		
6	69.97	3312	10	20	22.61		
7	93.58	4344	12.5	20	22.61		

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-022123.mtw
 Equation: $Q = 0.162666 \cdot A + 18.2166$
 RSD: 4.213 %
 Correlation coefficient: 0.999032

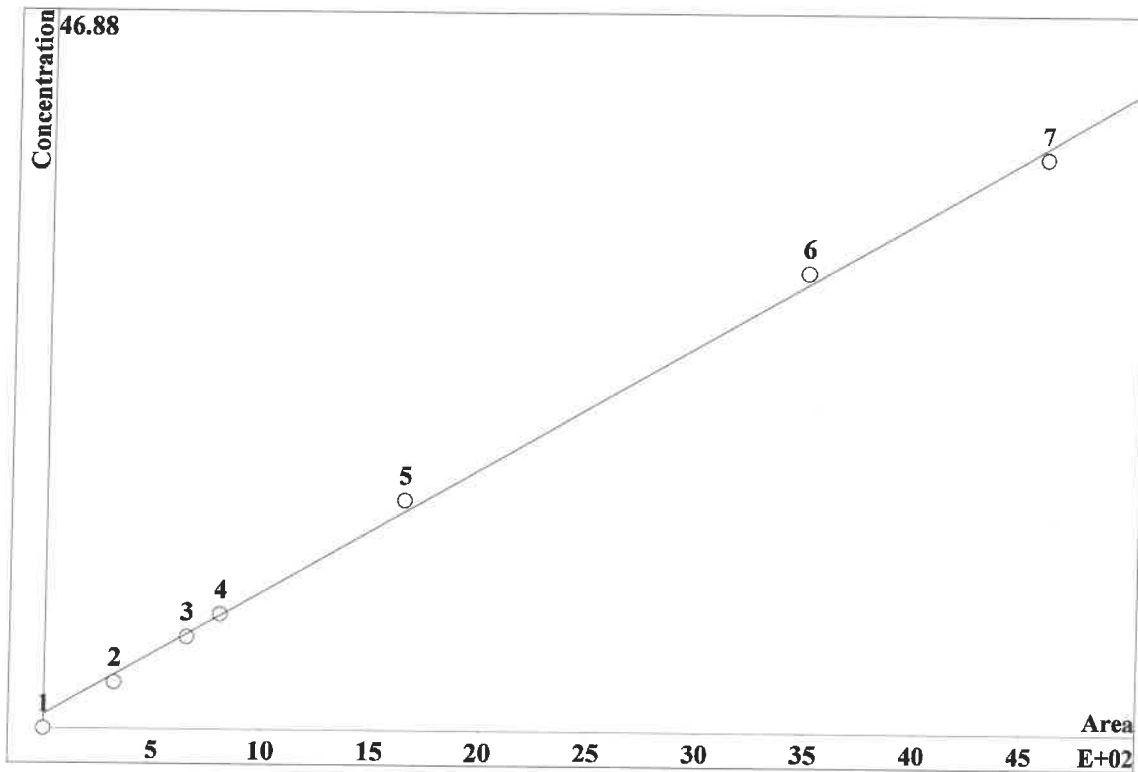

K3 = 0 K2 = 0 K1 = 0.162666 K0 = 18.2166
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	8.242	323.2	3	20	26.01		
3	16.92	652.2	6	20	26.01		
4	20.99	802.8	7.5	20	26.01		
5	43.78	1643	15	20	26.01		
6	94.3	3489	30	20	26.01		
7	124.6	4590	37.5	20	26.01		

Report date: 2/22/2023 11:53:29 AM
Printed by: wet


Ident: STD1
Analysis from: 2/21/2023 10:44:54 AM
File: _2023-02-21_

Last save: 2/21/2023 4:00:42 PM

Method: AnionsIC2-022123.mtw
Run operator: wet
Analysis number: 33358

Last save: 2/21/2023 2:38:

SAMPLE:
: IZ/MA
Vial number: 2'
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

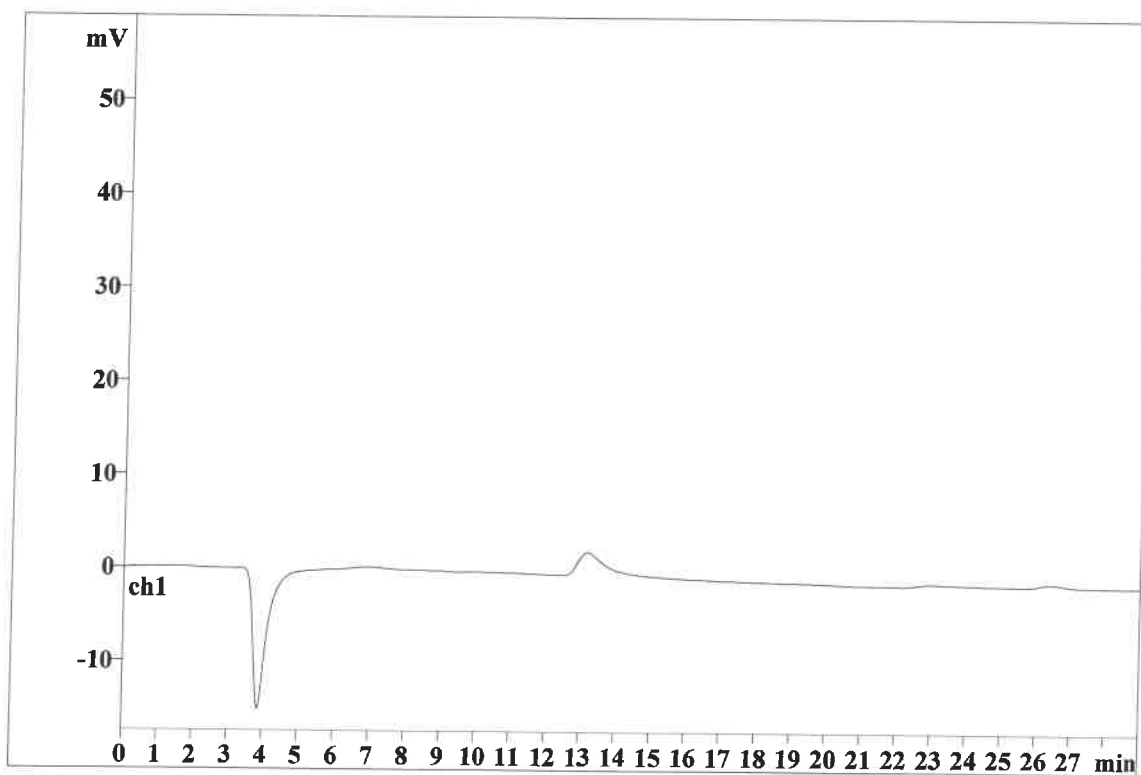

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 2/22/2023 11:53:38 AM
Printed by: wet


Ident: STD2
Analysis from: 2/21/2023 11:16:32 AM
File: _2023-02-21_

Last save: 2/21/2023 4:05:53 PM

Method: AnionsIC2-022123.mtw
Run operator: wet
Analysis number: 33359

Last save: 2/21/2023 2:38:

SAMPLE:
: IZ/MA
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

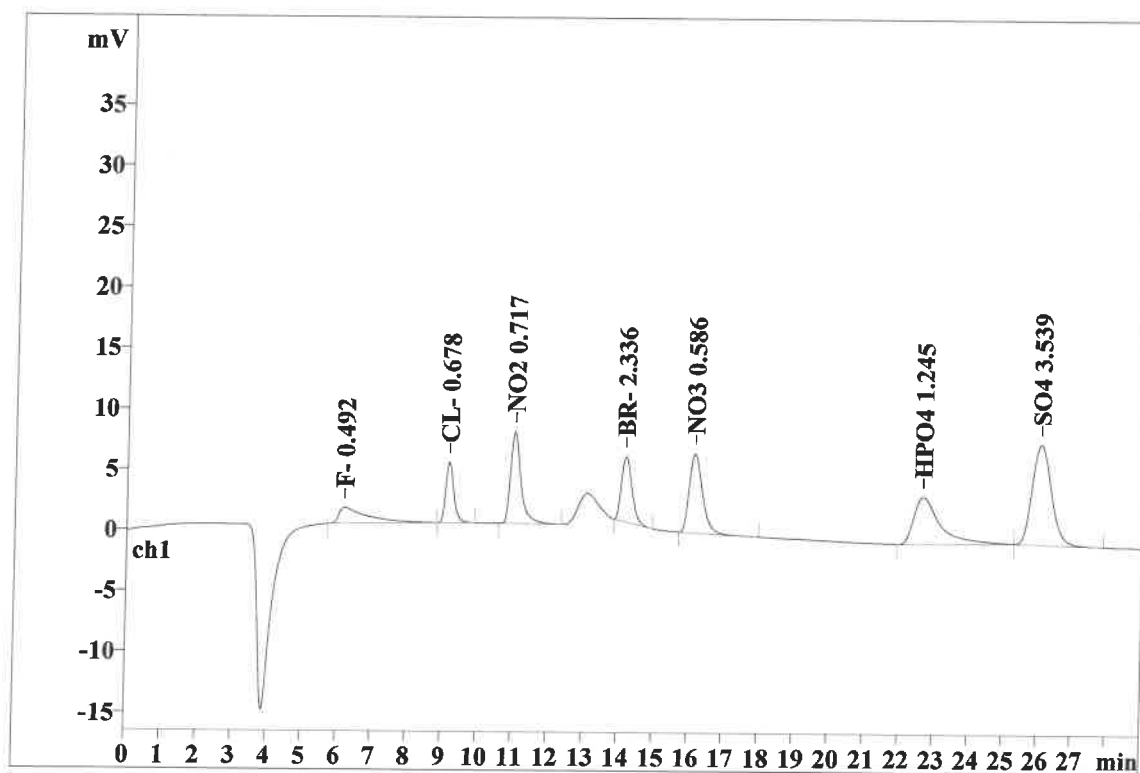

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.18	0.732	1.30	3.42	73.347	6.53
2	9.16	0.243	4.99	13.17	80.059	7.13
3	11.01	0.293	7.54	19.92	153.905	13.71
4	14.17	0.324	5.40	14.26	113.152	10.08
5	16.13	0.401	6.52	17.22	172.360	15.36
6	22.65	0.715	3.87	10.22	206.396	18.39
7	26.04	0.608	8.24	21.76	323.163	28.79
7	29.00	0.474	37.86	99.98	1122.383	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/22/2023 11:53:46 AM
Printed by: wet


Ident: STD3
Analysis from: 2/21/2023 11:48:10 AM
File: _2023-02-21_

Last save: 2/21/2023 4:00:42 PM

Method: AnionsIC2-022123.mtw
Run operator: wet
Analysis number: 33360

Last save: 2/21/2023 2:38:

SAMPLE:
: IZ/MA
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

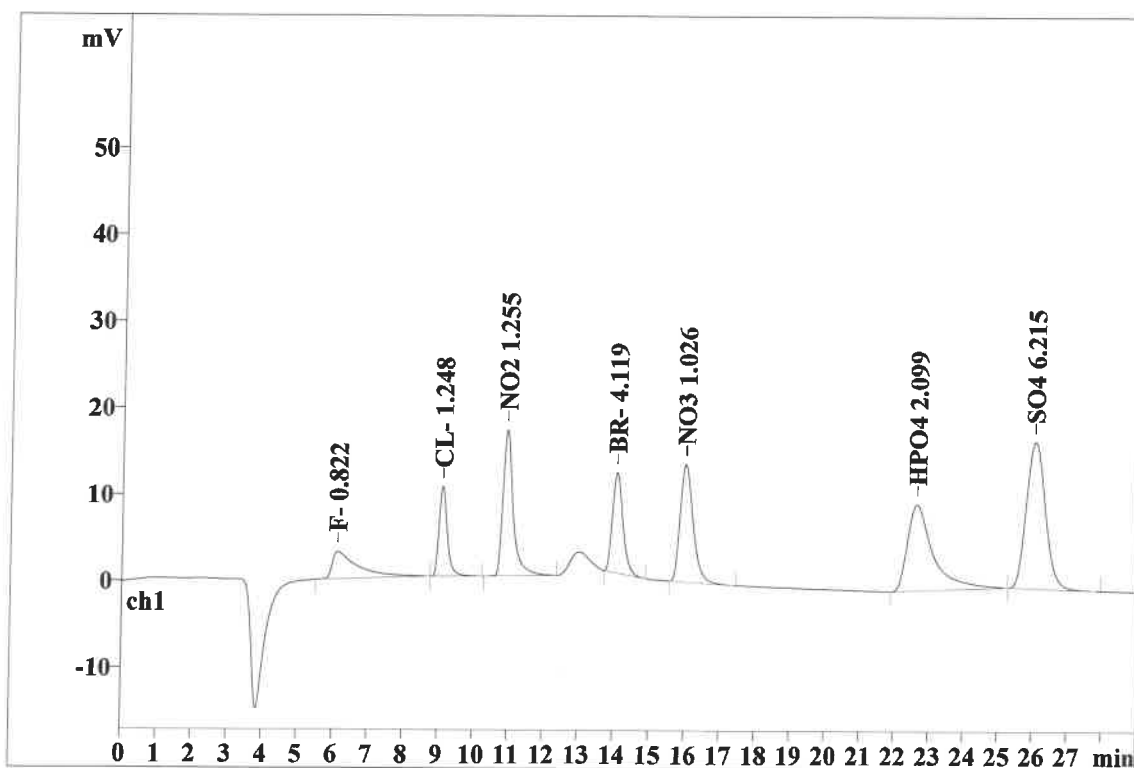

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.11	0.668	3.15	3.82	161.313	6.62
2	9.09	0.242	10.35	12.57	170.040	6.98
3	10.92	0.292	16.86	20.47	346.928	14.24
4	14.05	0.320	11.55	14.02	239.776	9.84
5	15.97	0.393	13.60	16.51	351.707	14.43
6	22.61	0.698	9.93	12.06	515.049	21.13
7	26.01	0.598	16.92	20.55	652.177	26.76
7	29.00	0.459	82.35	99.99	2436.989	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/22/2023 11:53:54 AM
Printed by: wet


Ident: STD4
Analysis from: 2/21/2023 1:37:38 PM
File: _2023-02-21_

Last save: 2/21/2023 4:00:42 PM

Method: AnionsIC2-022123.mtw
Run operator: wet
Analysis number: 33364

Last save: 2/21/2023 2:38:

SAMPLE:
: IZ/MA
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

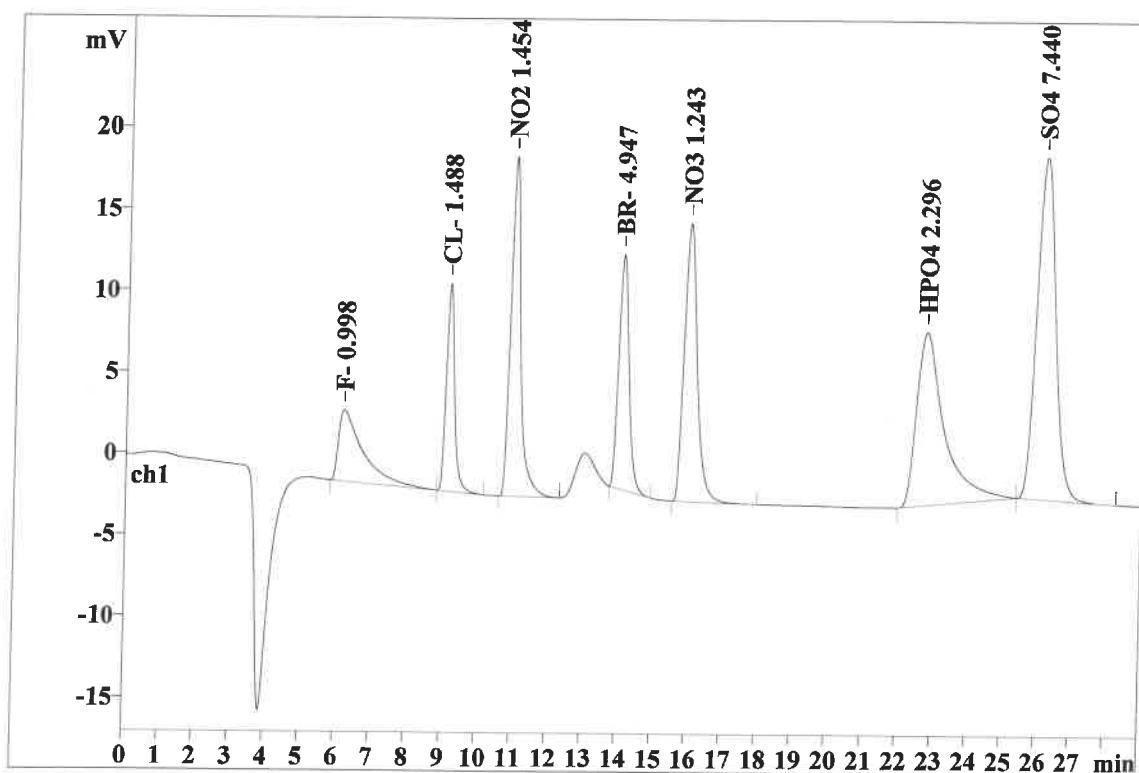

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.19	0.647	4.37	4.32	208.153	7.03
2	9.15	0.241	12.75	12.61	207.890	7.02
3	10.96	0.289	20.85	20.62	418.231	14.12
4	14.07	0.318	14.44	14.28	298.531	10.08
5	15.98	0.390	17.08	16.89	440.103	14.86
6	22.75	0.745	10.64	10.52	586.352	19.80
7	26.14	0.594	20.98	20.75	802.818	27.10
7	29.00	0.461	101.11	100.00	2962.078	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/22/2023 11:54:01 AM
Printed by: wet


Ident: STD5
Analysis from: 2/21/2023 2:09:16 PM
File: _2023-02-21_

Last save: 2/21/2023 4:00:42 PM

Method: AnionsIC2-022123.mtw
Run operator: wet
Analysis number: 33365

Last save: 2/21/2023 2:38:

SAMPLE:
: IZ/MA
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

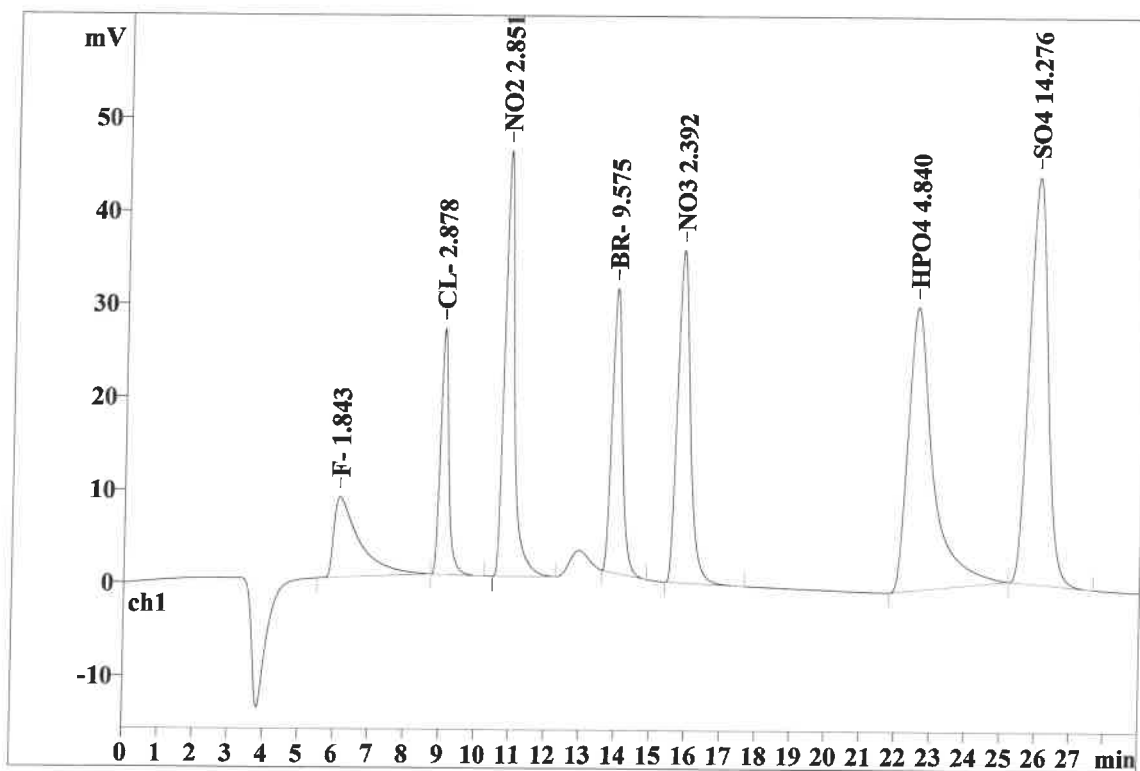

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.13	0.677	8.63	3.90	433.643	6.71
2	9.04	0.238	26.50	11.96	427.294	6.61
3	10.84	0.287	45.79	20.67	919.454	14.22
4	13.94	0.313	30.61	13.82	627.183	9.70
5	15.82	0.383	35.76	16.14	908.244	14.05
6	22.53	0.666	30.45	13.75	1506.127	23.30
7	25.94	0.583	43.78	19.77	1643.268	25.42
7	29.00	0.449	221.52	100.00	6465.213	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/22/2023 11:54:09 AM
Printed by: wet


Ident: STD6
Analysis from: 2/21/2023 2:40:53 PM
File: _2023-02-21_

Last save: 2/21/2023 4:00:42 PM

Method: AnionsIC2-022123.mtw
Run operator: wet
Analysis number: 33366

Last save: 2/21/2023 2:38:

SAMPLE:
: IZ/MA
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

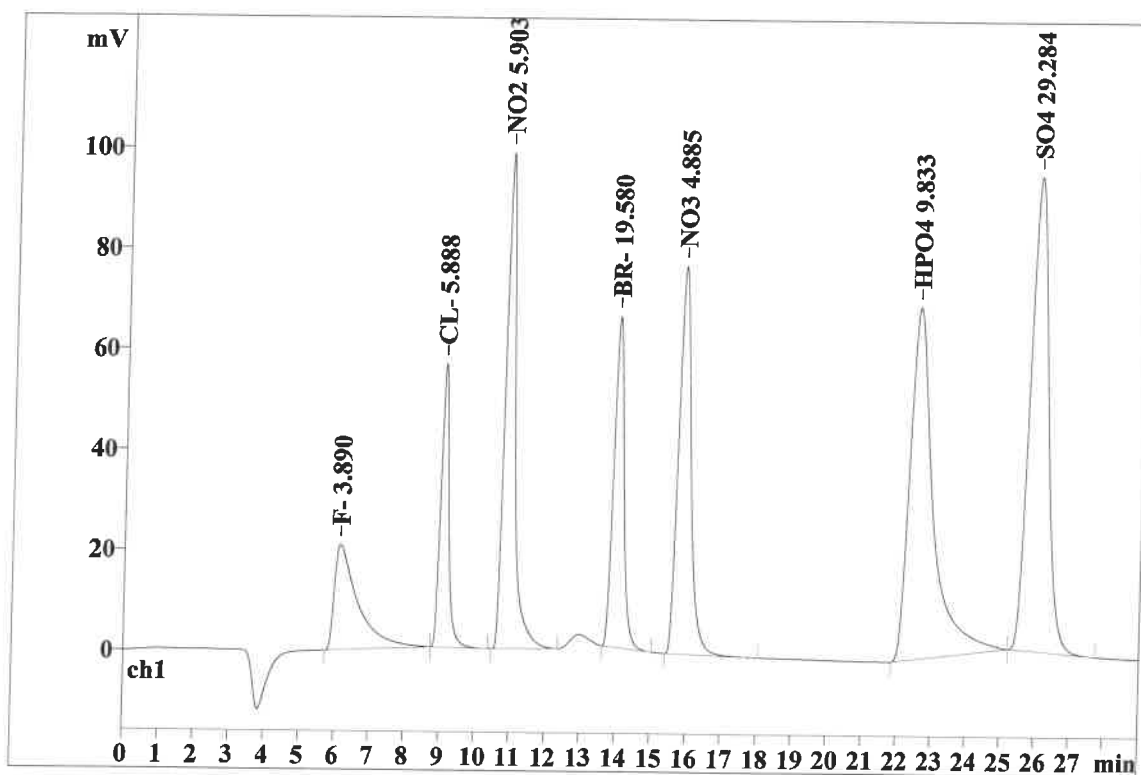

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.13	0.634	20.89	4.32	979.528	7.02
2	9.05	0.234	56.44	11.68	902.087	6.46
3	10.85	0.291	98.56	20.40	2013.979	14.43
4	13.98	0.309	65.85	13.63	1337.635	9.58
5	15.82	0.375	77.05	15.95	1923.216	13.78
6	22.53	0.639	69.97	14.48	3311.775	23.73
7	25.97	0.574	94.30	19.52	3488.521	25.00
7	29.00	0.436	483.06	100.00	13956.741	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/22/2023 11:54:18 AM
Printed by: wet


Ident: STD7
Analysis from: 2/21/2023 3:12:31 PM
File: _2023-02-21_

Last save: 2/21/2023 4:00:42 PM

Method: AnionsIC2-022123.mtw
Run operator: wet
Analysis number: 33367

Last save: 2/21/2023 2:38:

SAMPLE:
: IZ/MA
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

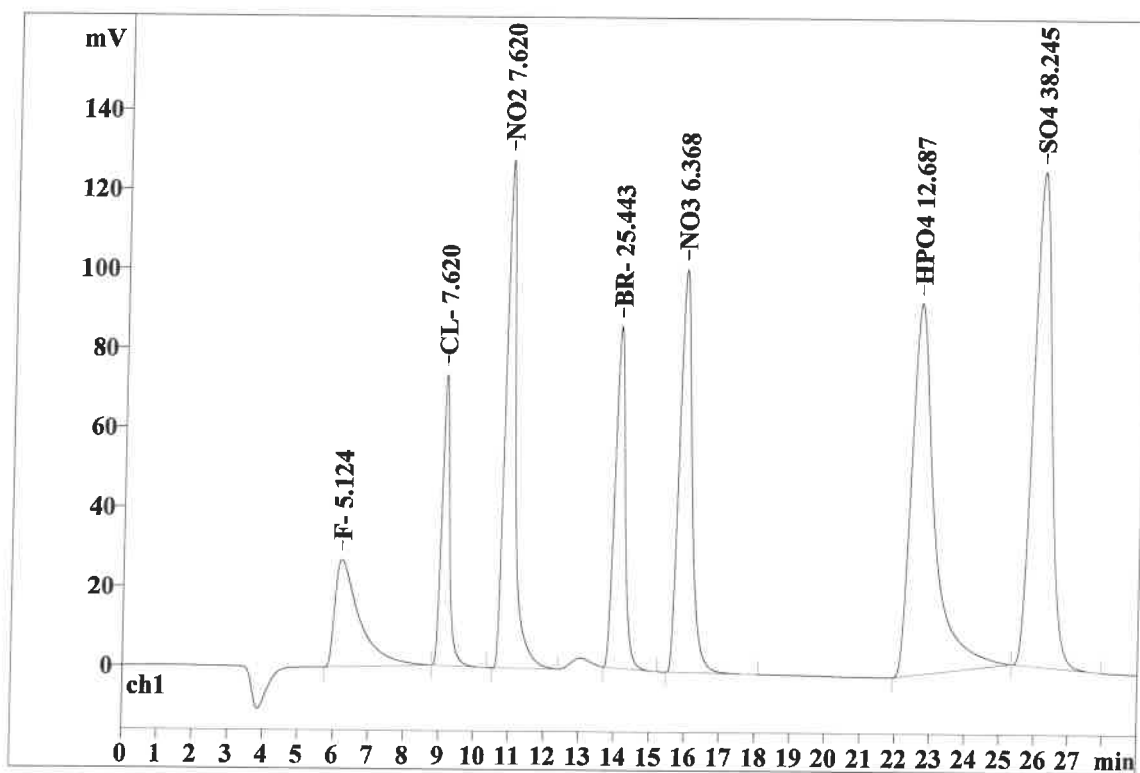

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.20	0.671	27.03	4.26	1308.751	7.14
2	9.10	0.234	73.41	11.57	1175.426	6.41
3	10.90	0.292	127.97	20.18	2629.874	14.35
4	14.05	0.309	86.08	13.57	1753.981	9.57
5	15.89	0.373	101.56	16.01	2527.479	13.79
6	22.61	0.628	93.58	14.76	4343.957	23.70
7	26.08	0.571	124.56	19.64	4590.316	25.04
7	29.00	0.440	634.19	100.00	18329.785	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/22/2023 11:54:53 AM
Printed by: wet


Ident: ICV
Analysis from: 2/21/2023 5:02:05 PM
File: _2023-02-21_

Last save: 2/21/2023 5:30:05 PM

Method: AnionsIC2-022123.mtw
Run operator: wet
Analysis number: 33372

Last save: 2/21/2023 4:07:

SAMPLE:
:
Vial number: 23
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

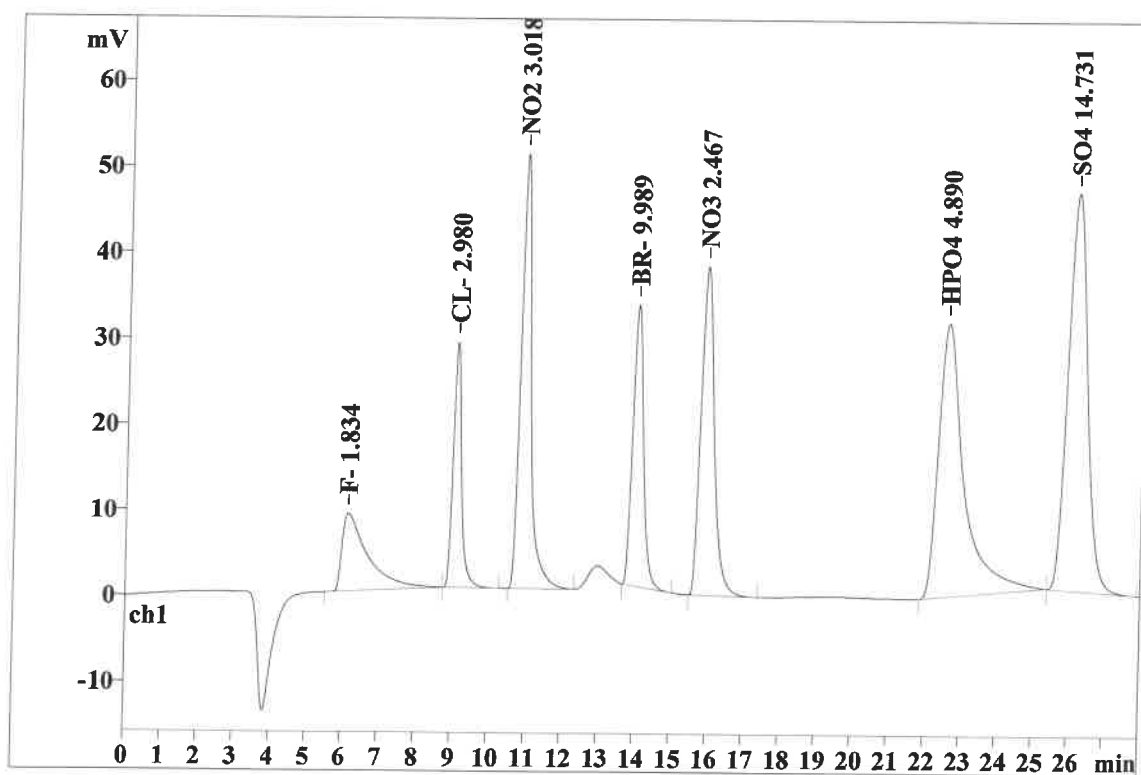

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.14	0.670	9.05	3.81	446.779	6.47
2	9.07	0.236	28.58	12.03	459.826	6.65
3	10.89	0.285	50.64	21.32	1014.118	14.68
4	14.01	0.314	32.79	13.80	675.678	9.78
5	15.90	0.383	38.30	16.13	971.732	14.06
6	22.57	0.664	31.83	13.40	1581.625	22.89
7	26.14	0.589	46.31	19.50	1760.194	25.47
7	28.00	0.449	237.51	100.00	6909.952	100.00

This report has been created by IC Net
METROHM LTD

Report date: 2/22/2023 11:55:14 AM
Printed by: wet


Ident: ICB
Analysis from: 2/21/2023 6:03:26 PM
File: _2023-02-21_

Last save: 2/21/2023 6:31:26 PM

Method: AnionsIC2-022123.mtw
Run operator: wet
Analysis number: 33374

Last save: 2/21/2023 4:07:

SAMPLE:
: IZ/MA
Vial number: 10
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

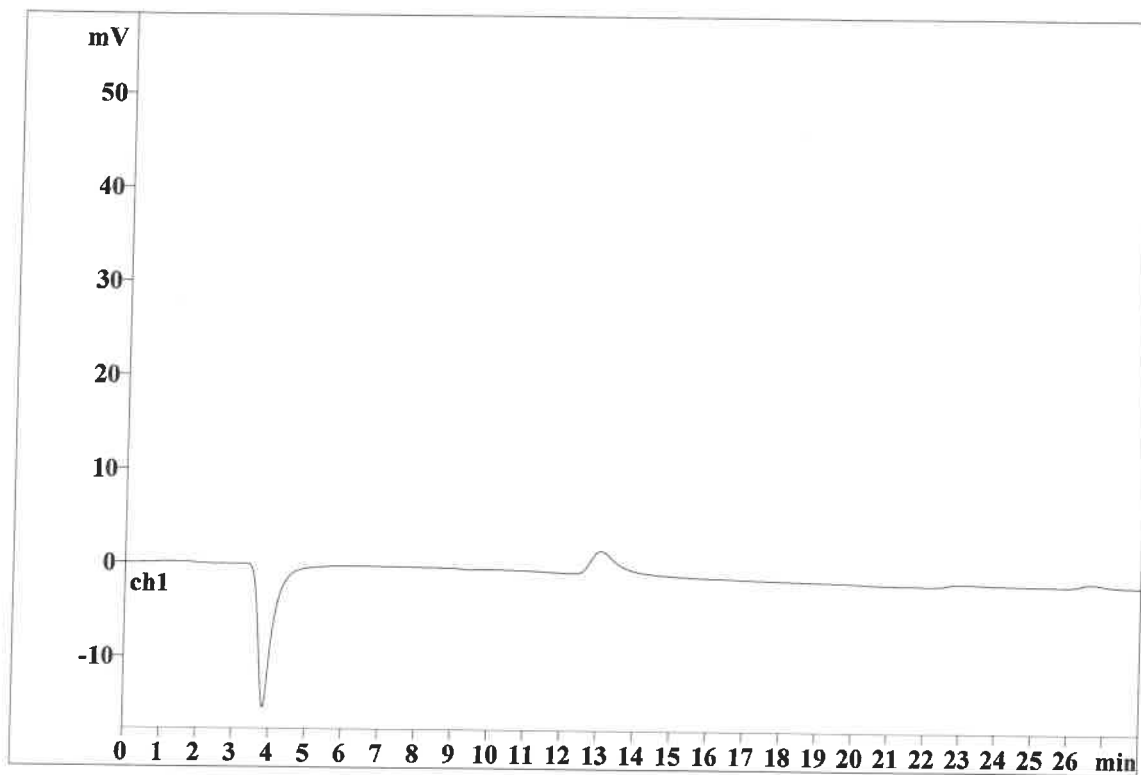

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 3/17/2023 10:12:52 AM
Printed by: wet


Ident: CCV
Analysis from: 3/16/2023 10:02:29 AM
File: _2023-03-16_

Last save: 3/16/2023 10:31:29 AM

Method: AnionsIC2-022123.mtw
Run operator: wet
Analysis number: 33572

Last save: 2/24/2023 11:36

SAMPLE:
: IZ/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

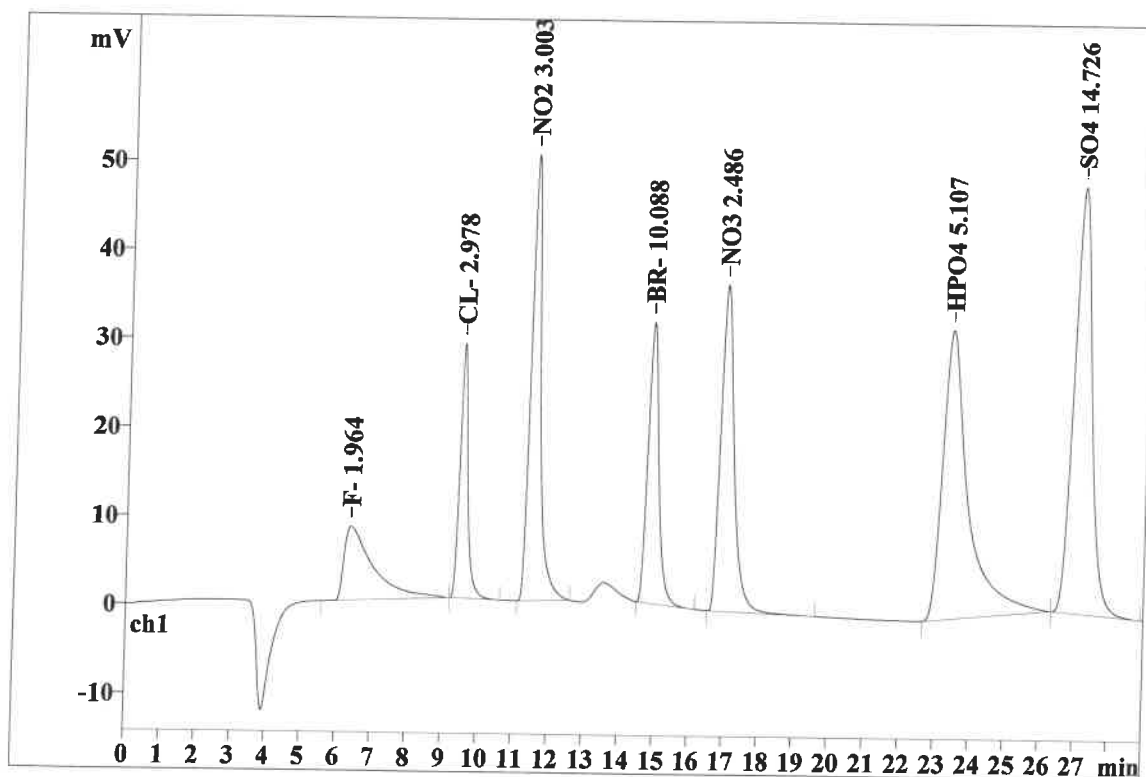

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.37	0.783	8.31	3.52	480.727	6.84
2	9.50	0.233	28.73	12.15	459.630	6.54
3	11.47	0.287	50.24	21.25	1009.073	14.36
4	14.85	0.322	31.68	13.40	682.535	9.71
5	16.94	0.394	36.76	15.55	979.386	13.93
6	23.37	0.664	32.57	13.78	1658.091	23.59
7	27.09	0.555	48.08	20.34	1759.633	25.03
7	29.00	0.463	236.36	100.00	7029.074	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/17/2023 10:13:13 AM
Printed by: wet


Ident: CCB
Analysis from: 3/16/2023 10:34:28 AM
File: _2023-03-16_

Last save: 3/17/2023 10:13:08 AM

Method: AnionsIC2-022123.mtw
Run operator: wet
Analysis number: 33573

Last save: 2/24/2023 11:36

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

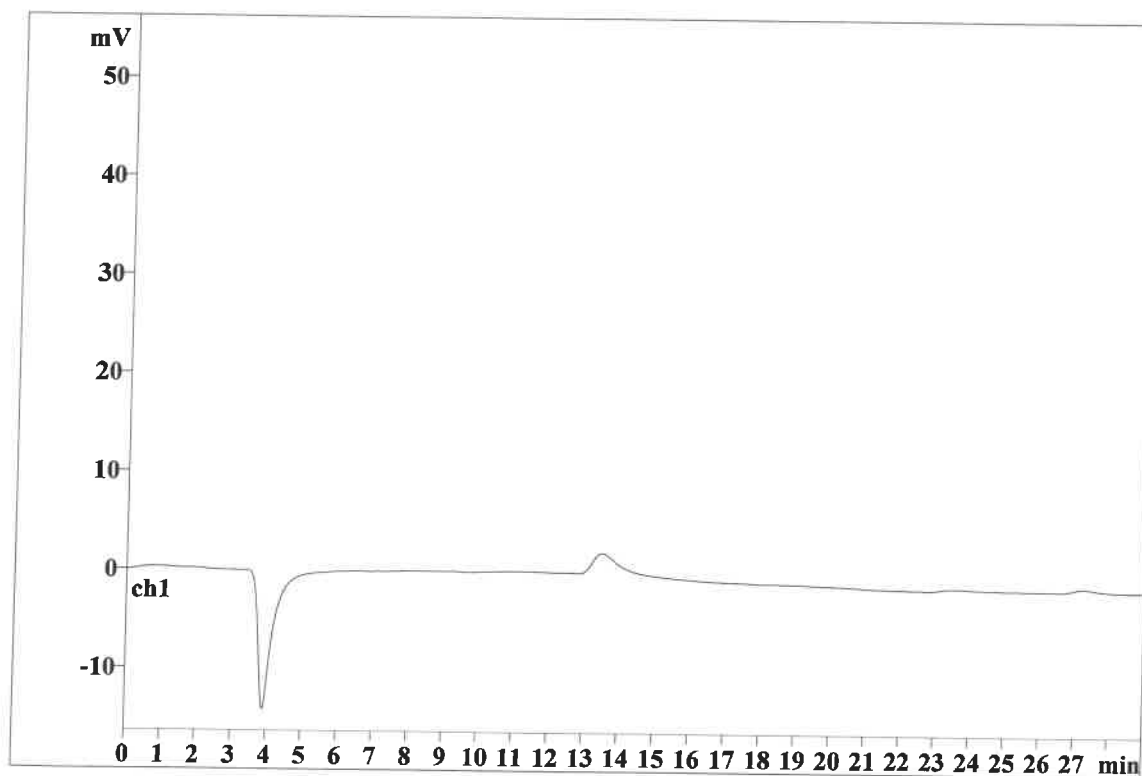

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 3/17/2023 10:13:29 AM
Printed by: wet


Ident: LB124536BLW
Analysis from: 3/16/2023 11:06:05 AM
File: _2023-03-16_

Last save: 3/17/2023 10:13:25 AM

Method: AnionsIC2-022123.mtw
Run operator: wet
Analysis number: 33574

Last save: 2/24/2023 11:36

SAMPLE:
: IZ/MA
Vial number: 13
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

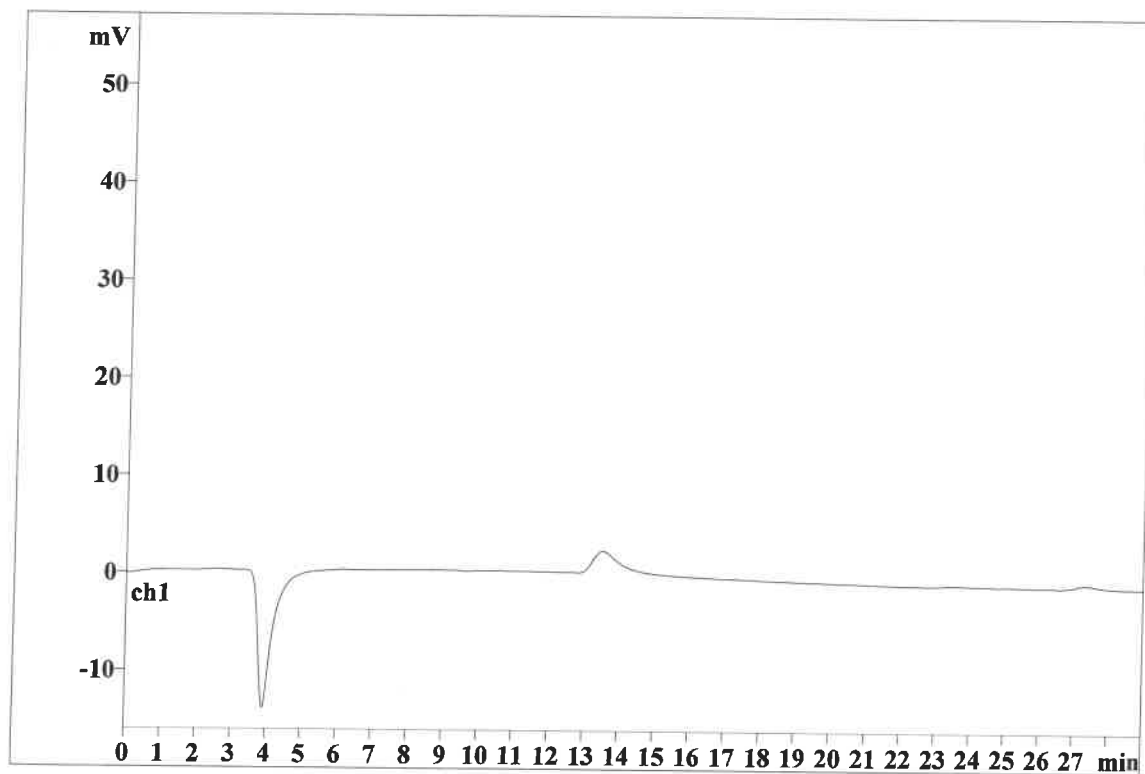

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 3/17/2023 10:13:38 AM
Printed by: wet


Ident: LB124536BSW
Analysis from: 3/16/2023 11:37:43 AM
File: _2023-03-16_

Last save: 3/17/2023 10:12:44 AM

Method: AnionsIC2-022123.mtw
Run operator: wet
Analysis number: 33575

Last save: 2/24/2023 11:36

SAMPLE:
: IZ/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

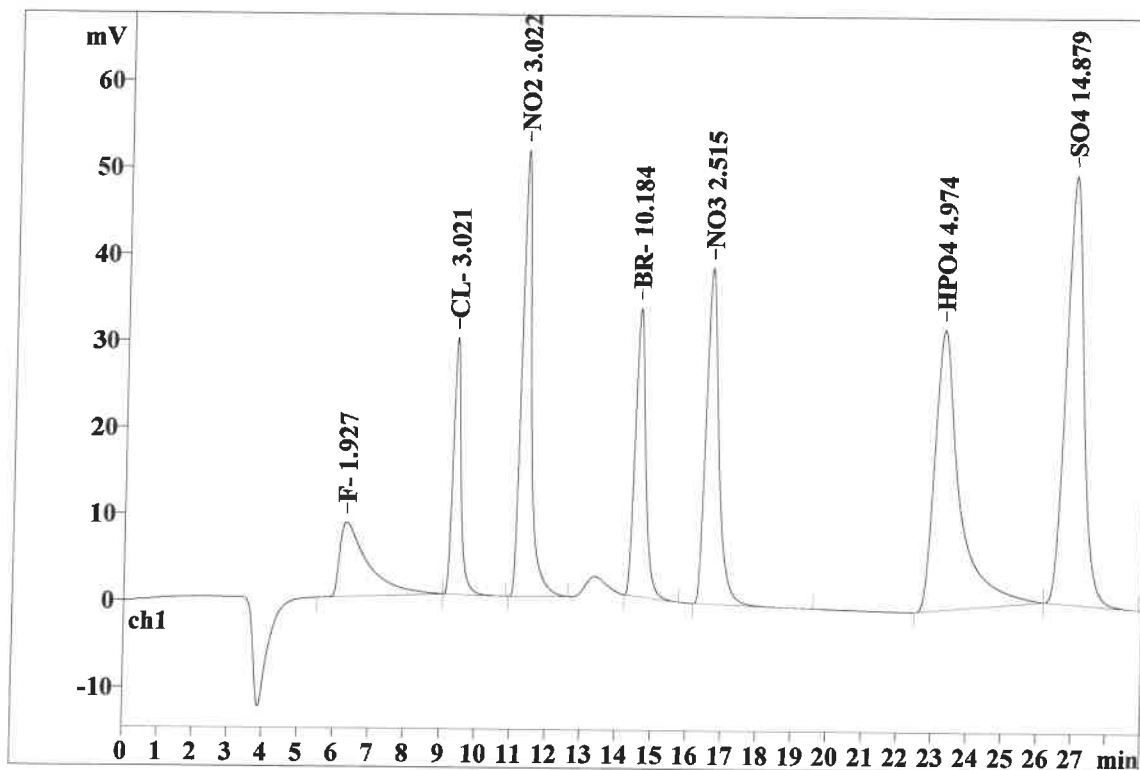

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.31	0.742	8.59	3.53	471.065	6.71
2	9.36	0.227	29.68	12.18	466.203	6.64
3	11.27	0.280	51.51	21.14	1015.746	14.47
4	14.55	0.310	33.26	13.65	689.210	9.82
5	16.57	0.378	38.77	15.91	990.665	14.11
6	23.22	0.648	32.40	13.29	1611.147	22.94
7	26.91	0.544	49.49	20.31	1777.897	25.32
7	29.00	0.447	243.71	100.00	7021.934	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/17/2023 10:13:56 AM
Printed by: wet


Ident: 01923-01
Analysis from: 3/16/2023 12:10:17 PM
File: _2023-03-16_

Last save: 3/16/2023 12:39:17 PM

Method: AnionsIC2-022123.mtw
Run operator: wet
Analysis number: 33576

Last save: 2/24/2023 11:36

SAMPLE:
: IZ/MA
Vial number: 25
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

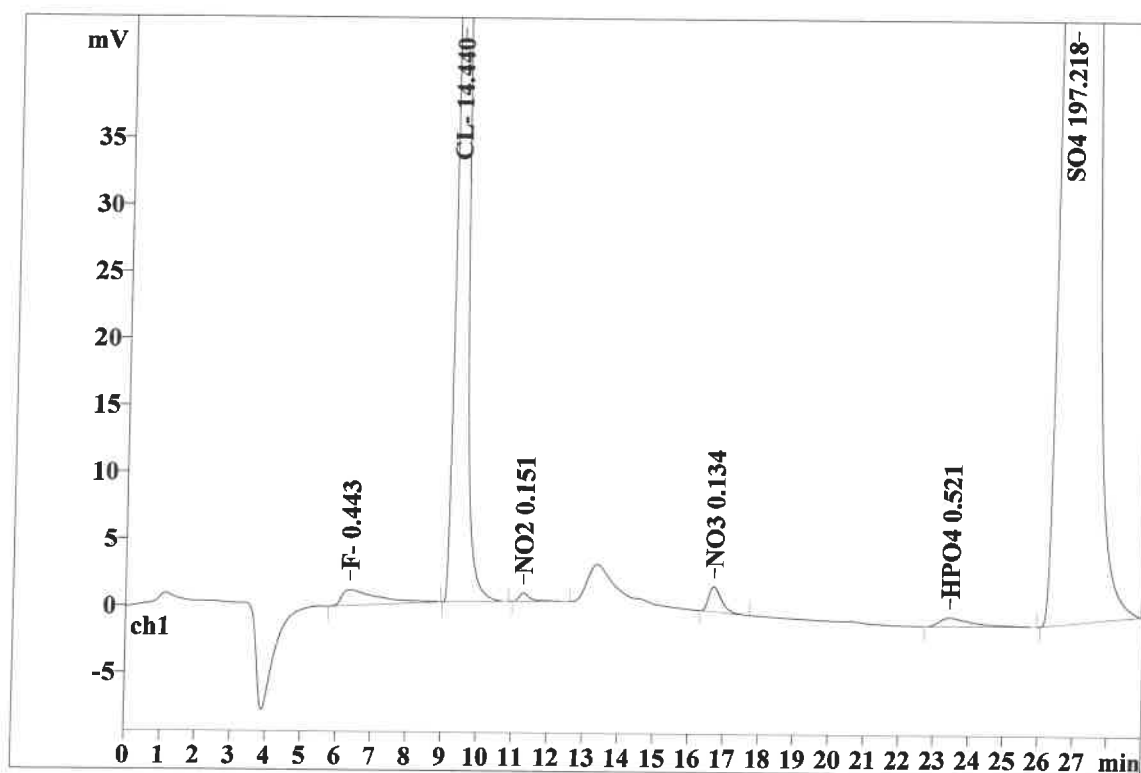

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.36	0.991	1.18	0.15	84.122	0.32
2	9.35	0.219	144.03	17.99	2212.432	8.52
3	11.28	0.290	0.64	0.08	14.797	0.06
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.69	0.384	1.90	0.24	48.423	0.19
6	23.44	0.926	0.65	0.08	43.239	0.17
7	26.79	0.555	652.15	81.46	23560.436	90.74
7	29.00	0.481	800.55	100.00	25963.449	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/17/2023 10:14:07 AM
Printed by: wet


Ident: 01923-01MS
Analysis from: 3/16/2023 12:41:55 PM
File: _2023-03-16_

Last save: 3/16/2023 1:10:55 PM

Method: AnionsIC2-022123.mtw
Run operator: wet
Analysis number: 33577

Last save: 2/24/2023 11:36

SAMPLE:
: IZ/MA
Vial number: 26
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

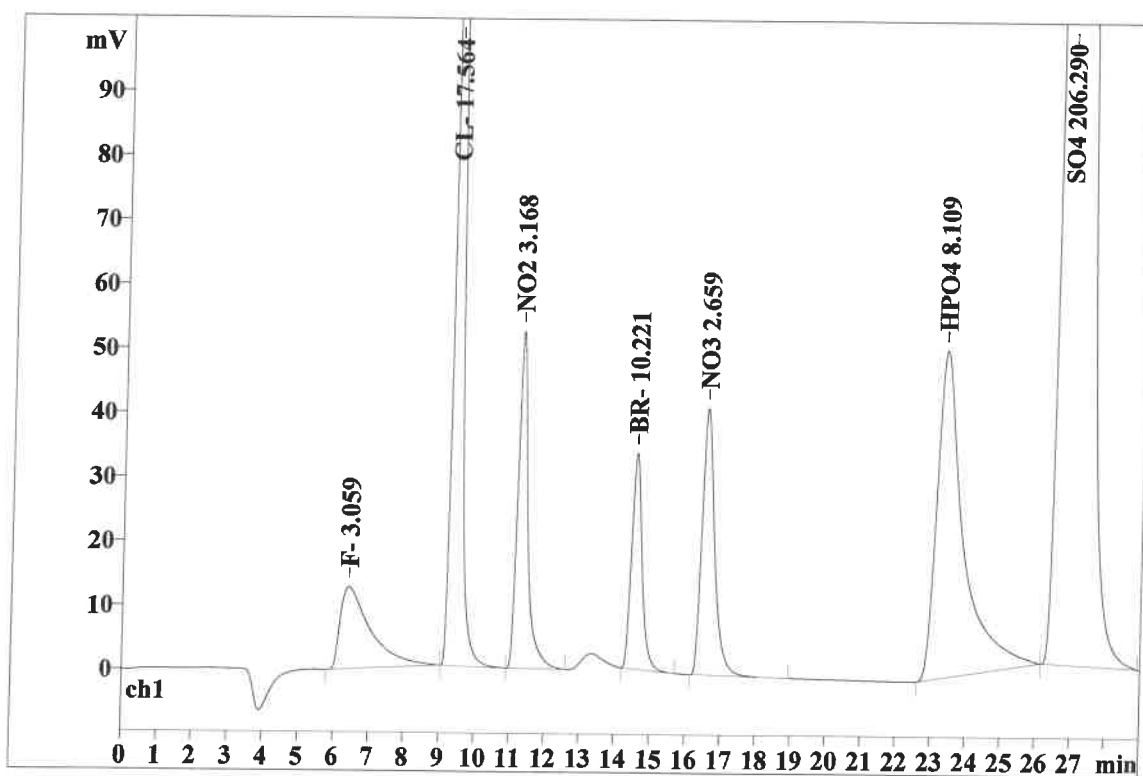

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.39	0.850	12.72	1.22	765.926	2.28
2	9.36	0.218	175.93	16.85	2690.085	8.00
3	11.26	0.287	52.45	5.02	1066.634	3.17
4	14.54	0.308	33.63	3.22	691.775	2.06
5	16.53	0.375	41.50	3.97	1047.591	3.12
6	23.33	0.691	50.96	4.88	2715.160	8.08
7	26.87	0.559	677.16	64.84	24644.258	73.30
7	29.00	0.470	1044.35	100.00	33621.429	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/17/2023 10:14:17 AM
Printed by: wet


Ident: 01923-01MSD
Analysis from: 3/16/2023 1:13:33 PM
File: _2023-03-16_

Last save: 3/16/2023 1:42:40 PM

Method: AnionsIC2-022123.mtw
Run operator: wet
Analysis number: 33578

Last save: 2/24/2023 11:36

SAMPLE: ·
: IZ/MA
Vial number: 27
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

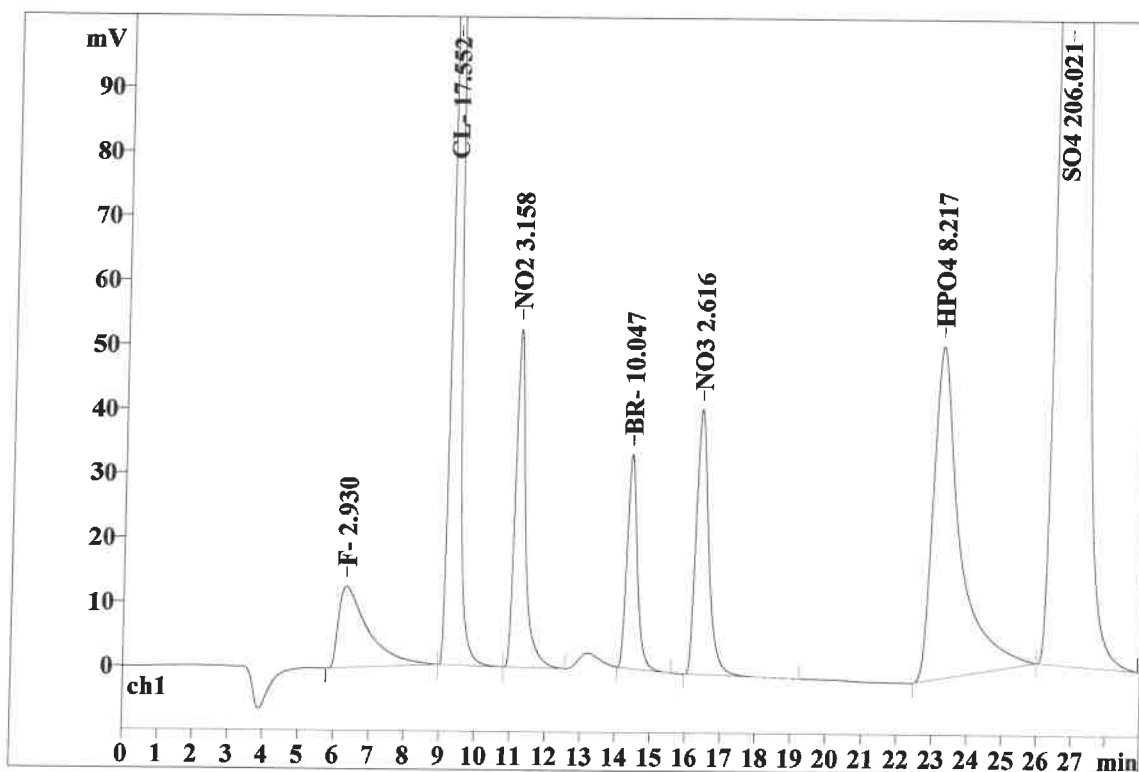

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.32	0.810	12.61	1.21	732.294	2.18
2	9.28	0.216	177.45	16.97	2688.279	8.01
3	11.16	0.284	52.61	5.03	1063.222	3.17
4	14.39	0.306	33.28	3.18	679.718	2.03
5	16.36	0.371	41.22	3.94	1030.532	3.07
6	23.17	0.690	51.71	4.94	2753.170	8.20
7	26.69	0.558	677.07	64.73	24612.047	73.34
7	29.00	0.462	1045.94	100.00	33559.262	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/17/2023 10:15:04 AM
 Printed by: wet


Ident: O1935-02
 Analysis from: 3/16/2023 2:17:07 PM
 File: _2023-03-16_

Last save: 3/17/2023 10:14:57 AM

Method: AnionsIC2-022123.mtw
 Run operator: wet
 Analysis number: 33580

Last save: 2/24/2023 11:36

SAMPLE:
 : IZ/MA
 Vial number: 15
 Volume: 20.0 µL
 Dilution: 1.00
 Amount: 1.0000

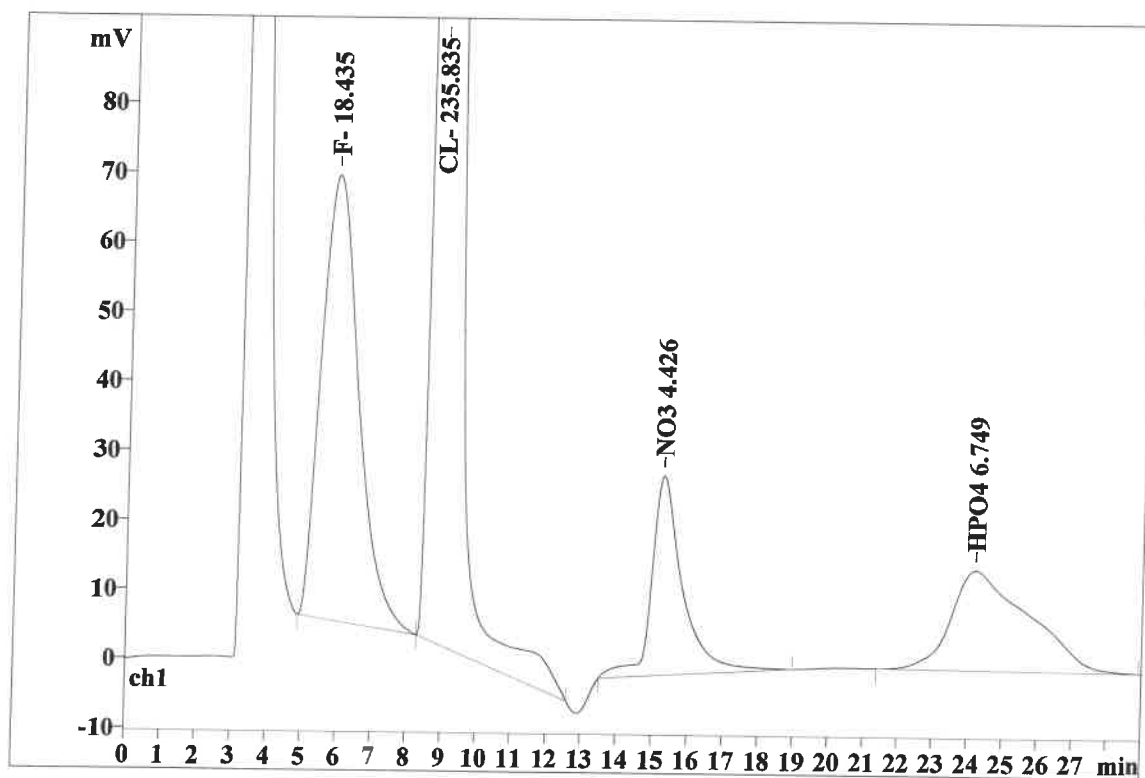

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.83	1.156	64.09	4.69	4773.599	10.65
2	8.85	0.420	1259.02	92.16	36068.763	80.46
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	15.24	0.787	28.68	2.10	1746.967	3.90
6	24.19	2.545	14.40	1.05	2236.322	4.99
7	0.00	0.000	0.00	0.00	0.000	0.00
7	29.00	0.701	1366.20	100.00	44825.651	100.00

This report has been created by IC Net
 METROHM LTD

Report date: 3/17/2023 10:16:34 AM
Printed by: wet


Ident: O1935-02DLX5
Analysis from: 3/16/2023 2:48:47 PM
File: _2023-03-16_

Last save: 3/17/2023 10:16:31 AM

Method: AnionsIC2-022123.mtw
Run operator: wet
Analysis number: 33581

Last save: 2/24/2023 11:36

SAMPLE:
: IZ/MA
Vial number: 18
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

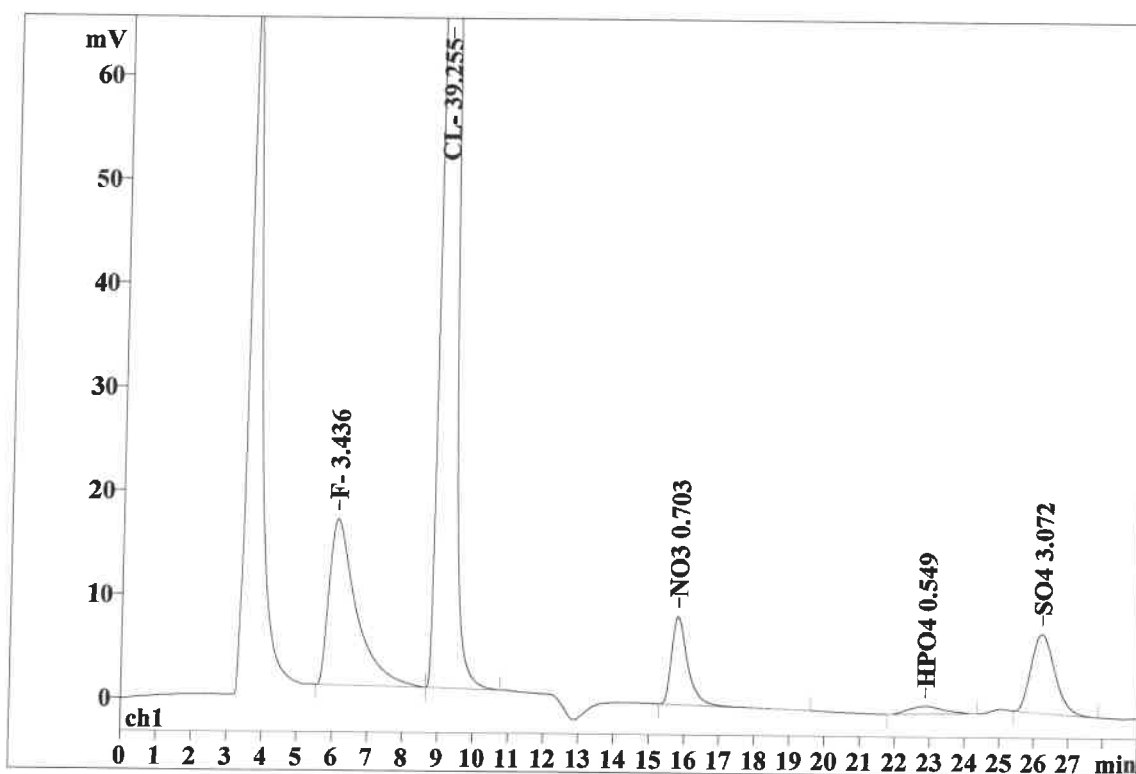

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.08	0.764	15.99	4.39	864.349	11.42
2	9.06	0.265	331.12	90.97	6007.143	79.40
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	15.78	0.465	8.49	2.33	273.672	3.62
6	22.85	1.129	0.75	0.21	53.156	0.70
7	26.19	0.751	7.60	2.09	367.407	4.86
7	29.00	0.482	363.96	100.00	7565.728	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/17/2023 10:17:47 AM
Printed by: wet


Ident: CCV
Analysis from: 3/16/2023 6:29:27 PM
File: _2023-03-16_

Last save: 3/16/2023 6:58:28 PM

Method: AnionsIC2-022123.mtw
Run operator: wet
Analysis number: 33588

Last save: 2/24/2023 11:36

SAMPLE:
: IZ/MA
Vial number: 22
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

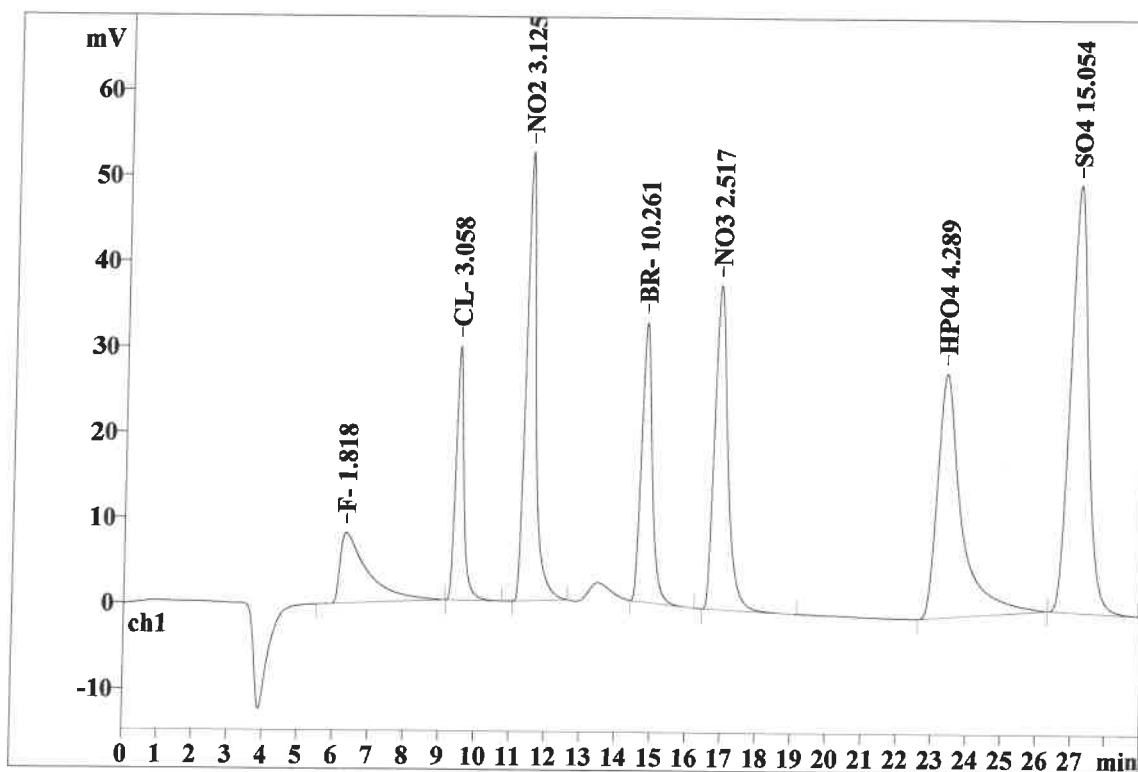

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.32	0.717	8.24	3.44	442.656	6.49
2	9.46	0.230	29.68	12.40	471.793	6.92
3	11.41	0.287	52.43	21.91	1051.565	15.42
4	14.76	0.318	32.65	13.64	694.543	10.18
5	16.84	0.389	37.87	15.83	991.478	14.54
6	23.31	0.628	28.48	11.90	1370.139	20.09
7	27.07	0.545	49.93	20.87	1798.842	26.37
7	29.00	0.445	239.29	100.00	6821.016	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/17/2023 10:18:04 AM
Printed by: wet


Ident: CCB
Analysis from: 3/16/2023 7:01:09 PM
File: _2023-03-16_

Last save: 3/17/2023 10:18:01 AM

Method: AnionsIC2-022123.mtw
Run operator: wet
Analysis number: 33589

Last save: 2/24/2023 11:36

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

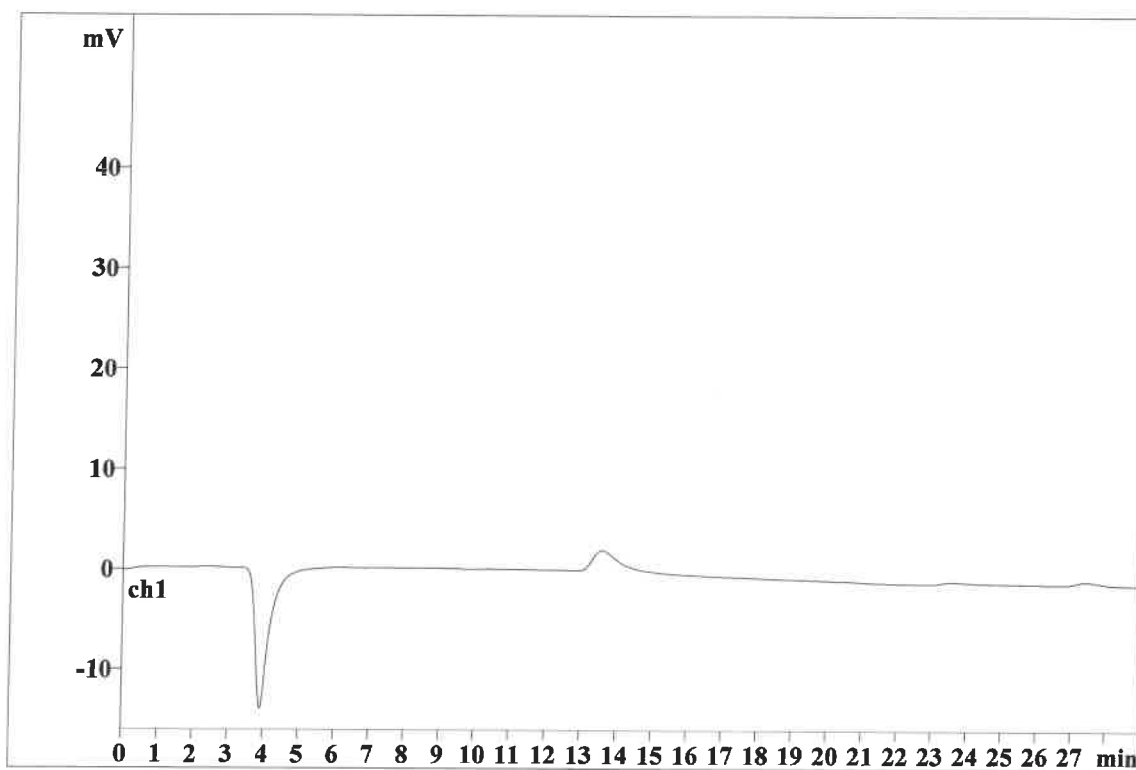

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD