


LB124587 INSTRUMENT: CV1

7471B

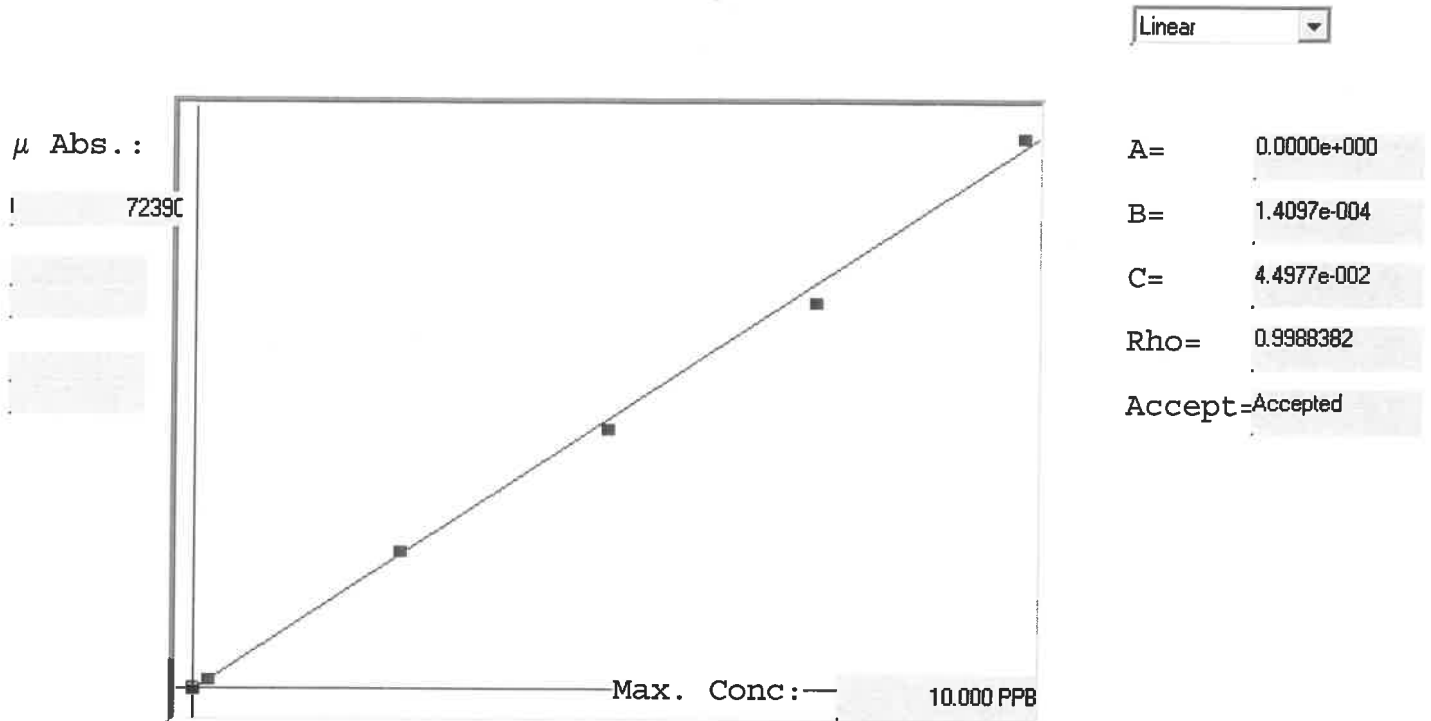

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	
0.0	0.000	0.044	0.044	-10	0.000	-10					1.00
0.2	0.200	0.240	0.040	1386	0.0 %	1386					20
2.5	2.500	2.612	0.112	18208	0.0 %	18208					4.5
5.0	5.000	4.854	-0.146	34111	0.0 %	34111					-3
7.5	7.500	7.200	-0.300	50757	0.0 %	50757					-4
10.0	10.000	10.250	0.250	72390	0.0 %	72390					3

LB124587 INSTRUMENT ID:CV1

Method: 7471B

Operator: Admin

Date of Analysis: 20 Mar 2023 18:48:23

Sample ID	Extended ID	µ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	-10	-	0.0000	7471B	PPB	20 Mar 2023 19:20:00	S	Std
0.2 - 1	50.2	1386	-	0.2000	7471B	PPB	20 Mar 2023 19:22:16	S	Std
2.5 - 1	52.5	18208	-	2.5000	7471B	PPB	20 Mar 2023 19:24:35	S	Std
5.0 - 1	55.0	34111	-	5.0000	7471B	PPB	20 Mar 2023 19:29:24	S	Std
7.5 - 1	57.5	50757	-	7.5000	7471B	PPB	20 Mar 2023 19:31:40	S	Std
10.0 - 1	59.0	72390	-	10.0000	7471B	PPB	20 Mar 2023 19:51:41	S	Std
ICV100 - 1	ICV100	27620	3.9387	-	7471B	PPB	20 Mar 2023 19:54:48	U	SMPL
ICB100 - 1	ICB100	5	0.0457	-	7471B	PPB	20 Mar 2023 19:57:03	U	SMPL
CCV08 - 1	CCV08	34216	4.8685	-	7471B	PPB	20 Mar 2023 20:02:25	U	SMPL
CCB08 - 1	CCB08	18	0.0475	-	7471B	PPB	20 Mar 2023 20:04:40	U	SMPL
CRA - 1	CRA	1224	0.2175	-	7471B	PPB	20 Mar 2023 20:12:13	U	SMPL
HighStd - 1	HighStd	71159	10.0766	-	7471B	PPB	20 Mar 2023 20:14:28	U	SMPL
ChkStd - 1	ChkStd	44302	6.2904	-	7471B	PPB	20 Mar 2023 20:16:43	U	SMPL
PB151539BL - 1	PB151539BL	-133	0.0262	-	7471B	PPB	20 Mar 2023 20:19:02	U	SMPL
PB151539BS - 1	PB151539BS	27612	3.9376	-	7471B	PPB	20 Mar 2023 20:21:20	U	SMPL
O1924-01 - 1	RB21136	2393	0.3823	-	7471B	PPB	20 Mar 2023 20:23:36	U	SMPL
O1924-01DUP - 1	RB21136DUP	2138	0.3464	-	7471B	PPB	20 Mar 2023 20:25:54	U	SMPL
O1924-01MS - 1	RB21136MS	23057	3.2954	-	7471B	PPB	20 Mar 2023 20:28:11	U	SMPL
O1924-01MSD - 1	RB21136MSD	22688	3.2434	-	7471B	PPB	20 Mar 2023 20:30:29	U	SMPL
O1924-03 - 1	CHRT26700	327	0.0911	-	7471B	PPB	20 Mar 2023 20:32:46	U	SMPL
CCV09 - 1	CCV09	34251	4.8735	-	7471B	PPB	20 Mar 2023 20:35:03	U	SMPL
CCB09 - 1	CCB09	-18	0.0424	-	7471B	PPB	20 Mar 2023 20:37:18	U	SMPL
O1924-05 - 1	CHRT27051	553	0.1229	-	7471B	PPB	20 Mar 2023 20:39:35	U	SMPL
O1928-01 - 1	031423-1	2071	0.3369	-	7471B	PPB	20 Mar 2023 20:41:51	U	SMPL
O1936-01 - 1	OR-03152023	4183	0.6347	-	7471B	PPB	20 Mar 2023 20:44:07	U	SMPL
O1939-04 - 1	20071	1024	0.1893	-	7471B	PPB	20 Mar 2023 20:46:23	U	SMPL
O1954-01 - 1	SV-TP1-0316	911	0.1734	-	7471B	PPB	20 Mar 2023 20:48:39	U	SMPL
O1954-03 - 1	SV-TP2-0316	823	0.1610	-	7471B	PPB	20 Mar 2023 20:50:55	U	SMPL
O1954-05 - 1	SV-TP3-0316	751	0.1508	-	7471B	PPB	20 Mar 2023 20:53:12	U	SMPL
O1954-07 - 1	SV-TP4-0316	6891	1.0164	-	7471B	PPB	20 Mar 2023 20:55:29	U	SMPL
O1954-09 - 1	SV-TP5-0316	6423	0.9505	-	7471B	PPB	20 Mar 2023 20:57:47	U	SMPL
O1964-01 - 1	UNION-2	6432	0.9517	-	7471B	PPB	20 Mar 2023 21:00:03	U	SMPL
CCV10 - 1	CCV10	37037	5.2662	-	7471B	PPB	20 Mar 2023 21:05:57	U	SMPL
CCB10 - 1	CCB10	-42	0.0391	-	7471B	PPB	20 Mar 2023 21:08:13	U	SMPL
O1964-04 - 1	MAPLE-4	13983	2.0162	-	7471B	PPB	20 Mar 2023 21:10:30	U	SMPL
O1964-07 - 1	MAPLE-5	2305	0.3699	-	7471B	PPB	20 Mar 2023 21:12:46	U	SMPL
O1964-10 - 1	MAPLE-6	3120	0.4848	-	7471B	PPB	20 Mar 2023 21:15:02	U	SMPL
O1965-01 - 1	COMP-1	2218	0.3577	-	7471B	PPB	20 Mar 2023 21:17:18	U	SMPL
O1965-02 - 1	COMP-2	1720	0.2875	-	7471B	PPB	20 Mar 2023 21:19:34	U	SMPL
O1965-03 - 1	COMP-3	4483	0.6770	-	7471B	PPB	20 Mar 2023 21:21:51	U	SMPL
O1974-01 - 1	SHELL-ROAD-1	11262	1.6326	-	7471B	PPB	20 Mar 2023 21:24:09	U	SMPL
O1974-04 - 1	SHELL-ROAD-2	11845	1.7148	-	7471B	PPB	20 Mar 2023 21:26:26	U	SMPL
PB151540BL - 1	PB151540BL	28	0.0489	-	7471B	PPB	20 Mar 2023 21:28:43	U	SMPL
PB151540BS - 1	PB151540BS	0	0.0450	-	7471B	PPB	20 Mar 2023 21:30:59	U	SMPL
CCV11 - 1	CCV11	37333	5.3080	-	7471B	PPB	20 Mar 2023 21:33:15	U	SMPL
CCB11 - 1	CCB11	-43	0.0389	-	7471B	PPB	20 Mar 2023 21:35:31	U	SMPL
O1932-03 - 1	CE-86B-031423	53687	7.6135	-	7471B	PPB	20 Mar 2023 21:37:48	U	SMPL
O1932-03DUP - 1	CE-86B-031423DUP	53270	7.5547	-	7471B	PPB	20 Mar 2023 21:40:05	U	SMPL
O1932-03MS - 1	CE-86B-031423MS	34769	4.9465	-	7471B	PPB	20 Mar 2023 21:42:22	U	SMPL
O1932-03MSD - 1	CE-86B-031423MSD	35061	4.9877	-	7471B	PPB	20 Mar 2023 21:44:41	U	SMPL
O1932-07 - 1	CE-81-031423	21696	3.1036	-	7471B	PPB	20 Mar 2023 21:46:59	U	SMPL
O1932-11 - 1	CE-43-031423	44740	6.3522	-	7471B	PPB	20 Mar 2023 21:49:17	U	SMPL
O1932-15 - 1	JPP-6A-031423	68254	9.6670	-	7471B	PPB	20 Mar 2023 21:51:34	U	SMPL
O1932-19 - 1	JPP-6C-031423	24660	3.5214	-	7471B	PPB	20 Mar 2023 21:53:53	U	SMPL
O1944-01 - 1	MC-1	1180	0.2113	-	7471B	PPB	20 Mar 2023 21:56:13	U	SMPL
O1963-01 - 1	NYE-SOIL-0316	107660	15.2222	-	7471B	PPB	20 Mar 2023 21:58:30	U	SMPL
CCV12 - 1	CCV12	37192	5.2881	-	7471B	PPB	20 Mar 2023 22:00:45	U	SMPL
CCB12 - 1	CCB12	-19	0.0423	-	7471B	PPB	20 Mar 2023 22:03:04	U	SMPL
O1998-01 - 1	BRAOD-CHANNEL-SUBSTATION-TP1	21454	3.0694	-	7471B	PPB	20 Mar 2023 22:05:21	U	SMPL
O1998-03 - 1	BRAOD-CHANNEL-SUBSTATION-TP2	20088	2.8769	-	7471B	PPB	20 Mar 2023 22:07:37	U	SMPL
O1998-05 - 1	10TH-ST-SUBSTATION-TP1	196115	27.6921	-	7471B	PPB	20 Mar 2023 22:09:54	U	SMPL
O1998-07 - 1	10TH-ST-SUBSTATION-TP2	175083	24.7271	-	7471B	PPB	20 Mar 2023 22:12:11	U	SMPL
O2001-01 - 1	IRV-1	4923	0.7390	-	7471B	PPB	20 Mar 2023 22:14:32	U	SMPL
O2001-04 - 1	IRV-2	14292	2.0598	-	7471B	PPB	20 Mar 2023 22:16:51	U	SMPL
O2001-07 - 1	IRV-3	1854	0.3063	-	7471B	PPB	20 Mar 2023 22:19:08	U	SMPL
O2002-01 - 1	031023-3	1291	0.2270	-	7471B	PPB	20 Mar 2023 22:21:26	U	SMPL
O1924-01LX5 - 1		-23	0.0417	-	7471B	PPB	20 Mar 2023 22:23:43	U	SMPL
O1932-03LX5 - 1		9846	1.4330	-	7471B	PPB	20 Mar 2023 22:25:58	U	SMPL
CCV13 - 1	CCV13	37410	5.3188	-	7471B	PPB	20 Mar 2023 22:28:14	U	SMPL
CCB13 - 1	CCB13	-63	0.0361	-	7471B	PPB	20 Mar 2023 22:30:31	U	SMPL
O1963-01DLX5 - 1		20444	2.9271	-	7471B	PPB	20 Mar 2023 22:32:48	U	SMPL
O1998-05DLX5 - 1		37714	5.3617	-	7471B	PPB	20 Mar 2023 22:35:05	U	SMPL
O1998-07DLX5 - 1		25532	3.6443	-	7471B	PPB	20 Mar 2023 22:37:22	U	SMPL
CCV14 - 1	CCV14	36368	5.1719	-	7471B	PPB	20 Mar 2023 22:39:40	U	SMPL
CCB14 - 1	CCB14	-68	0.0354	-	7471B	PPB	20 Mar 2023 22:41:59	U	SMPL