

LB124649


INSTRUMENT : CV1

7470A

Linear

 μ Abs.:

32025

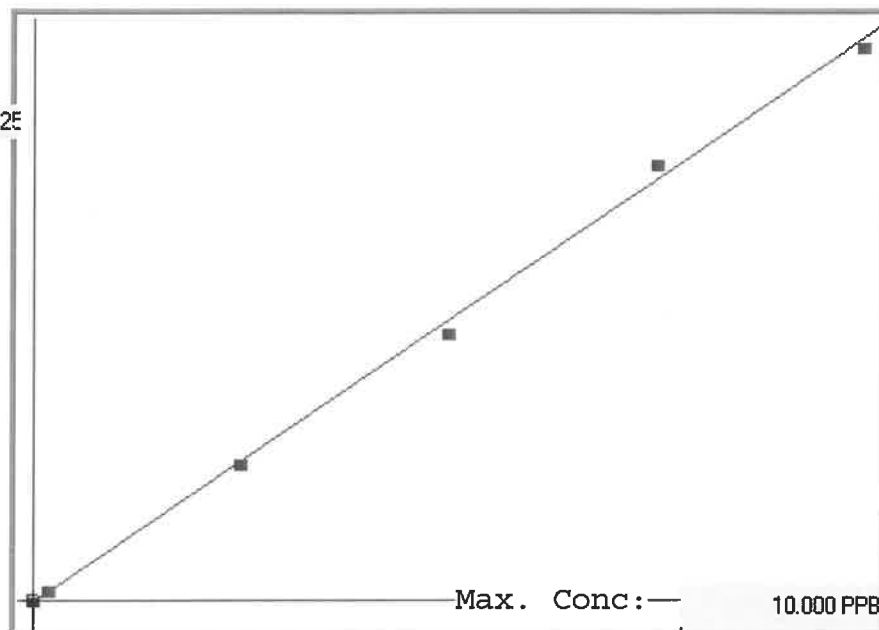

A= 0.0000e+000

B= 3.0718e-004

C= 4.3218e-002

Rho= 0.9990954

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	y.D
0.0	0.000	0.042	0.042	-4	0.000	-4	0				15
0.2	0.200	0.230	0.030	609	0.0 %	609					-1
2.5	2.500	2.469	-0.031	7897	0.0 %	7897					-4
5.0	5.000	4.787	-0.213	15444	0.0 %	15444					4
7.5	7.500	7.791	0.291	25222	0.0 %	25222					-1
10.0	10.000	9.881	-0.119	32025	0.0 %	32025					

LB124649 INSTRUMENT ID:CV1

Method: 7470A

Operator: Admin

Date of Analysis: 23 Mar 2023 15:47:38

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	-	-	0.0000	7470A	PPB	23 Mar 2023 16:11:18	S	Std
0.2 - 1	50.2	609	-	0.2000	7470A	PPB	23 Mar 2023 16:13:35	S	Std
2.5 - 1	52.5	7897	-	2.5000	7470A	PPB	23 Mar 2023 16:15:52	S	Std
5.0 - 1	55.0	15444	-	5.0000	7470A	PPB	23 Mar 2023 16:18:10	S	Std
7.5 - 1	57.5	25222	-	7.5000	7470A	PPB	23 Mar 2023 16:20:26	S	Std
10.0 - 1	59.0	32025	-	10.0000	7470A	PPB	23 Mar 2023 16:35:54	S	Std
ICV01 - 1	ICV01	13447	4.1738	-	7470A	PPB	23 Mar 2023 16:42:55	U	SMPL
ICB01 - 1	ICB01	-16	0.0383	-	7470A	PPB	23 Mar 2023 16:45:10	U	SMPL
CCV01 - 1	CCV01	14652	4.5440	-	7470A	PPB	23 Mar 2023 16:51:33	U	SMPL
CCB01 - 1	CCB01	1	0.0435	-	7470A	PPB	23 Mar 2023 16:53:48	U	SMPL
CRA - 1	CRA	592	0.2251	-	7470A	PPB	23 Mar 2023 16:56:04	U	SMPL
HighStd - 1	HighStd	29165	9.0021	-	7470A	PPB	23 Mar 2023 16:58:20	U	SMPL
ChkStd - 1	ChkStd	21000	6.4940	-	7470A	PPB	23 Mar 2023 17:00:35	U	SMPL
PB151634BL - 1	PBW	-5	0.0417	-	7470A	PPB	23 Mar 2023 17:02:53	U	SMPL
PB151634BS - 1	LCSW	11762	3.6562	-	7470A	PPB	23 Mar 2023 17:05:10	U	SMPL
O2020-02 - 1	SP-1	12	0.0469	-	7470A	PPB	23 Mar 2023 17:07:27	U	SMPL
O2020-12 - 1	SP-2	62	0.0623	-	7470A	PPB	23 Mar 2023 17:09:44	U	SMPL
O2020-22 - 1	SP-3	49	0.0583	-	7470A	PPB	23 Mar 2023 17:12:02	U	SMPL
O2020-32 - 1	SP-4	23	0.0503	-	7470A	PPB	23 Mar 2023 17:14:19	U	SMPL
O2021-04 - 1	JPP-6E-032023	10	0.0463	-	7470A	PPB	23 Mar 2023 17:16:35	U	SMPL
CCV02 - 1	CCV02	15289	4.7397	-	7470A	PPB	23 Mar 2023 17:22:12	U	SMPL
CCB02 - 1	CCB02	-40	0.0309	-	7470A	PPB	23 Mar 2023 17:24:26	U	SMPL
O2021-08 - 1	JPP-6D-032023	24	0.0506	-	7470A	PPB	23 Mar 2023 17:26:43	U	SMPL
O2021-12 - 1	JPP-46A-032023	37	0.0546	-	7470A	PPB	23 Mar 2023 17:28:59	U	SMPL
O2021-16 - 1	JPP-46B-032023	34	0.0537	-	7470A	PPB	23 Mar 2023 17:31:15	U	SMPL
O2023-02 - 1	TP-11-TEST-PIT-ON-CENTRAL	56	0.0604	-	7470A	PPB	23 Mar 2023 17:33:31	U	SMPL
O2023-04 - 1	TP-12-TEST-PIT-ON-OCEAN	24	0.0506	-	7470A	PPB	23 Mar 2023 17:35:47	U	SMPL
O2023-06 - 1	TP-13-TEST-PIT-ON-GRAVELLY	-21	0.0368	-	7470A	PPB	23 Mar 2023 17:38:03	U	SMPL
O2032-03 - 1	S-2	978	0.3436	-	7470A	PPB	23 Mar 2023 17:40:20	U	SMPL
O2032-03DUP - 1	S-2DUP	1004	0.3516	-	7470A	PPB	23 Mar 2023 17:42:37	U	SMPL
O2032-03MS - 1	S-2MS	12021	3.7358	-	7470A	PPB	23 Mar 2023 17:44:54	U	SMPL
O2032-03MSD - 1	S-2MSD	11933	3.7088	-	7470A	PPB	23 Mar 2023 17:47:10	U	SMPL
CCV03 - 1	CCV03	15828	4.9046	-	7470A	PPB	23 Mar 2023 17:49:26	U	SMPL
CCB03 - 1	CCB03	-54	0.0266	-	7470A	PPB	23 Mar 2023 17:51:44	U	SMPL
PB151635BL - 1	PBW	50	0.0586	-	7470A	PPB	23 Mar 2023 17:54:01	U	SMPL
PB151635BS - 1	LCSW	14520	4.5034	-	7470A	PPB	23 Mar 2023 17:56:17	U	SMPL
O2036-02 - 1	72-11939	-33	0.0331	-	7470A	PPB	23 Mar 2023 17:58:33	U	SMPL
O2045-07 - 1	WC1-20230322	212	0.1083	-	7470A	PPB	23 Mar 2023 18:00:50	U	SMPL
O2045-07DUP - 1	WC1-20230322DUP	216	0.1096	-	7470A	PPB	23 Mar 2023 18:03:06	U	SMPL
O2045-07MS - 1	WC1-20230322MS	10589	3.2959	-	7470A	PPB	23 Mar 2023 18:05:22	U	SMPL
O2045-07MSD - 1	WC1-20230322MSD	11852	3.6839	-	7470A	PPB	23 Mar 2023 18:07:39	U	SMPL
O2032-03LX5 - 1		121	0.0804	-	7470A	PPB	23 Mar 2023 18:09:57	U	SMPL
O2032-03A - 1		13569	4.2113	-	7470A	PPB	23 Mar 2023 18:17:39	U	SMPL
O2045-07LX5 - 1		-81	0.0183	-	7470A	PPB	23 Mar 2023 18:19:55	U	SMPL
CCV04 - 1	CCV04	16527	5.1199	-	7470A	PPB	23 Mar 2023 18:22:12	U	SMPL
CCB04 - 1	CCB04	-29	0.0343	-	7470A	PPB	23 Mar 2023 18:24:28	U	SMPL
O2045-07A - 1		14096	4.3732	-	7470A	PPB	23 Mar 2023 18:26:46	U	SMPL
PB151585TB - 1		-42	0.0303	-	7470A	PPB	23 Mar 2023 18:29:01	U	SMPL
PB151617TB - 1		2	0.0438	-	7470A	PPB	23 Mar 2023 18:34:01	U	SMPL
CCV05 - 1	CCV05	16968	5.2554	-	7470A	PPB	23 Mar 2023 18:36:16	U	SMPL
CCB05 - 1	CCB05	-29	0.0343	-	7470A	PPB	23 Mar 2023 18:38:32	U	SMPL