

=====

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

3/27/2023 13:00

Test: Total CN

Sample Id	<i>mg/L</i> Result	Dil. 1 +	Response	Errors
ICV1	92.751	0.0	0.070	
ICB1	2.198	0.0	0.002	
CCV1	242.292	0.0	0.183	
CCB1	1.883	0.0	0.001	
PB151733BL	2.174	0.0	0.002	
O2068-01	2.155	0.0	0.002	
O2068-01DUP	2.112	0.0	0.002	
O2070-04	1.691	0.0	0.001	
O2102-02	1.925	0.0	0.001	
O2107-02	1.833	0.0	0.001	
O2070-02	2.248	0.0	0.002	
CCV2	249.103	0.0	0.188	
CCB2	2.161	0.0	0.002	

N	13
Mean	46.502
SD	91.8742
CV%	197.57

Aquakem v. 7.2AQ1

Results from time period:

Mon Mar 27 12:51:47 2023

Mon Mar 27 12:58:05 2023

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	1.5503	µg/l	3/27/2023 10:39:14	
5.0PPBCN	A	Total CN	P	5.1323	µg/l	3/27/2023 10:39:15	
10PPBCN	A	Total CN	P	10.2965	µg/l	3/27/2023 10:39:16	
50PPBCN	A	Total CN	P	49.0847	µg/l	3/27/2023 10:39:17	
100PPBCN	A	Total CN	P	98.1843	µg/l	3/27/2023 10:39:18	
250PPBCN	A	Total CN	P	250.609	µg/l	3/27/2023 10:39:19	
500PPBCN	A	Total CN	P	500.1429	µg/l	3/27/2023 10:39:20	
ICV1	S	Total CN	P	92.751	µg/l	3/27/2023 12:51:47	
ICB1	S	Total CN	P	2.1982	µg/l	3/27/2023 12:51:50	
CCV1	S	Total CN	P	242.2917	µg/l	3/27/2023 12:51:51	
CCB1	S	Total CN	P	1.883	µg/l	3/27/2023 12:51:54	
PB151733BL	S	Total CN	P	2.1741	µg/l	3/27/2023 12:51:56	
O2068-01	S	Total CN	P	2.1553	µg/l	3/27/2023 12:51:57	
O2068-01DUP	S	Total CN	P	2.1116	µg/l	3/27/2023 12:57:58	
O2070-04	S	Total CN	P	1.6909	µg/l	3/27/2023 12:58:00	
O2102-02	S	Total CN	P	1.9251	µg/l	3/27/2023 12:58:01	
O2107-02	S	Total CN	P	1.8334	µg/l	3/27/2023 12:58:02	
O2070-02	S	Total CN	P	2.2483	µg/l	3/27/2023 12:58:03	
CCV2	S	Total CN	P	249.1029	µg/l	3/27/2023 12:58:04	
CCB2	S	Total CN	P	2.1614	µg/l	3/27/2023 12:58:05	

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

3/27/2023 10:39


Test Total CN

Accepted 3/27/2023 10:39

Factor 1325
Bias 0

Coeff. of det. 0.999966

Errors

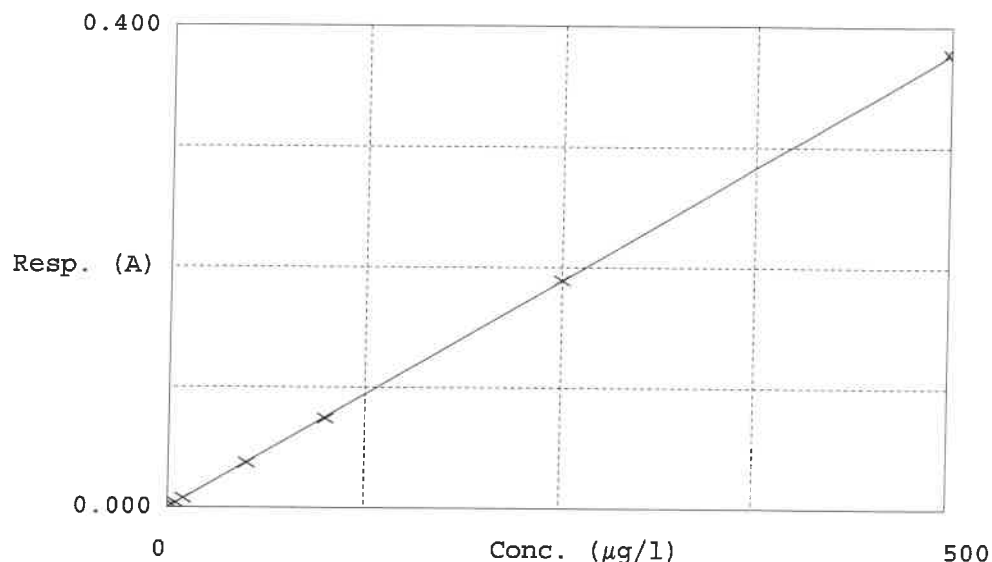

	Calibrator	Response	Calc. con.	Conc.	Re Errors
1	0.0PPBCN	0.001	1.5503	0.0000	-
2	5.0PPBCN	0.004	5.1323	5.0000	2.6
3	10PPBCN	0.008	10.2965	10.0000	3.0
4	50PPBCN	0.037	49.0847	50.0000	-1.8
5	100PPBCN	0.074	98.1843	100.0000	-1.8
6	250PPBCN	0.189	250.6090	250.0000	0.2
7	500PPBCN	0.378	500.1429	500.0000	0.0

12
3/27/23