


LB124708 INSTRUMENT: CU)

7470A

Linear

μ Abs.:

42261

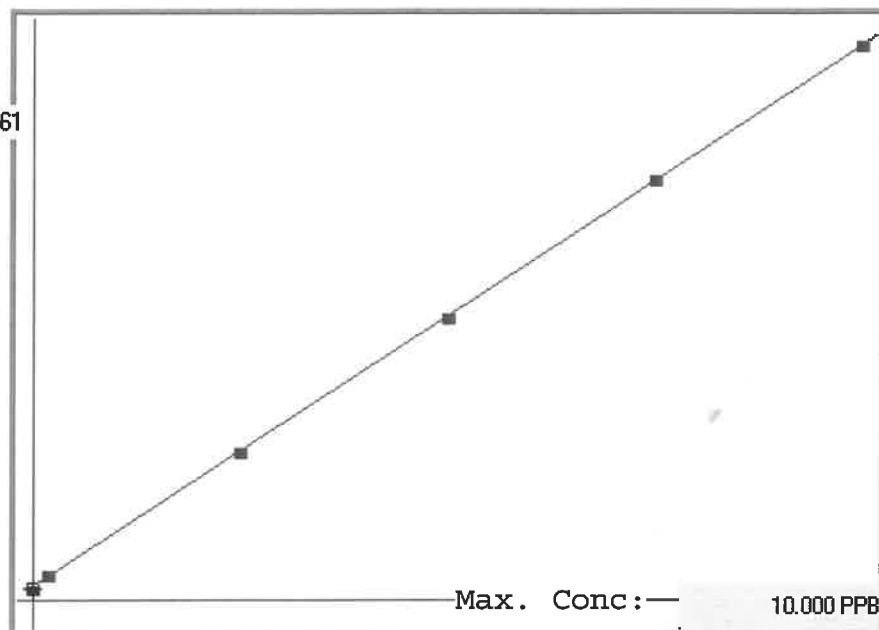

A= 0.0000e+000

B= 2.4252e-004

C= -2.5301e-001

Rho= 0.9999749

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.023	-0.023	948	0.000	948	0				
0.2	0.200	0.243	0.043	2045	0.0 %	2045					
2.5	2.500	2.484	-0.016	11287	0.0 %	11287					
5.0	5.000	4.973	-0.027	21549	0.0 %	21549					
7.5	7.500	7.527	0.027	32080	0.0 %	32080					
10.0	10.000	9.996	-0.004	42261	0.0 %	42261					

9.0
22
7
1
0.0

LB124708, INSTRUMENT ID: CV1

Method: 7470A

Operator: Admin

Date of Analysis: 27 Mar 2023 19:08:59

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	30.0	948	-	0.0000	7470A	PPB	27 Mar 2023 19:12:58	S	Std
0.2 - 1	50.2	2045	-	0.2000	7470A	PPB	27 Mar 2023 19:15:15	S	Std
2.5 - 1	52.5	11287	-	2.5000	7470A	PPB	27 Mar 2023 19:17:32	S	Std
5.0 - 1	55.0	21549	-	5.0000	7470A	PPB	27 Mar 2023 19:19:49	S	Std
7.5 - 1	57.5	32080	-	7.5000	7470A	PPB	27 Mar 2023 19:22:06	S	Std
10.0 - 1	59.0	42261	-	10.0000	7470A	PPB	27 Mar 2023 19:24:22	S	Std
ICV03 - 1	ICV03	18489	4.2309	-	7470A	PPB	27 Mar 2023 19:32:50	U	SMPL
ICB03 - 1	ICB03	849	-0.0471	-	7470A	PPB	27 Mar 2023 19:35:05	U	SMPL
CCV11 - 1	CCV11	23416	5.4258	-	7470A	PPB	27 Mar 2023 19:41:28	U	SMPL
CCB11 - 1	CCB11	826	-0.0527	-	7470A	PPB	27 Mar 2023 19:43:43	U	SMPL
CRA - 1	CRA	1945	0.2187	-	7470A	PPB	27 Mar 2023 19:45:58	U	SMPL
HighStd - 1	HighStd	40294	9.5190	-	7470A	PPB	27 Mar 2023 19:48:14	U	SMPL
ChkStd - 1	ChkStd	26806	6.2479	-	7470A	PPB	27 Mar 2023 19:50:29	U	SMPL
PB151738BL - 1	PBW	718	-0.0789	-	7470A	PPB	27 Mar 2023 19:52:46	U	SMPL
PB151738BS - 1	LCSW	17529	3.9981	-	7470A	PPB	27 Mar 2023 19:55:03	U	SMPL
O2047-02 - 1	R-PIT	798	-0.0595	-	7470A	PPB	27 Mar 2023 19:57:19	U	SMPL
O2058-02 - 1	CHAMBER-B-72-EAST	986	-0.0139	-	7470A	PPB	27 Mar 2023 19:59:36	U	SMPL
O2068-01 - 1	CONCRETE-TCLP	967	-0.0185	-	7470A	PPB	27 Mar 2023 20:01:53	U	SMPL
O2070-02 - 1	SOILPILE-1-0323	998	-0.0110	-	7470A	PPB	27 Mar 2023 20:04:10	U	SMPL
O2070-04 - 1	SOILPILE-2-0323	825	-0.0529	-	7470A	PPB	27 Mar 2023 20:06:25	U	SMPL
CCV12 - 1	CCV12	21391	4.9347	-	7470A	PPB	27 Mar 2023 20:08:41	U	SMPL
CCB12 - 1	CCB12	714	-0.0798	-	7470A	PPB	27 Mar 2023 20:10:56	U	SMPL
O2070-04DUP - 1	SOILPILE-2-0323DUP	783	-0.0631	-	7470A	PPB	27 Mar 2023 20:13:12	U	SMPL
O2070-04MS - 1	SOILPILE-2-0323MS	15288	3.4546	-	7470A	PPB	27 Mar 2023 20:15:27	U	SMPL
O2070-04MSD - 1	SOILPILE-2-0323MSD	14976	3.3789	-	7470A	PPB	27 Mar 2023 20:17:43	U	SMPL
O2070-04LX5 - 1		30	-0.2457	-	7470A	PPB	27 Mar 2023 20:19:59	U	SMPL
O2070-04A - 1		16539	3.7580	-	7470A	PPB	27 Mar 2023 20:22:15	U	SMPL
CCV13 - 1	CCV13	21366	4.9286	-	7470A	PPB	27 Mar 2023 20:24:31	U	SMPL
CCB13 - 1	CCB13	721	-0.0782	-	7470A	PPB	27 Mar 2023 20:26:48	U	SMPL
PB151641TB - 1		848	-0.0474	-	7470A	PPB	27 Mar 2023 20:59:00	U	SMPL
CCV14 - 1	CCV14	21579	4.9803	-	7470A	PPB	27 Mar 2023 21:01:17	U	SMPL
CCB14 - 1	CCB14	727	-0.0767	-	7470A	PPB	27 Mar 2023 21:03:33	U	SMPL