

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

3/28/2023 12:27

Reviewed by : 12 Instrument ID : Konelab

Test: CNEPA-NEW

Sample Id	^{mp/12} Result	Dil. 1 +	Response	Errors
ICV001 ICV001	93.431	0.0	0.099	
ICB001 ICB001	1.952	0.0	0.009	
CCV001 CCV001	243.047	0.0	0.246	
CCB001 CCB001	1.842	0.0	0.009	
12 PB151756BL PBW756	2.042	0.0	0.009	
O2007-05 MCB954	2.974	0.0	0.010	
O2007-06 MCB956	2.795	0.0	0.010	
O2007-10 MCB964	3.225	0.0	0.011	
O2007-11 MCB964D	3.085	0.0	0.010	
O2007-12 MCB964S	93.495	0.0	0.099	
O2007-13 MCB966	3.690	0.0	0.011	
O2007-14 MCB967	2.490	0.0	0.010	
CCV002 CCV002	251.780	0.0	0.254	
CCB002 CCB002	1.867	0.0	0.009	

N	14
Mean	50.551
SD	89.5421
CV%	177.13

Aquakem v. 7.2AQ1

Results from time period:

Tue Mar 28 11:20:39 2023

Tue Mar 28 12:13:03 2023

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time
S0.0	A	CNEPA-NE\ P		1.8291	µg/l	3/28/2023 11:20:39
S5.0	A	CNEPA-NE\ P		4.5069	µg/l	3/28/2023 11:20:40
S10.0	A	CNEPA-NE\ P		9.6311	µg/l	3/28/2023 11:20:41
S100.0	A	CNEPA-NE\ P		97.0042	µg/l	3/28/2023 11:20:42
S250.0	A	CNEPA-NE\ P		252.8347	µg/l	3/28/2023 11:20:43
S500.0	A	CNEPA-NE\ P		499.1942	µg/l	3/28/2023 11:20:44
ICV001 ICV001	S	CNEPA-NE\ P		93.4307	µg/l	3/28/2023 11:59:11
ICB001 ICB001	S	CNEPA-NE\ P		1.952	µg/l	3/28/2023 11:59:12
CCV001 CCV001	S	CNEPA-NE\ P		243.047	µg/l	3/28/2023 11:59:14
CCB001 CCB001	S	CNEPA-NE\ P		1.8418	µg/l	3/28/2023 11:59:16
PB151756BL PBW756	S	CNEPA-NE\ P		2.0423	µg/l	3/28/2023 11:59:18
O2007-05 MCB954	S	CNEPA-NE\ P		2.974	µg/l	3/28/2023 12:06:45
O2007-06 MCB956	S	CNEPA-NE\ P		2.7946	µg/l	3/28/2023 12:06:46
O2007-10 MCB964	S	CNEPA-NE\ P		3.2253	µg/l	3/28/2023 12:06:48
O2007-11 MCB964D	S	CNEPA-NE\ P		3.0852	µg/l	3/28/2023 12:06:51
O2007-12 MCB964S	S	CNEPA-NE\ P		93.4949	µg/l	3/28/2023 12:06:52
O2007-13 MCB966	S	CNEPA-NE\ P		3.6898	µg/l	3/28/2023 12:12:56
O2007-14 MCB967	S	CNEPA-NE\ P		2.49	µg/l	3/28/2023 12:12:58
CCV002 CCV002	S	CNEPA-NE\ P		251.7799	µg/l	3/28/2023 12:13:00
CCB002 CCB002	S	CNEPA-NE\ P		1.8667	µg/l	3/28/2023 12:13:02

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

3/28/2023 11:28

Test CNEPA-NEW

Accepted

3/28/2023 11:28

~~Factor~~ Slope
Bias Y. Intercept


~~1019~~ 0.000981
0.007

12
03/28/23

Coeff. of det.

0.999892

Errors

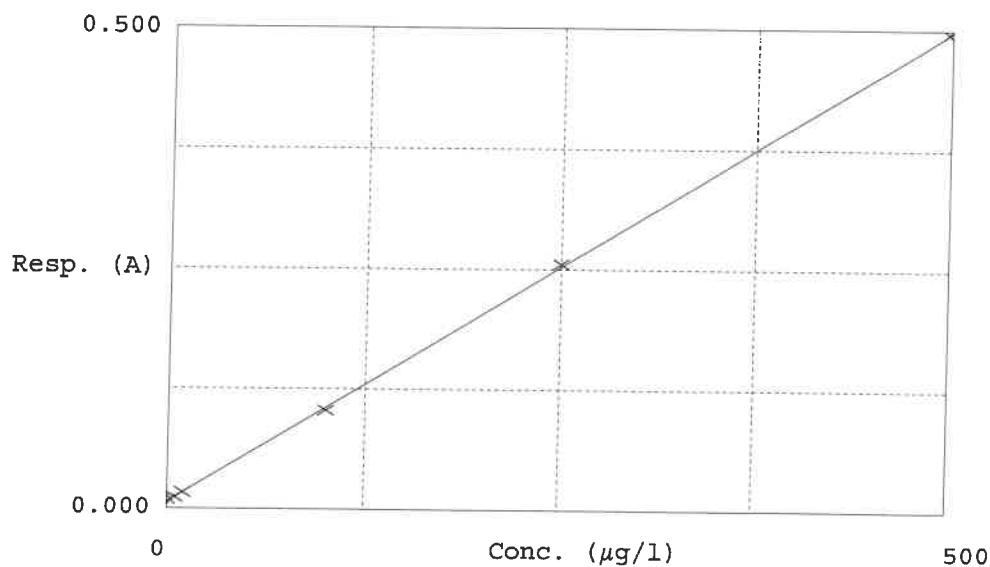

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN 50.0	0.009	1.8291	0.0000	-
2	5.0PPBCN 50.0	0.012	4.5069	5.0000	-P.P
3	10PPBCN 50.0	0.017	9.6311	10.0000	-3.7
4	100PPBCN 500.0	0.103	97.0042	100.0000	-3.0
5	250PPBCN 5250.0	0.255	252.8347	250.0000	1.1
6	500PPBCN 5500.0	0.497	499.1942	500.0000	-0.2

12
3/28/23