


7470A

LB124759, INSTRUMENT: CV1

Linear

 μ Abs.:

55086

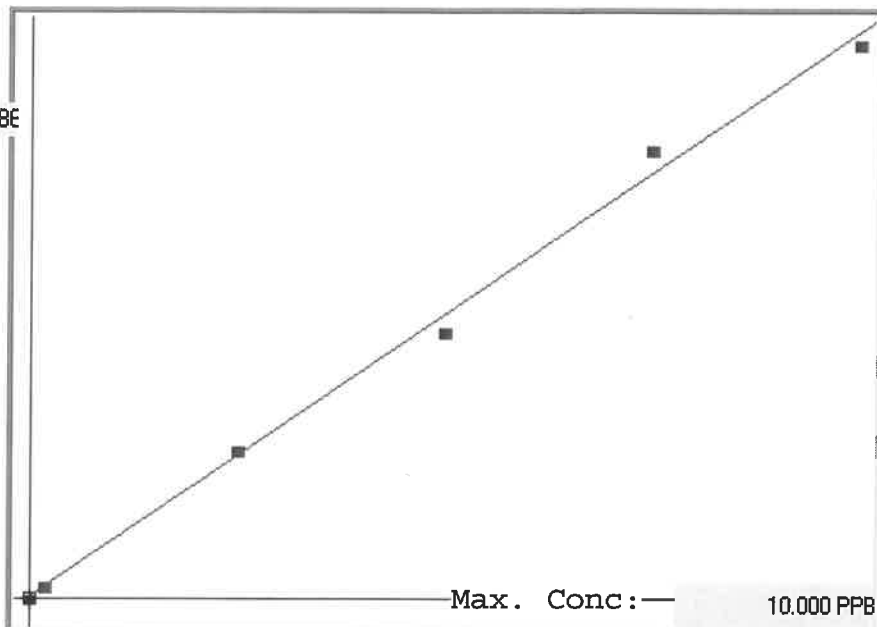

A= 0.0000e+000

B= 1.7804e-004

C= -3.1221e-002

Rho= 0.9980696

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.004	-0.004	153	0.000	153	0			
0.2	0.200	0.194	-0.006	1263	0.0 %	1263				
2.5	2.500	2.611	0.111	14839	0.0 %	14839				
5.0	5.000	4.711	-0.289	26638	0.0 %	26638				
7.5	7.500	7.912	0.412	44613	0.0 %	44613				
10.0	10.000	9.776	-0.224	55086	0.0 %	55086				

Y.P
 13
 4
 -6
 5
 -2

LB124759, INSTRUMENT ID:CV1

Method: 7470A		Operator: Admin		Date of Analysis: 30 Mar 2023 15:42:54					
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	153	-	0.0000	7470A	PPB	30 Mar 2023 16:17:10	S	Std
0.2 - 1	50.2	1263	-	0.2000	7470A	PPB	30 Mar 2023 16:19:27	S	Std
2.5 - 1	52.5	14839	-	2.5000	7470A	PPB	30 Mar 2023 16:21:45	S	Std
5.0 - 1	55.0	26638	-	5.0000	7470A	PPB	30 Mar 2023 16:24:02	S	Std
7.5 - 1	57.5	44613	-	7.5000	7470A	PPB	30 Mar 2023 16:26:18	S	Std
10.0 - 1	510.0	55086	-	10.0000	7470A	PPB	30 Mar 2023 16:28:34	S	Std
ICV06 - 1	ICV06	24079	4.2558	-	7470A	PPB	30 Mar 2023 16:31:31	U	SMPL
ICB06 - 1	ICB06	37	-0.0246	-	7470A	PPB	30 Mar 2023 16:33:45	U	SMPL
CCV23 - 1	CCV23	29247	5.1760	-	7470A	PPB	30 Mar 2023 16:36:01	U	SMPL
CCB23 - 1	CCB23	48	-0.0227	-	7470A	PPB	30 Mar 2023 16:38:16	U	SMPL
CRA - 1	CRA	1220	0.1860	-	7470A	PPB	30 Mar 2023 16:40:32	U	SMPL
HighStd - 1	HighStd	53116	9.4256	-	7470A	PPB	30 Mar 2023 16:42:47	U	SMPL
ChkStd - 1	ChkStd	39871	7.0675	-	7470A	PPB	30 Mar 2023 16:45:03	U	SMPL
PB151802BL - 1	PBW	36	-0.0250	-	7470A	PPB	30 Mar 2023 16:47:21	U	SMPL
PB151802BS - 1	LCSW	21391	3.7773	-	7470A	PPB	30 Mar 2023 16:49:38	U	SMPL
O2124-01 - 1	E9074-PVSC-001	111	-0.0115	-	7470A	PPB	30 Mar 2023 16:51:55	U	SMPL
O2128-01 - 1	LOC25-10-032923	138	-0.0067	-	7470A	PPB	30 Mar 2023 16:54:11	U	SMPL
O2128-01DUP - 1	LOC25-10-032923DUP	141	-0.0061	-	7470A	PPB	30 Mar 2023 16:56:28	U	SMPL
O2128-01MS - 1	LOC25-10-032923MS	21225	3.7477	-	7470A	PPB	30 Mar 2023 16:58:45	U	SMPL
O2128-01MSD - 1	LOC25-10-032923MSD	21438	3.7856	-	7470A	PPB	30 Mar 2023 17:01:01	U	SMPL
CCV24 - 1	CCV24	28841	5.1037	-	7470A	PPB	30 Mar 2023 17:06:02	U	SMPL
CCB24 - 1	CCB24	45	-0.0232	-	7470A	PPB	30 Mar 2023 17:08:17	U	SMPL
O2128-02 - 1	LOC25-10-032923	165	-0.0018	-	7470A	PPB	30 Mar 2023 17:10:33	U	SMPL
O2128-03 - 1	LOC25-35-032923	483	0.0548	-	7470A	PPB	30 Mar 2023 17:12:49	U	SMPL
O2128-04 - 1	LOC25-35-032923	317	0.0252	-	7470A	PPB	30 Mar 2023 17:15:04	U	SMPL
O2128-01LX5 - 1		123	-0.0093	-	7470A	PPB	30 Mar 2023 17:17:20	U	SMPL
O2128-01A - 1		23869	4.2185	-	7470A	PPB	30 Mar 2023 17:19:36	U	SMPL
CCV25 - 1	CCV25	26541	4.6942	-	7470A	PPB	30 Mar 2023 17:21:53	U	SMPL
CCB25 - 1	CCB25	18	-0.0280	-	7470A	PPB	30 Mar 2023 17:24:11	U	SMPL