

LB124950


7470A

INSTRUMENT 1D? CV1

Linear

 μ Abs.:

43459

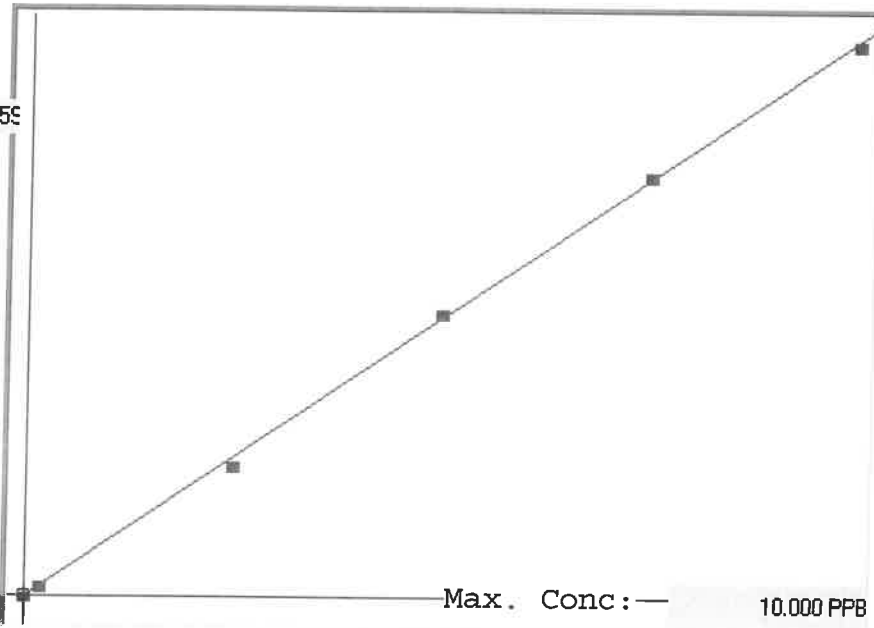

A= 0.0000e+000

B= 2.2807e-004

C= 9.7291e-003

Rho= 0.9996979

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	
0.0	0.000	0.036	0.036	116	0.000	116	0				0/00
0.2	0.200	0.214	0.014	896	0.0 %	896					17
2.5	2.500	2.344	-0.156	10234	0.0 %	10234					-6
5.0	5.000	5.104	0.104	22336	0.0 %	22336					2
7.5	7.500	7.581	0.081	33195	0.0 %	33195					1
10.0	10.000	9.921	-0.079	43459	0.0 %	43459					1

LB124950 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 13 Apr 2023 10:19:20

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	116	-	0.0000	7470A	PPB	13 Apr 2023 10:22:47	S	Std
0.2 - 1	50.2	896	-	0.2000	7470A	PPB	13 Apr 2023 10:25:05	S	Std
2.5 - 1	52.5	10234	-	2.5000	7470A	PPB	13 Apr 2023 10:27:23	S	Std
5.0 - 1	55	22336	-	5.0000	7470A	PPB	13 Apr 2023 10:29:40	S	Std
7.5 - 1	57.5	33195	-	7.5000	7470A	PPB	13 Apr 2023 10:37:07	S	Std
10.0 - 1	511	43459	-	10.0000	7470A	PPB	13 Apr 2023 10:46:50	S	Std
ICV19 - 1	ICV19	17589	4.0213	-	7470A	PPB	13 Apr 2023 10:51:20	U	SMPL
ICB19 - 1	ICB19	1	0.0100	-	7470A	PPB	13 Apr 2023 10:53:35	U	SMPL
CCV56 - 1	CCV56	21037	4.8077	-	7470A	PPB	13 Apr 2023 10:58:22	U	SMPL
CCB56 - 1	CCB56	61	0.0236	-	7470A	PPB	13 Apr 2023 11:00:37	U	SMPL
CRA - 1	CRA	794	0.1908	-	7470A	PPB	13 Apr 2023 11:02:53	U	SMPL
HighStd - 1	HighStd	43342	9.8948	-	7470A	PPB	13 Apr 2023 11:07:47	U	SMPL
ChkStd - 1	ChkStd	29452	6.7289	-	7470A	PPB	13 Apr 2023 11:10:03	U	SMPL
PB152071BL - 1	PBW	55	0.0223	-	7470A	PPB	13 Apr 2023 11:15:03	U	SMPL
PB152071BS - 1	LCSW	17129	3.9164	-	7470A	PPB	13 Apr 2023 11:17:18	U	SMPL
O2262-04 - 1	JPP-2-040723	322	0.0832	-	7470A	PPB	13 Apr 2023 11:19:35	U	SMPL
O2262-08 - 1	JPP-1-040723	399	0.1007	-	7470A	PPB	13 Apr 2023 11:21:51	U	SMPL
O2262-12 - 1	JPP-3A-040723	432	0.1083	-	7470A	PPB	13 Apr 2023 11:24:08	U	SMPL
O2262-12DUP - 1	JPP-3A-040723DUP	481	0.1194	-	7470A	PPB	13 Apr 2023 11:26:26	U	SMPL
O2262-12MS - 1	JPP-3A-040723MS	16198	3.7040	-	7470A	PPB	13 Apr 2023 11:28:41	U	SMPL
CCV57 - 1	CCV57	20573	4.7018	-	7470A	PPB	13 Apr 2023 11:33:46	U	SMPL
CCB57 - 1	CCB57	50	0.0211	-	7470A	PPB	13 Apr 2023 11:36:02	U	SMPL
O2262-12MSD - 1	JPP-3A-040723MSD	15961	3.6500	-	7470A	PPB	13 Apr 2023 11:38:19	U	SMPL
PB152072BL - 1	PBW	304	0.0791	-	7470A	PPB	13 Apr 2023 11:40:34	U	SMPL
PB152072BS - 1	LCSW	16229	3.7111	-	7470A	PPB	13 Apr 2023 11:42:51	U	SMPL
O2220-02 - 1	COMP	173	0.0492	-	7470A	PPB	13 Apr 2023 11:45:07	U	SMPL
O2247-02 - 1	PK-10S	270	0.0713	-	7470A	PPB	13 Apr 2023 11:47:24	U	SMPL
O2247-04 - 1	PK-10I	101	0.0328	-	7470A	PPB	13 Apr 2023 11:49:43	U	SMPL
O2247-06 - 1	PK-10D	108	0.0344	-	7470A	PPB	13 Apr 2023 11:52:00	U	SMPL
O2247-06DUP - 1	PK-10DDUP	214	0.0585	-	7470A	PPB	13 Apr 2023 11:54:17	U	SMPL
O2247-09 - 1	O2247-06MS	19926	4.5543	-	7470A	PPB	13 Apr 2023 12:24:44	U	SMPL
O2247-10 - 1	O2247-06MSD	19397	4.4336	-	7470A	PPB	13 Apr 2023 12:27:00	U	SMPL
CCV58 - 1	CCV58	21510	4.9155	-	7470A	PPB	13 Apr 2023 12:34:00	U	SMPL
CCB58 - 1	CCB58	95	0.0314	-	7470A	PPB	13 Apr 2023 12:36:16	U	SMPL
O2247-12 - 1	RW-12I	414	0.1042	-	7470A	PPB	13 Apr 2023 12:38:33	U	SMPL
O2247-14 - 1	RW-12D	1113	0.2636	-	7470A	PPB	13 Apr 2023 12:40:48	U	SMPL
O2268-01 - 1	50002-TOTE	136324	31.1013	-	7470A	PPB	13 Apr 2023 12:43:04	U	SMPL
O2286-04 - 1	328	3012	0.6967	-	7470A	PPB	13 Apr 2023 12:45:20	U	SMPL
O2288-02 - 1	GROUND-WATER	324	0.0836	-	7470A	PPB	13 Apr 2023 12:47:40	U	SMPL
O2291-01 - 1	23330	1385	0.3256	-	7470A	PPB	13 Apr 2023 12:49:56	U	SMPL
O2291-02 - 1	2344	1263	0.2978	-	7470A	PPB	13 Apr 2023 12:52:13	U	SMPL
O2293-01 - 1	IDW-LIQ-FRAC-041123	737	0.1778	-	7470A	PPB	13 Apr 2023 12:54:30	U	SMPL
O2319-01 - 1	E9074-PVSC-002	300	0.0782	-	7470A	PPB	13 Apr 2023 12:56:48	U	SMPL
CCV59 - 1	CCV59	22033	5.0348	-	7470A	PPB	13 Apr 2023 12:59:04	U	SMPL
CCB59 - 1	CCB59	145	0.0428	-	7470A	PPB	13 Apr 2023 13:01:20	U	SMPL
PB151998TB - 1		377	0.0957	-	7470A	PPB	13 Apr 2023 13:03:36	U	SMPL
PB2262-12LX5 - 1		71	0.0259	-	7470A	PPB	13 Apr 2023 13:05:52	U	SMPL
PB2262-12A - 1		18413	4.2092	-	7470A	PPB	13 Apr 2023 13:08:07	U	SMPL
O2247-06LX5 - 1		-9	0.0077	-	7470A	PPB	13 Apr 2023 13:10:23	U	SMPL
O2247-06A - 1		19418	4.4384	-	7470A	PPB	13 Apr 2023 13:12:39	U	SMPL
O2268-01DLX10 - 1		11704	2.6791	-	7470A	PPB	13 Apr 2023 13:14:55	U	SMPL
CCV60 - 1	CCV60	22704	5.1879	-	7470A	PPB	13 Apr 2023 13:17:12	U	SMPL
CCB60 - 1	CCB60	-89	-0.0106	-	7470A	PPB	13 Apr 2023 13:19:30	U	SMPL