

LB12506P

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

4/20/2023 14:24

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.966	0.0	0.092	
ICB1	-0.011	0.0	0.006	
CCV1	0.963	0.0	0.092	
CCB1	-0.007	0.0	0.006	
PB152264BL	-0.002	0.0	0.007	
PB152264BS	0.959	0.0	0.092	
O2213-12	0.019	0.0	0.009	
O2415-01	0.018	0.0	0.009	
O2415-01DUP	0.026	0.0	0.009	
O2415-01MS	1.234	0.0	0.116	
O2415-01MSD	1.228	0.0	0.115	
CCV2	0.962	0.0	0.092	
CCB2	-0.006	0.0	0.007	

N	13
Mean	0.488
SD	0.5506
CV%	112.74

Aquakem v. 7.2AQ1

Results from time period:

Thu Apr 20 13:29:25 2023

Thu Apr 20 14:12:51 2023

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0027	mg/l	4/20/2023 13:29:25	
0.05PPM	A	Phenolics-	P	0.0515	mg/l	4/20/2023 13:29:26	
0.1PPM	A	Phenolics-	P	0.1081	mg/l	4/20/2023 13:29:27	
0.25PPM	A	Phenolics-	P	0.2433	mg/l	4/20/2023 13:29:28	
0.50PPM	A	Phenolics-	P	0.5024	mg/l	4/20/2023 13:29:29	
1.0PPM	A	Phenolics-	P	0.9843	mg/l	4/20/2023 13:29:30	
2.0PPM	A	Phenolics-	P	2.0077	mg/l	4/20/2023 13:29:31	
ICV1	S	Phenolics-	P	0.9659	mg/l	4/20/2023 14:05:30	
ICB1	S	Phenolics-	P	-0.0107	mg/l	4/20/2023 14:05:32	
CCV1	S	Phenolics-	P	0.9629	mg/l	4/20/2023 14:05:34	
CCB1	S	Phenolics-	P	-0.0075	mg/l	4/20/2023 14:05:35	
PB152264BL	S	Phenolics-	P	-0.0024	mg/l	4/20/2023 14:05:37	
PB152264BS	S	Phenolics-	P	0.9594	mg/l	4/20/2023 14:05:40	
O2213-12	S	Phenolics-	P	0.0189	mg/l	4/20/2023 14:12:43	
O2415-01	S	Phenolics-	P	0.0181	mg/l	4/20/2023 14:12:45	
O2415-01DUP	S	Phenolics-	P	0.0264	mg/l	4/20/2023 14:12:46	
O2415-01MS	S	Phenolics-	P	1.2344	mg/l	4/20/2023 14:12:47	
O2415-01MSD	S	Phenolics-	P	1.2282	mg/l	4/20/2023 14:12:48	
CCV2	S	Phenolics-	P	0.9617	mg/l	4/20/2023 14:12:49	
CCB2	S	Phenolics-	P	-0.006	mg/l	4/20/2023 14:12:50	

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

4/20/2023 13:33


Test Phenolics-

Accepted 4/20/2023 13:33

Factor 11.34
Bias 0.007

Coeff. of det. 0.999863

Errors

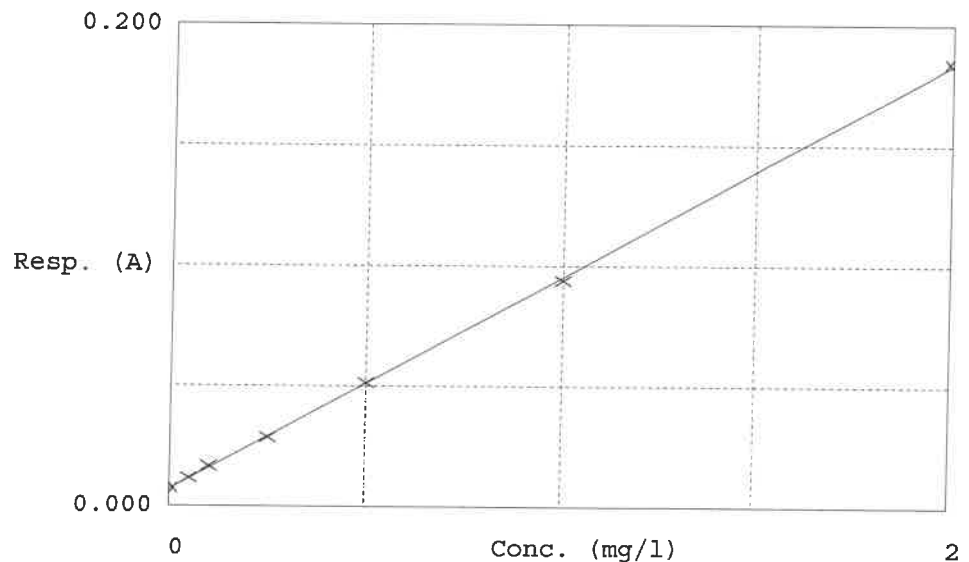

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.007	0.0027	0.0000	-
2	Phenol-2	0.012	0.0515	0.0500	3.0
3	Phenol-2	0.017	0.1081	0.1000	8.1
4	Phenol-2	0.029	0.2433	0.2500	-2.7
5	Phenol-2	0.051	0.5024	0.5000	0.5
6	Phenol-2	0.094	0.9843	1.0000	-1.6
7	Phenol-2	0.184	2.0077	2.0000	0.4

12

4/20/23