

=====
Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

5/5/2023 14:36

Test: Total CN

Table with 5 columns: Sample Id, Result, Dil. 1 +, Response, Errors.
Handwritten notes: 105% (50-150), 88% (90-110), 12, 5/5/23.

N 20
Mean 69.609
SD 95.8875
CV% 137.75

Aquakem v. 7.2AQ1

Results from time period:

Fri May 05 14:01:19 2023

Fri May 05 14:34:22 2023

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	1.0642	µg/l	5/5/2023 10:09:54	
5.0PPBCN	A	Total CN	P	5.7173	µg/l	5/5/2023 10:09:55	
10PPBCN	A	Total CN	P	9.6815	µg/l	5/5/2023 10:09:56	
50PPBCN	A	Total CN	P	48.5051	µg/l	5/5/2023 10:09:57	
100PPBCN	A	Total CN	P	99.1176	µg/l	5/5/2023 10:09:58	
250PPBCN	A	Total CN	P	251.1782	µg/l	5/5/2023 10:09:59	
500PPBCN	A	Total CN	P	499.7361	µg/l	5/5/2023 10:10:00	
ICV1	S	Total CN	P	95.2128	µg/l	5/5/2023 14:01:20	
ICB1	S	Total CN	P	0.9252	µg/l	5/5/2023 14:01:21	
CCV1	S	Total CN	P	243.4561	µg/l	5/5/2023 14:01:24	
CCB1	S	Total CN	P	0.8507	µg/l	5/5/2023 14:01:25	
RL CHECK	S	Total CN	P	5.239	µg/l	5/5/2023 14:01:28	
PB152608BL	S	Total CN	P	0.4918	µg/l	5/5/2023 14:01:29	
PB152608BS	S	Total CN	P	95.7044	µg/l	5/5/2023 14:08:53	
MIDPB152608	S	Total CN	P	246.2046	µg/l	5/5/2023 14:08:55	
O2618-05	S	Total CN	P	14.7326	µg/l	5/5/2023 14:08:57	
O2618-05DUP	S	Total CN	P	14.6097	µg/l	5/5/2023 14:08:58	
O2618-05MS	S	Total CN	P	51.5094	µg/l	5/5/2023 14:09:01	
O2618-05MSD	S	Total CN	P	51.2865	µg/l	5/5/2023 14:14:34	
CCV2	S	Total CN	P	246.7544	µg/l	5/5/2023 14:14:35	
CCB2	S	Total CN	P	0.8503	µg/l	5/5/2023 14:14:36	
O2618-01	S	Total CN	P	16.9489	µg/l	5/5/2023 14:14:37	
O2618-03	S	Total CN	P	45.4978	µg/l	5/5/2023 14:14:38	
O2213-12	S	Total CN	P	2.8959	µg/l	5/5/2023 14:34:17	
O2213-12RE	S	Total CN	P	4.3375	µg/l	5/5/2023 14:34:20	
CCV3	S	Total CN	P	253.9146	µg/l	5/5/2023 14:34:21	
CCB3	S	Total CN	P	0.7552	µg/l	5/5/2023 14:34:22	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

5/5/2023 10:10 Reviewed by : 12 Instrument ID : Konelab


Test Total CN

Accepted 5/5/2023 10:10

Factor 1298
Bias 0.001

Coeff. of det. 0.999970

Errors

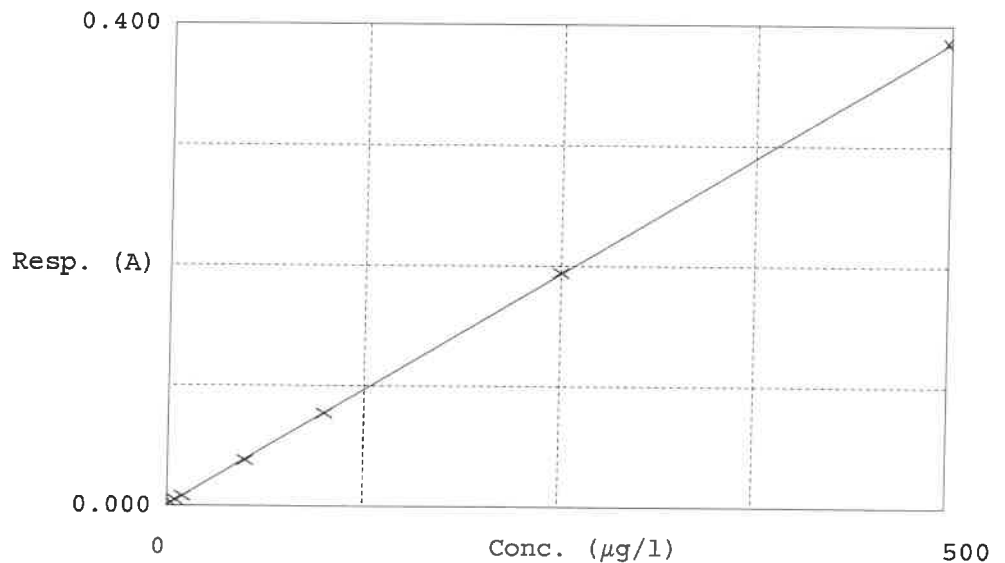

	Calibrator	Response	Calc. con.	Conc.	Re Errors
1	0.0PPBCN	0.001	1.0642	0.0000	-
2	5.0PPBCN	0.005	5.7173	5.0000	14.3
3	10PPBCN	0.008	9.6815	10.0000	-3.2
4	50PPBCN	0.038	48.5051	50.0000	-3.0
5	100PPBCN	0.077	99.1176	100.0000	-0.9
6	250PPBCN	0.194	251.1782	250.0000	0.5
7	500PPBCN	0.386	499.7361	500.0000	-0.1

12
5/5/23