

LB125399


7470A

/ INSTRUMENT ID: CV2

Linear

 μ Abs.:

4306E

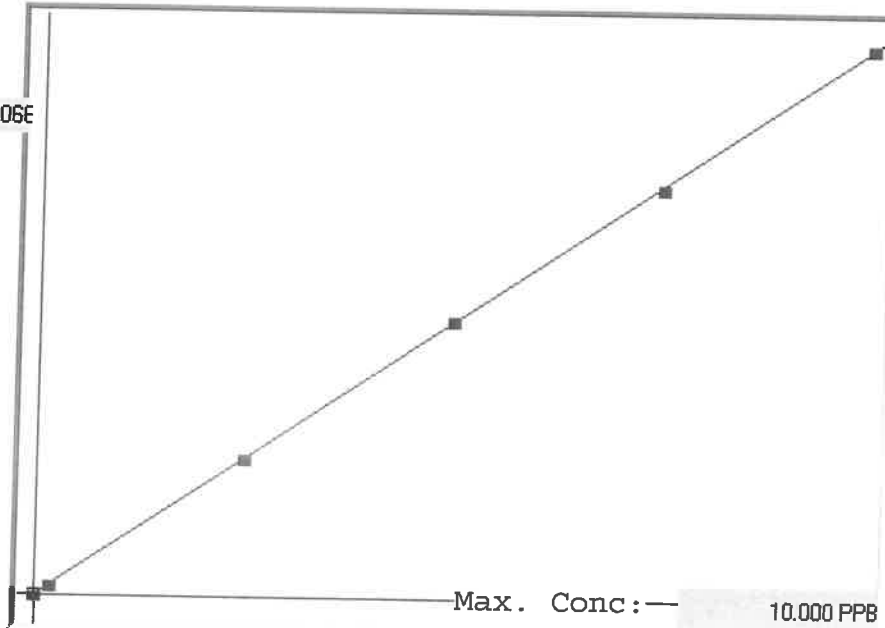

A= 0.0000e+000

B= 2.3267e-004

C= -5.0545e-003

Rho= 0.9999784

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	1/0/0
0.0	0.000	-0.002	-0.002	14	0.000	14	0				
0.2	0.200	0.186	-0.014	823	0.0 %	823					
2.5	2.500	2.516	0.016	10836	0.0 %	10836					
5.0	5.000	5.029	0.029	21637	0.0 %	21637					
7.5	7.500	7.455	-0.045	32064	0.0 %	32064					
10.0	10.000	10.015	0.015	43066	0.0 %	43066					

LB125399 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 11 May 2023 08:59:08

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	14	-	0.0000	7470A	PPB	11 May 2023 09:44:54	S	Std
0.2 - 1	50.2	823	-	0.2000	7470A	PPB	11 May 2023 09:47:12	S	Std
2.5 - 1	52.5	10836	-	2.5000	7470A	PPB	11 May 2023 09:49:29	S	Std
5.0 - 1	55	21637	-	5.0000	7470A	PPB	11 May 2023 09:51:46	S	Std
7.5 - 1	57.5	32064	-	7.5000	7470A	PPB	11 May 2023 09:54:03	S	Std
10.0 - 1	510	43066	-	10.0000	7470A	PPB	11 May 2023 09:56:20	S	Std
ICV72 - 1	ICV72	17574	4.0838	-	7470A	PPB	11 May 2023 09:59:04	U	SMPL
ICB72 - 1	ICB72	-183	-0.0476	-	7470A	PPB	11 May 2023 10:01:19	U	SMPL
CCV46 - 1	CCV46	20216	4.6985	-	7470A	PPB	11 May 2023 10:03:36	U	SMPL
CCB46 - 1	CCB46	-199	-0.0514	-	7470A	PPB	11 May 2023 10:05:51	U	SMPL
CRA - 1	CRA	792	0.1792	-	7470A	PPB	11 May 2023 10:08:08	U	SMPL
HighStd - 1	HighStd	43711	10.1650	-	7470A	PPB	11 May 2023 10:10:24	U	SMPL
ChkStd - 1	ChkStd	30119	7.0026	-	7470A	PPB	11 May 2023 10:12:40	U	SMPL
PB152712BL - 1	PBW	-220	-0.0562	-	7470A	PPB	11 May 2023 10:14:58	U	SMPL
PB152712BS - 1	LCSW	17109	3.9756	-	7470A	PPB	11 May 2023 10:17:16	U	SMPL
O2665-02 - 1	TR-612-COMP-01	-133	-0.0360	-	7470A	PPB	11 May 2023 10:19:33	U	SMPL
O2665-09 - 1	TR-612-COMP-02	-44	-0.0153	-	7470A	PPB	11 May 2023 10:21:50	U	SMPL
O2691-02 - 1	AU-504-COMP-06	-16	-0.0088	-	7470A	PPB	11 May 2023 10:24:07	U	SMPL
O2691-09 - 1	AU-504-COMP-07	61	0.0091	-	7470A	PPB	11 May 2023 10:26:24	U	SMPL
O2693-01 - 1	BEL-23-002	-17	-0.0090	-	7470A	PPB	11 May 2023 10:28:40	U	SMPL
CCV47 - 1	CCV47	20878	4.8526	-	7470A	PPB	11 May 2023 10:30:55	U	SMPL
CCB47 - 1	CCB47	-132	-0.0358	-	7470A	PPB	11 May 2023 10:33:11	U	SMPL
O2693-01DUP - 1	BEL-23-002DUP	-20	-0.0097	-	7470A	PPB	11 May 2023 10:35:27	U	SMPL
O2693-01MS - 1	BEL-23-002MS	14754	3.4277	-	7470A	PPB	11 May 2023 10:37:43	U	SMPL
O2693-01MSD - 1	BEL-23-002MSD	16959	3.9407	-	7470A	PPB	11 May 2023 10:39:58	U	SMPL
O2693-01LX5 - 1		-139	-0.0374	-	7470A	PPB	11 May 2023 10:42:15	U	SMPL
O2693-01A - 1		16668	3.8730	-	7470A	PPB	11 May 2023 10:50:12	U	SMPL
PB152676TB - 1	PB152676TB	-181	-0.0472	-	7470A	PPB	11 May 2023 10:52:28	U	SMPL
CCV48 - 1	CCV48	21446	4.9847	-	7470A	PPB	11 May 2023 10:54:45	U	SMPL
CCB48 - 1	CCB48	-159	-0.0420	-	7470A	PPB	11 May 2023 10:57:03	U	SMPL