

7470A


LB125554

INSTRUMENT NO: CVZ

Linear

 μ Abs.:

44248

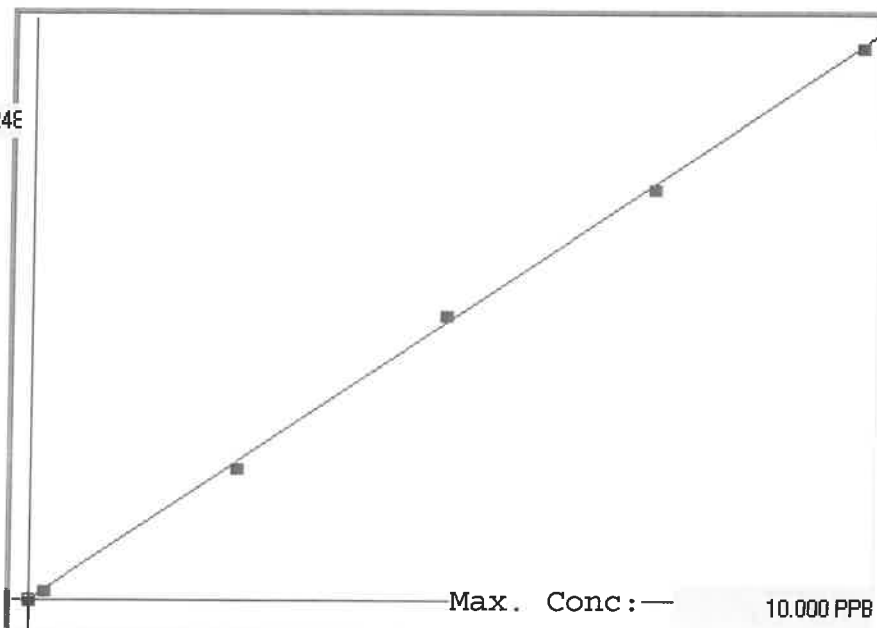

A= 0.0000e+000

B= 2.2549e-004

C= 2.7091e-003

Rho= 0.9997837

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.005	0.005	9	0.000	9	0				1
0.2	0.200	0.201	0.001	881	0.0 %	881					-4
2.5	2.500	2.410	-0.090	10677	0.0 %	10677					3
5.0	5.000	5.155	0.155	22852	0.0 %	22852					-1
7.5	7.500	7.448	-0.052	33020	0.0 %	33020					0
10.0	10.000	9.980	-0.020	44248	0.0 %	44248					

LB125554

Method: 7470A

Operator: Admin

Date of Analysis: 19 May 2023 11:03:33

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	56	9	-	0.0000	7470A	PPB	19 May 2023 11:25:56	S	Std
0.2 - 1	50.2	881	-	0.2000	7470A	PPB	19 May 2023 11:28:13	S	Std
2.5 - 1	52.5	10677	-	2.5000	7470A	PPB	19 May 2023 11:30:31	S	Std
5.0 - 1	57.5	22852	-	5.0000	7470A	PPB	19 May 2023 11:32:48	S	Std
7.5 - 1	51.6	33020	-	7.5000	7470A	PPB	19 May 2023 11:35:05	S	Std
10.0 - 1		44248	-	10.0000	7470A	PPB	19 May 2023 11:40:04	S	Std
ICV84 - 1	ICV84	17539	3.9575	-7470A	PPB	U	19 May 2023 11:42:48	U	SMPL
ICB84 - 1	ICB84	-177	-0.0372	-7470A	PPB	U	19 May 2023 11:45:03	U	SMPL
CCV86 - 1	CCV86	23944	5.4017	-7470A	PPB	U	19 May 2023 11:47:20	U	SMPL
CCB86 - 1	CCB86	-181	-0.0381	-7470A	PPB	U	19 May 2023 11:49:35	U	SMPL
CRA - 1	CRA	832	0.1903	-7470A	PPB	U	19 May 2023 11:51:52	U	SMPL
HighStd - 1	HighStd	43498	9.8109	-7470A	PPB	U	19 May 2023 11:54:08	U	SMPL
ChkStd - 1	ChkStd	31168	7.0306	-7470A	PPB	U	19 May 2023 11:56:24	U	SMPL
PB152890BL - 1	PBW	-130	-0.0266	-7470A	PPB	U	19 May 2023 11:58:42	U	SMPL
PB152890BS - 1	LCSW	18816	4.2454	-7470A	PPB	U	19 May 2023 12:01:00	U	SMPL
O2818-01 - 1	P001-CS001-01	1809	0.4106	-7470A	PPB	U	19 May 2023 12:08:17	U	SMPL
O2818-01DUP - 1	P001-CS001-01DUP	1576	0.3581	-7470A	PPB	U	19 May 2023 12:10:34	U	SMPL
O2818-02 - 1	O2818-01MS	18422	4.1566	-7470A	PPB	U	19 May 2023 12:12:51	U	SMPL
O2818-03 - 1	O2818-01MSD	17798	4.0159	-7470A	PPB	U	19 May 2023 12:15:09	U	SMPL
O2818-04 - 1	P001-CS001-02	1423	0.3236	-7470A	PPB	U	19 May 2023 12:17:26	U	SMPL
CCV87 - 1	CCV87	22995	5.1877	-7470A	PPB	U	19 May 2023 12:19:44	U	SMPL
CCB87 - 1	CCB87	-63	-0.0115	-7470A	PPB	U	19 May 2023 12:21:59	U	SMPL
O2818-05 - 1	P001-CS002-01	1373	0.3123	-7470A	PPB	U	19 May 2023 12:24:16	U	SMPL
O2818-06 - 1	P001-CS003-01	1651	0.3750	-7470A	PPB	U	19 May 2023 12:26:31	U	SMPL
O2818-07 - 1	P001-CS004-01	317	0.0742	-7470A	PPB	U	19 May 2023 12:28:47	U	SMPL
O2818-08 - 1	P001-CS005-01	-75	-0.0142	-7470A	PPB	U	19 May 2023 12:31:03	U	SMPL
O2818-09 - 1	P001-CS006-01	67	0.0178	-7470A	PPB	U	19 May 2023 12:33:19	U	SMPL
O2818-10 - 1	P001-CS007-01	445	0.1030	-7470A	PPB	U	19 May 2023 12:35:36	U	SMPL
O2818-11 - 1	P001-CS008-01	22	0.0077	-7470A	PPB	U	19 May 2023 12:37:52	U	SMPL
O2818-12 - 1	P001-CS009-01	188	0.0451	-7470A	PPB	U	19 May 2023 12:40:10	U	SMPL
O2818-13 - 1	P001-CS010-01	15	0.0061	-7470A	PPB	U	19 May 2023 12:42:27	U	SMPL
PB152891BL - 1	PBW	38	0.0113	-7470A	PPB	U	19 May 2023 12:44:43	U	SMPL
CCV88 - 1	CCV88	23304	5.2574	-7470A	PPB	U	19 May 2023 12:46:58	U	SMPL
CCB88 - 1	CCB88	-57	-0.0101	-7470A	PPB	U	19 May 2023 12:49:14	U	SMPL
PB152891BS - 1	LCSW	16679	3.7636	-7470A	PPB	U	19 May 2023 12:51:30	U	SMPL
O2820-01 - 1	8321	-114	-0.0230	-7470A	PPB	U	19 May 2023 12:53:46	U	SMPL
O2820-01DUP - 1	8321DUP	36	0.0108	-7470A	PPB	U	19 May 2023 12:56:02	U	SMPL
O2820-01MS - 1	8321MS	15217	3.4339	-7470A	PPB	U	19 May 2023 12:58:18	U	SMPL
O2820-01MSD - 1	8321MSD	15999	3.6102	-7470A	PPB	U	19 May 2023 13:00:34	U	SMPL
O2820-02 - 1	8327	-30	-0.0041	-7470A	PPB	U	19 May 2023 13:02:51	U	SMPL
MP152857TB - 1	MP152857TB	14	0.0059	-7470A	PPB	U	19 May 2023 13:05:09	U	SMPL
PB152868TB - 1	PB152868TB	3	0.0034	-7470A	PPB	U	19 May 2023 13:07:26	U	SMPL
CCV89 - 1	CCV89	23095	5.2103	-7470A	PPB	U	19 May 2023 13:09:43	U	SMPL
CCB89 - 1	CCB89	-131	-0.0268	-7470A	PPB	U	19 May 2023 13:12:01	U	SMPL
O2818-01A - 1		16169	3.6486	-7470A	PPB	U	19 May 2023 13:16:33	U	SMPL
O2820-01LX5 - 1		-178	-0.0374	-7470A	PPB	U	19 May 2023 13:18:50	U	SMPL
O2820-01A - 1		16679	3.7636	-7470A	PPB	U	19 May 2023 13:21:08	U	SMPL
O2818-01LX5 - 1		347	0.0810	-7470A	PPB	U	19 May 2023 13:38:07	U	SMPL
CCV90 - 1	CCV90	21480	4.8461	-7470A	PPB	U	19 May 2023 13:40:39	U	SMPL
CCB90 - 1	CCB90	-121	-0.0246	-7470A	PPB	U	19 May 2023 13:42:55	U	SMPL