

LB125616


7471B

INSTRUMENT ID: CMA

Linear

 μ Abs.:

66009

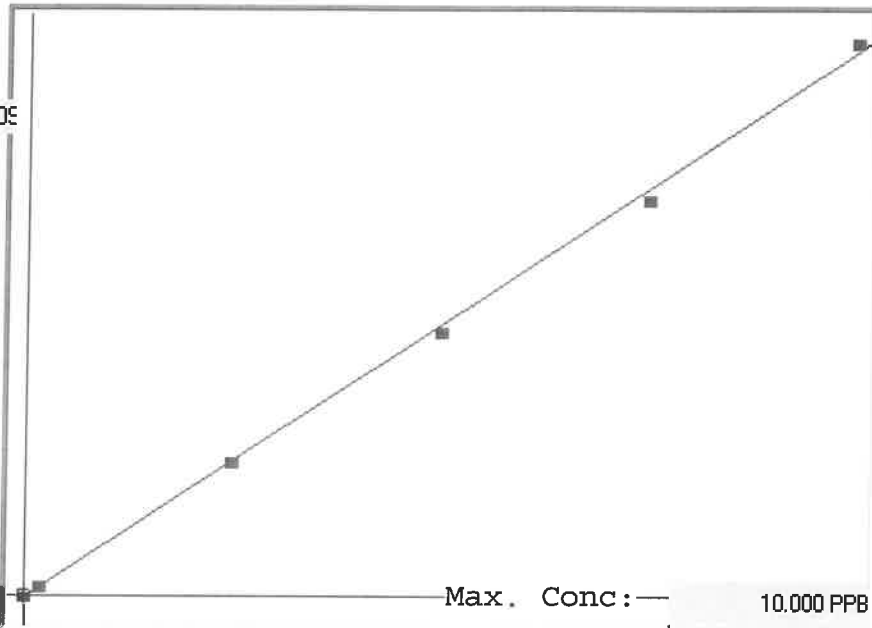

A= 0.0000e+000

B= 1.5369e-004

C= 3.5643e-002

Rho= 0.9994883

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	
0.0	0.000	0.065	0.065	190	0.000	190					110
0.2	0.200	0.238	0.038	1317	0.0 %	1317					19
2.5	2.500	2.504	0.004	16061	0.0 %	16061					0
5.0	5.000	4.900	-0.100	31652	0.0 %	31652					-2
7.5	7.500	7.312	-0.188	47344	0.0 %	47344					-3
10.0	10.000	10.181	0.181	66009	0.0 %	66009					2

LB125616 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 24 May 2023 11:09:02

Sample ID	Extended ID	μ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	190	-	0.0000	7471B	PPB	24 May 2023 11:25:05	S	Std
0.2 - 1	50.2	1317	-	0.2000	7471B	PPB	24 May 2023 11:27:23	S	Std
2.5 - 1	52.5	16061	-	2.5000	7471B	PPB	24 May 2023 11:29:40	S	Std
5.0 - 1	55	31652	-	5.0000	7471B	PPB	24 May 2023 11:31:57	S	Std
7.5 - 1	57.5	47344	-	7.5000	7471B	PPB	24 May 2023 11:34:14	S	Std
10.0 - 1	510	66009	-	10.0000	7471B	PPB	24 May 2023 11:41:48	S	Std
ICV88 - 1	ICV88	27070	4.1961	-	7471B	PPB	24 May 2023 11:44:41	U	SMPL
ICB88 - 1	ICB88	-90	0.0218	-	7471B	PPB	24 May 2023 11:46:56	U	SMPL
CCV07 - 1	CCV07	32139	4.9751	-	7471B	PPB	24 May 2023 11:49:13	U	SMPL
CCB07 - 1	CCB07	-103	0.0198	-	7471B	PPB	24 May 2023 11:51:29	U	SMPL
CRA - 1	CRA	1269	0.2307	-	7471B	PPB	24 May 2023 11:53:47	U	SMPL
HighStd - 1	HighStd	67003	10.3335	-	7471B	PPB	24 May 2023 11:56:02	U	SMPL
ChkStd - 1	ChkStd	45039	6.9578	-	7471B	PPB	24 May 2023 11:58:17	U	SMPL
PB153006BL - 1	PBS	-319	-0.0134	-	7471B	PPB	24 May 2023 12:00:36	U	SMPL
PB153006BS - 1	LCSS	25809	4.0023	-	7471B	PPB	24 May 2023 12:05:31	U	SMPL
O2884-01 - 1	2001	3506	0.5745	-	7471B	PPB	24 May 2023 12:07:47	U	SMPL
O2884-02 - 1	2006	26031	4.0364	-	7471B	PPB	24 May 2023 12:10:06	U	SMPL
O2891-01 - 1	290-328	81292	12.5296	-	7471B	PPB	24 May 2023 12:12:25	U	SMPL
O2892-01 - 1	TP-30	6007	0.9589	-	7471B	PPB	24 May 2023 12:14:44	U	SMPL
O2892-04 - 1	TP-31	1844	0.3191	-	7471B	PPB	24 May 2023 12:17:02	U	SMPL
CCV08 - 1	CCV08	32529	5.0351	-	7471B	PPB	24 May 2023 12:19:18	U	SMPL
CCB08 - 1	CCB08	-16	0.0332	-	7471B	PPB	24 May 2023 12:21:33	U	SMPL
O2892-07 - 1	TP-33	1603	0.2820	-	7471B	PPB	24 May 2023 12:23:51	U	SMPL
O2892-10 - 1	TP-32	8873	1.3994	-	7471B	PPB	24 May 2023 12:26:07	U	SMPL
O2892-13 - 1	TP-29	536395	HIGH	-	7471B	PPB	24 May 2023 12:28:22	X	
O2894-01 - 1	TP-40A	3280	0.5398	-	7471B	PPB	24 May 2023 12:30:11	U	SMPL
O2894-04 - 1	TP-50A	5715	0.9140	-	7471B	PPB	24 May 2023 12:32:43	U	SMPL
O2894-04DUP - 1	TP-50ADUP	6211	0.9902	-	7471B	PPB	24 May 2023 12:34:59	U	SMPL
O2894-04MS - 1	TP-50AMS	33174	5.1342	-	7471B	PPB	24 May 2023 12:37:16	U	SMPL
O2894-04MSD - 1	TP-50AMSD	32105	4.9699	-	7471B	PPB	24 May 2023 12:39:33	U	SMPL
PB153007BL - 1	PBS	-111	0.0186	-	7471B	PPB	24 May 2023 12:41:53	U	SMPL
PB153007BS - 1	LCSS	24197	3.7545	-	7471B	PPB	24 May 2023 12:44:11	U	SMPL
CCV09 - 1	CCV09	32929	5.0966	-	7471B	PPB	24 May 2023 12:46:26	U	SMPL
CCB09 - 1	CCB09	-48	0.0283	-	7471B	PPB	24 May 2023 12:48:44	U	SMPL
O2886-01 - 1	WC-1	2550	0.4276	-	7471B	PPB	24 May 2023 12:51:01	U	SMPL
O2888-01 - 1	S-H4(BHF)	12738	1.9934	-	7471B	PPB	24 May 2023 12:53:17	U	SMPL
O2888-02 - 1	MID2-44(10-11)	205	0.0671	-	7471B	PPB	24 May 2023 12:55:33	U	SMPL
O2888-03 - 1	FS-SB-20(ELEV-28-26)	615	0.1302	-	7471B	PPB	24 May 2023 12:57:49	U	SMPL
O2888-04 - 1	FS-SB-20(ELEV-13-11)	329	0.0862	-	7471B	PPB	24 May 2023 13:00:05	U	SMPL
O2897-01 - 1	OILY-SOLIDS-0523	14896	2.3250	-	7471B	PPB	24 May 2023 13:02:21	U	SMPL
O2899-01 - 1	SB06A	3500	0.5736	-	7471B	PPB	24 May 2023 13:04:38	U	SMPL
O2899-02 - 1	SB06B	10374	1.6300	-	7471B	PPB	24 May 2023 13:06:57	U	SMPL
O2899-04 - 1	SB01	6292	1.0027	-	7471B	PPB	24 May 2023 13:09:14	U	SMPL
O2899-06 - 1	SB08	2038	0.3489	-	7471B	PPB	24 May 2023 13:11:30	U	SMPL
CCV10 - 1	CCV10	32670	5.0568	-	7471B	PPB	24 May 2023 13:13:46	U	SMPL
CCB10 - 1	CCB10	-84	0.0227	-	7471B	PPB	24 May 2023 13:16:01	U	SMPL
O2899-08 - 1	SB14	2604	0.4359	-	7471B	PPB	24 May 2023 13:18:20	U	SMPL
O2902-01 - 1	FMC-0096	622	0.1312	-	7471B	PPB	24 May 2023 13:20:35	U	SMPL
O2902-02 - 1	FMC-665	924	0.1777	-	7471B	PPB	24 May 2023 13:22:51	U	SMPL
O2904-01 - 1	EO-3-052323	2737	0.4563	-	7471B	PPB	24 May 2023 13:30:10	U	SMPL
O2904-01DUP - 1	EO-3-052323DUP	2678	0.4472	-	7471B	PPB	24 May 2023 13:32:26	U	SMPL
O2904-01MS - 1	EO-3-052323MS	28307	4.3862	-	7471B	PPB	24 May 2023 13:34:42	U	SMPL
O2904-01MSD - 1	EO-3-052323MSD	25463	3.9491	-	7471B	PPB	24 May 2023 13:36:59	U	SMPL
CCV11 - 1	CCV11	32227	4.9887	-	7471B	PPB	24 May 2023 13:39:19	U	SMPL
CCB11 - 1	CCB11	-105	0.0195	-	7471B	PPB	24 May 2023 13:41:37	U	SMPL
O2894-04LX5 - 1		1116	0.2072	-	7471B	PPB	24 May 2023 13:43:55	U	SMPL
O2894-04A - 1		32982	5.1047	-	7471B	PPB	24 May 2023 13:46:11	U	SMPL
O2904-01LX5 - 1		519	0.1154	-	7471B	PPB	24 May 2023 13:48:28	U	SMPL
O2904-01A - 1		29024	4.4964	-	7471B	PPB	24 May 2023 13:50:46	U	SMPL
O2891-01DLX2 - 1		40649	6.2831	-	7471B	PPB	24 May 2023 13:53:02	U	SMPL
O2892-13DLX10 - 1		97185	14.9722	-	7471B	PPB	24 May 2023 14:14:47	U	SMPL
O2892-13DLX50 - 1		20215	3.1425	-	7471B	PPB	24 May 2023 14:17:03	U	SMPL
CCV12 - 1	CCV12	32484	5.0282	-	7471B	PPB	24 May 2023 14:19:22	U	SMPL
CCB12 - 1	CCB12	-39	0.0296	-	7471B	PPB	24 May 2023 14:21:40	U	SMPL