

LB125781


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

39444

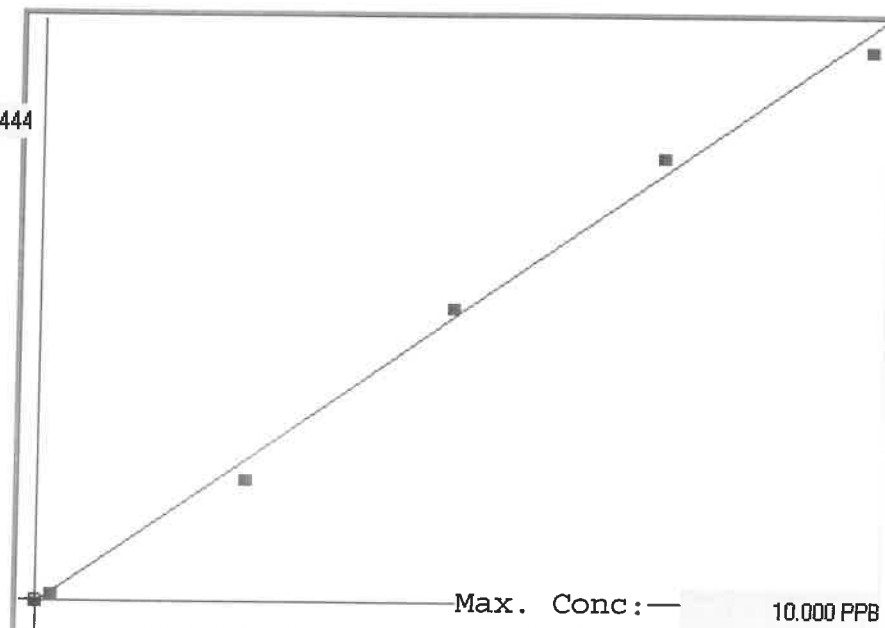

A= 0.0000e+000

B= 2.4410e-004

C= 5.4592e-002

Rho= 0.9978642

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.076	0.076	88	0.000	88	0				100
0.2	0.200	0.191	-0.009	557	0.0 %	557					-5
2.5	2.500	2.206	-0.294	8815	0.0 %	8815					-12
5.0	5.000	5.209	0.209	21116	0.0 %	21116					4
7.5	7.500	7.835	0.335	31874	0.0 %	31874					4
10.0	10.000	9.683	-0.317	39444	0.0 %	39444					-3

LB125781 IONSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 05 Jun 2023 11:47:34

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	88	-	0.0000	7470A	PPB	05 Jun 2023 11:56:01	S	Std
0.2 - 1	50.2	557	-	0.2000	7470A	PPB	05 Jun 2023 11:58:19	S	Std
2.5 - 1	52.5	8815	-	2.5000	7470A	PPB	05 Jun 2023 12:00:36	S	Std
5.0 - 1	55	21116	-	5.0000	7470A	PPB	05 Jun 2023 12:08:13	S	Std
7.5 - 1	57.5	31874	-	7.5000	7470A	PPB	05 Jun 2023 12:13:10	S	Std
10.0 - 1	511	39444	-	10.0000	7470A	PPB	05 Jun 2023 12:26:00	S	Std
ICV05 - 1	ICV05	15822	3.9168	-	7470A	PPB	05 Jun 2023 12:31:16	U	SMPL
ICB05 - 1	ICB05	-70	0.0375	-	7470A	PPB	05 Jun 2023 12:33:31	U	SMPL
CCV69 - 1	CCV69	21904	5.4014	-	7470A	PPB	05 Jun 2023 12:35:48	U	SMPL
CCB69 - 1	CCB69	-107	0.0285	-	7470A	PPB	05 Jun 2023 12:38:03	U	SMPL
CRA - 1	CRA	598	0.2006	-	7470A	PPB	05 Jun 2023 12:40:20	U	SMPL
HighStd - 1	HighStd	39286	9.6444	-	7470A	PPB	05 Jun 2023 12:42:35	U	SMPL
ChkStd - 1	ChkStd	29203	7.1831	-	7470A	PPB	05 Jun 2023 12:44:51	U	SMPL
PB153202BL - 1	PBW	-140	0.0204	-	7470A	PPB	05 Jun 2023 12:47:08	U	SMPL
PB153202BS - 1	LCSW	16728	4.1379	-	7470A	PPB	05 Jun 2023 12:49:26	U	SMPL
O3008-02 - 1	TP-18-0A	36	0.0634	-	7470A	PPB	05 Jun 2023 12:51:43	U	SMPL
O3008-05 - 1	TP-19-0A	-21	0.0495	-	7470A	PPB	05 Jun 2023 12:54:01	U	SMPL
O3016-02 - 1	WC28	-6	0.0531	-	7470A	PPB	05 Jun 2023 12:56:18	U	SMPL
O3016-05 - 1	WC29	21	0.0597	-	7470A	PPB	05 Jun 2023 12:58:35	U	SMPL
O3018-04 - 1	362	40	0.0644	-	7470A	PPB	05 Jun 2023 13:00:51	U	SMPL
CCV70 - 1	CCV70	21504	5.3037	-	7470A	PPB	05 Jun 2023 13:03:07	U	SMPL
CCB70 - 1	CCB70	-94	0.0316	-	7470A	PPB	05 Jun 2023 13:05:23	U	SMPL
O3018-06 - 1	348	50	0.0668	-	7470A	PPB	05 Jun 2023 13:07:39	U	SMPL
O3018-08 - 1	343	130	0.0863	-	7470A	PPB	05 Jun 2023 13:09:54	U	SMPL
O3018-10 - 1	72-11991	81	0.0744	-	7470A	PPB	05 Jun 2023 13:12:10	U	SMPL
O3018-12 - 1	278	42	0.0648	-	7470A	PPB	05 Jun 2023 13:14:26	U	SMPL
O3018-14 - 1	RT-4648	55	0.0680	-	7470A	PPB	05 Jun 2023 13:16:42	U	SMPL
O3020-04 - 1	M-060123RB04	32	0.0624	-	7470A	PPB	05 Jun 2023 13:18:58	U	SMPL
O3029-02 - 1	TP-6	18	0.0590	-	7470A	PPB	05 Jun 2023 13:21:15	U	SMPL
O3029-05 - 1	TP-7	34	0.0629	-	7470A	PPB	05 Jun 2023 13:23:32	U	SMPL
O3029-08 - 1	TP-8	21	0.0597	-	7470A	PPB	05 Jun 2023 13:25:49	U	SMPL
O3029-11 - 1	TP-9	15	0.0583	-	7470A	PPB	05 Jun 2023 13:28:05	U	SMPL
CCV71 - 1	CCV71	21047	5.1922	-	7470A	PPB	05 Jun 2023 13:30:21	U	SMPL
CCB71 - 1	CCB71	-92	0.0321	-	7470A	PPB	05 Jun 2023 13:32:37	U	SMPL
O3029-14 - 1	TP-10	13	0.0578	-	7470A	PPB	05 Jun 2023 13:34:54	U	SMPL
O3032-02 - 1	TP-20-0A	23	0.0602	-	7470A	PPB	05 Jun 2023 13:37:10	U	SMPL
O3032-05 - 1	TP-21-0A	27	0.0612	-	7470A	PPB	05 Jun 2023 13:39:26	U	SMPL
O3032-05DUP - 1	TP-21-0ADUP	8	0.0565	-	7470A	PPB	05 Jun 2023 13:41:42	U	SMPL
O3032-05MS - 1	TP-21-0AMS	15836	3.9202	-	7470A	PPB	05 Jun 2023 13:43:58	U	SMPL
O3032-05MSD - 1	TP-21-0AMSD	16879	4.1748	-	7470A	PPB	05 Jun 2023 13:46:15	U	SMPL
PB153203BL - 1	PBW	-138	0.0209	-	7470A	PPB	05 Jun 2023 13:48:32	U	SMPL
PB153203BS - 1	LCSW	17783	4.3954	-	7470A	PPB	05 Jun 2023 13:50:51	U	SMPL
O2997-01 - 1	DMA-1103	-114	0.0268	-	7470A	PPB	05 Jun 2023 13:53:08	U	SMPL
O2997-01DUP - 1	DMA-1103DUP	18	0.0590	-	7470A	PPB	05 Jun 2023 13:55:26	U	SMPL
CCV72 - 1	CCV72	21059	5.1951	-	7470A	PPB	05 Jun 2023 13:57:41	U	SMPL
CCB72 - 1	CCB72	-83	0.0343	-	7470A	PPB	05 Jun 2023 13:59:57	U	SMPL
O2997-01MS - 1	DMA-1103MS	16734	4.1394	-	7470A	PPB	05 Jun 2023 14:02:14	U	SMPL
O2997-01MSD - 1	DMA-1103MSD	17799	4.3993	-	7470A	PPB	05 Jun 2023 14:04:31	U	SMPL
O2997-02 - 1	DMA-1105	-149	0.0182	-	7470A	PPB	05 Jun 2023 14:06:47	U	SMPL
PB153210BL - 1	PBW	-13	0.0514	-	7470A	PPB	05 Jun 2023 14:09:05	U	SMPL
PB153210BS - 1	LCSW	15942	3.9461	-	7470A	PPB	05 Jun 2023 14:11:21	U	SMPL
O3016-06 - 1	B-45(OW)	688	0.2225	-	7470A	PPB	05 Jun 2023 14:13:37	U	SMPL
O3016-06DUP - 1	B-45(OW)DUP	484	0.1727	-	7470A	PPB	05 Jun 2023 14:18:37	U	SMPL
O3016-06MS - 1	B-45(OW)MS	17442	4.3122	-	7470A	PPB	05 Jun 2023 14:20:54	U	SMPL
O3016-06MSD - 1	B-45(OW)MSD	17237	4.2622	-	7470A	PPB	05 Jun 2023 14:25:53	U	SMPL
O3016-07 - 1	B-45(OW)	-101	0.0299	-	7470A	PPB	05 Jun 2023 14:28:09	U	SMPL
CCV73 - 1	CCV73	19399	4.7899	-	7470A	PPB	05 Jun 2023 14:30:26	U	SMPL
CCB73 - 1	CCB73	-98	0.0307	-	7470A	PPB	05 Jun 2023 14:32:42	U	SMPL
O3019-01 - 1	MH-289	271	0.1207	-	7470A	PPB	05 Jun 2023 14:34:59	U	SMPL
PB153186TB - 1	PB153186TB	-71	0.0373	-	7470A	PPB	05 Jun 2023 14:37:15	U	SMPL
PB153192TB - 1	PB153192TB	24	0.0605	-	7470A	PPB	05 Jun 2023 14:39:31	U	SMPL
O3032-05LX5 - 1		3	0.0553	-	7470A	PPB	05 Jun 2023 14:41:47	U	SMPL
O3032-05A - 1		15227	3.7715	-	7470A	PPB	05 Jun 2023 14:44:03	U	SMPL
O2997-01LX5 - 1		-84	0.0341	-	7470A	PPB	05 Jun 2023 14:46:19	U	SMPL
O2997-01A - 1		15939	3.9453	-	7470A	PPB	05 Jun 2023 14:57:26	U	SMPL
O3016-06LX5 - 1		-89	0.0329	-	7470A	PPB	05 Jun 2023 14:59:42	U	SMPL
O3016-06A - 1		17792	4.3976	-	7470A	PPB	05 Jun 2023 15:02:01	U	SMPL
CCV74 - 1	CCV74	19112	4.7199	-	7470A	PPB	05 Jun 2023 15:04:17	U	SMPL
CCB74 - 1	CCB74	-132	0.0224	-	7470A	PPB	05 Jun 2023 15:06:35	U	SMPL