

LB125822


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

46120

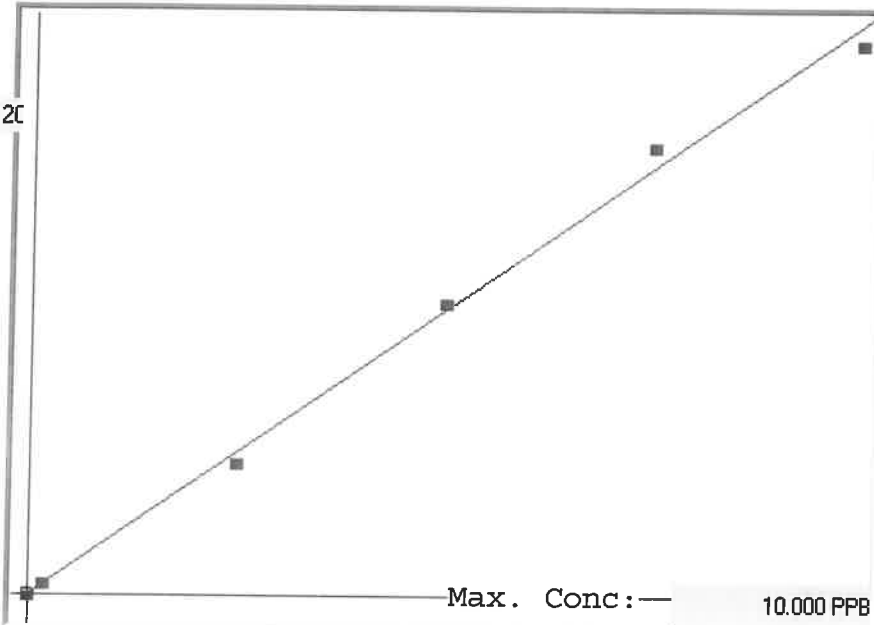

A= 0.0000e+000

B= 2.0987e-004

C= -7.2765e-003

Rho= 0.9982322

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	1/2/3/4/5
0.0	0.000	-0.006	-0.006	8	0.000	8	0				
0.2	0.200	0.204	0.004	1009	0.0 %	1009					1
2.5	2.500	2.335	-0.165	11159	0.0 %	11159					2
5.0	5.000	5.122	0.122	24439	0.0 %	24439					3
7.5	7.500	7.873	0.373	37546	0.0 %	37546					4
10.0	10.000	9.672	-0.328	46120	0.0 %	46120					5

LB125822 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 07 Jun 2023 10:56:01

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	8	-	0.0000	7470A	PPB	07 Jun 2023 11:03:19	S	Std
0.2 - 1	50.2	1009	-	0.2000	7470A	PPB	07 Jun 2023 11:05:37	S	Std
2.5 - 1	52.5	11159	-	2.5000	7470A	PPB	07 Jun 2023 11:07:55	S	Std
5.0 - 1	55	24439	-	5.0000	7470A	PPB	07 Jun 2023 11:10:12	S	Std
7.5 - 1	57.5	37546	-	7.5000	7470A	PPB	07 Jun 2023 11:12:29	S	Std
10.0 - 1	510	46120	-	10.0000	7470A	PPB	07 Jun 2023 11:20:04	S	Std
ICV09 - 1	ICV09	17978	3.7658	-	7470A	PPB	07 Jun 2023 11:23:02	U	SMPL
ICB09 - 1	ICB09	-166	-0.0421	-	7470A	PPB	07 Jun 2023 11:25:17	U	SMPL
CCV86 - 1	CCV86	23725	4.9719	-	7470A	PPB	07 Jun 2023 11:27:33	U	SMPL
CCB86 - 1	CCB86	-166	-0.0421	-	7470A	PPB	07 Jun 2023 11:29:49	U	SMPL
CRA - 1	CRA	973	0.1969	-	7470A	PPB	07 Jun 2023 11:32:05	U	SMPL
HighStd - 1	HighStd	45741	9.5925	-	7470A	PPB	07 Jun 2023 11:34:20	U	SMPL
ChkStd - 1	ChkStd	33900	7.1074	-	7470A	PPB	07 Jun 2023 11:36:36	U	SMPL
PB153256BL - 1	PBW	-148	-0.0383	-	7470A	PPB	07 Jun 2023 11:38:54	U	SMPL
PB153256BS - 1	LCSW	19480	4.0810	-	7470A	PPB	07 Jun 2023 11:46:01	U	SMPL
O3039-07 - 1	MW-34	457	0.0886	-	7470A	PPB	07 Jun 2023 11:48:17	U	SMPL
O3039-07DUP - 1	MW-34DUP	445	0.0861	-	7470A	PPB	07 Jun 2023 11:53:13	U	SMPL
O3039-07MS - 1	MW-34MS	16953	3.5507	-	7470A	PPB	07 Jun 2023 11:55:30	U	SMPL
O3039-07MSD - 1	MW-34MSD	16958	3.5517	-	7470A	PPB	07 Jun 2023 11:57:47	U	SMPL
O3039-08 - 1	MW-34	-73	-0.0226	-	7470A	PPB	07 Jun 2023 12:00:04	U	SMPL
CCV87 - 1	CCV87	22841	4.7864	-	7470A	PPB	07 Jun 2023 12:02:21	U	SMPL
CCB87 - 1	CCB87	-128	-0.0341	-	7470A	PPB	07 Jun 2023 12:04:37	U	SMPL
O3046-01 - 1	COMP-1-1-5	366	0.0695	-	7470A	PPB	07 Jun 2023 12:06:54	U	SMPL
O3046-07 - 1	COMP-2-6-10	292	0.0540	-	7470A	PPB	07 Jun 2023 12:09:09	U	SMPL
O3046-13 - 1	COMP-3-11-15	1064	0.2160	-	7470A	PPB	07 Jun 2023 12:11:26	U	SMPL
O3047-07 - 1	MW-41	-46	-0.0169	-	7470A	PPB	07 Jun 2023 12:13:42	U	SMPL
O3047-08 - 1	MW-41	42	0.0015	-	7470A	PPB	07 Jun 2023 12:16:00	U	SMPL
O3047-10 - 1	TWP-07	425	0.0819	-	7470A	PPB	07 Jun 2023 12:18:17	U	SMPL
O3047-11 - 1	TWP-07	-99	-0.0281	-	7470A	PPB	07 Jun 2023 12:20:33	U	SMPL
PB153257BL - 1	PBW	15	-0.0041	-	7470A	PPB	07 Jun 2023 12:22:50	U	SMPL
PB153257BS - 1	LCSW	15633	3.2737	-	7470A	PPB	07 Jun 2023 12:25:08	U	SMPL
O3024-01 - 1	TOPSOIL-OU3-GRILLO-1	641	0.1273	-	7470A	PPB	07 Jun 2023 12:30:31	U	SMPL
CCV88 - 1	CCV88	23526	4.9302	-	7470A	PPB	07 Jun 2023 12:32:46	U	SMPL
CCB88 - 1	CCB88	-100	-0.0283	-	7470A	PPB	07 Jun 2023 12:35:02	U	SMPL
O3024-01DUP - 1	TOPSOIL-OU3-GRILLO-1DUP	489	0.0954	-	7470A	PPB	07 Jun 2023 12:37:19	U	SMPL
O3024-01MS - 1	TOPSOIL-OU3-GRILLO-1MS	16014	3.3536	-	7470A	PPB	07 Jun 2023 12:39:34	U	SMPL
O3024-01MSD - 1	TOPSOIL-OU3-GRILLO-1MSD	15955	3.3412	-	7470A	PPB	07 Jun 2023 12:41:50	U	SMPL
PB153257TB - 1	PB153195TB	-89	-0.0260	-	7470A	PPB	07 Jun 2023 12:44:07	U	SMPL
O3024-01LX5 - 1		-6	-0.0085	-	7470A	PPB	07 Jun 2023 12:46:24	U	SMPL
O3024-01A - 1		19805	4.1492	-	7470A	PPB	07 Jun 2023 12:48:41	U	SMPL
O3039-07LX5 - 1		-78	-0.0236	-	7470A	PPB	07 Jun 2023 12:50:57	U	SMPL
O3039-07A - 1		20902	4.3795	-	7470A	PPB	07 Jun 2023 12:53:16	U	SMPL
CCV89 - 1	CCV89	24130	5.0569	-	7470A	PPB	07 Jun 2023 12:55:33	U	SMPL
CCB89 - 1	CCB89	-85	-0.0251	-	7470A	PPB	07 Jun 2023 12:57:50	U	SMPL