

Clear table

| Instrument ID: IC-2 |                      |                       |                       |                       |                       |                        |                       |                    |               | Analyst : IZ |  | Method: 300.0 / 9056A |  | Initial wt/<br>Final Vol |  |
|---------------------|----------------------|-----------------------|-----------------------|-----------------------|-----------------------|------------------------|-----------------------|--------------------|---------------|--------------|--|-----------------------|--|--------------------------|--|
| ident               | concentra<br>tion F- | concentratio<br>n CL- | concentrati<br>on NO2 | concentrati<br>on BR- | concentrati<br>on NO3 | concentrati<br>on HPO4 | concentrati<br>on SO4 | file name          | date time     |              |  |                       |  |                          |  |
| STD1                | 0.0000               | 0.0000                | 0.0000                | 0.0000                | 0.0000                | 0.0000                 | 0.0000                | 0.0000_2023-05-24_ | 5/24/23 11:45 | IZ/MA        |  |                       |  |                          |  |
| STD2                | 0.4650               | 0.6450                | 0.6890                | 2.2470                | 0.5640                | 1.1610                 | 3.4730                | 2023-05-24_        | 5/24/23 12:14 | IZ/MA        |  |                       |  |                          |  |
| STD3                | 0.8420               | 1.1870                | 1.1910                | 3.9750                | 0.9980                | 1.9540                 | 5.9810                | 2023-05-24_        | 5/24/23 12:44 | IZ/MA        |  |                       |  |                          |  |
| STD4                | 1.0050               | 1.5490                | 1.5190                | 5.0350                | 1.2650                | 2.5300                 | 7.5390                | 2023-05-24_        | 5/24/23 13:14 | IZ/MA        |  |                       |  |                          |  |
| STD5                | 1.8220               | 2.9260                | 2.9020                | 9.7750                | 2.4290                | 4.8170                 | 14.5120               | 2023-05-24_        | 5/24/23 13:43 | IZ/MA        |  |                       |  |                          |  |
| STD6                | 3.9990               | 5.8960                | 5.8810                | 19.5890               | 4.8900                | 9.9100                 | 29.3750               | 2023-05-24_        | 5/24/23 14:13 | IZ/MA        |  |                       |  |                          |  |
| STD7                | 5.0490               | 7.5980                | 7.6190                | 25.3790               | 6.3530                | 12.6260                | 38.1190               | 2023-05-24_        | 5/24/23 14:43 | IZ/MA        |  |                       |  |                          |  |
| ICV                 | 1.8290               | 2.9850                | 3.0620                | 9.9450                | 2.5060                | 4.6940                 | 14.7450               | 2023-05-24_        | 5/24/23 15:12 | IZ/MA        |  |                       |  |                          |  |
| ICB                 | 0.0000               | 0.0000                | 0.0000                | 0.0000                | 0.0000                | 0.0000                 | 0.0000                | 2023-05-24_        | 5/24/23 15:45 | IZ/MA        |  |                       |  |                          |  |
| CCV                 | 1.9040               | 2.8540                | 2.7150                | 9.4370                | 2.3470                | 5.0530                 | 14.0730               | 2023-06-13_        | 6/13/23 10:23 | IZ/MA        |  |                       |  |                          |  |
| CCB                 | 0.0000               | 0.0000                | 0.0000                | 0.0000                | 0.0000                | 0.0000                 | 0.0000                | 2023-06-13_        | 6/13/23 10:53 | IZ/MA        |  |                       |  |                          |  |
| LB125948BLW         | 0.0000               | 0.0000                | 0.0000                | 0.0000                | 0.0000                | 0.0000                 | 0.0000                | 2023-06-13_        | 6/13/23 11:22 | IZ/MA        |  |                       |  |                          |  |
| LB125948BSW         | 1.8880               | 2.8760                | 2.7220                | 9.4680                | 2.3710                | 5.3300                 | 14.2380               | 2023-06-13_        | 6/13/23 11:52 | IZ/MA        |  |                       |  |                          |  |
| O3175-01            | 0.0000               | 0.4020                | 0.0000                | 0.0000                | 0.2460                | 0.0000                 | 1.1010                | 2023-06-13_        | 6/13/23 12:27 | IZ/MA        |  |                       |  |                          |  |
| O3175-02            | 0.0000               | 0.0000                | 0.0000                | 0.0000                | 0.2070                | 0.0000                 | 1.1100                | 2023-06-13_        | 6/13/23 12:56 | IZ/MA        |  |                       |  |                          |  |
| O3175-03            | 0.0000               | 0.0000                | 0.0000                | 0.0000                | 0.2470                | 0.0000                 | 1.0980                | 2023-06-13_        | 6/13/23 13:26 | IZ/MA        |  |                       |  |                          |  |
| O3176-01            | 0.0000               | 0.0000                | 0.0000                | 0.0000                | 0.2610                | 0.0000                 | 1.0950                | 2023-06-13_        | 6/13/23 13:55 | IZ/MA        |  |                       |  |                          |  |
| O3176-01MS          | 2.0250               | 2.9880                | 2.7130                | 9.7550                | 2.5910                | 5.5950                 | 14.6840               | 2023-06-13_        | 6/13/23 14:25 | IZ/MA        |  |                       |  |                          |  |
| O3176-01MSD         | 1.8800               | 2.9380                | 2.7030                | 9.5620                | 2.6030                | 5.1900                 | 14.3220               | 2023-06-13_        | 6/13/23 14:55 | IZ/MA        |  |                       |  |                          |  |
| O3079-01X10         | 0.0000               | 152.8920              | 0.0000                | 1.0810                | 0.0000                | 0.7820                 | 2.9770                | 2023-06-13_        | 6/13/23 15:24 | IZ/MA        |  |                       |  |                          |  |
| O3079-01DLX300      | 0.0000               | 3.6690                | 0.0000                | 0.0000                | 0.0000                | 0.0000                 | 1.1450                | 2023-06-13_        | 6/13/23 15:54 | IZ/MA        |  |                       |  |                          |  |
| CCV                 | 1.8930               | 2.8530                | 2.9370                | 9.3830                | 2.3680                | 5.3710                 | 14.1130               | 2023-06-13_        | 6/13/23 16:24 | IZ/MA        |  |                       |  |                          |  |
| CCB                 | 0.0000               | 0.0000                | 0.0000                | 0.0000                | 0.0000                | 0.0000                 | 0.0000                | 2023-06-13_        | 6/13/23 17:00 | IZ/MA        |  |                       |  |                          |  |

Report date: 6/14/2023 1:38:10 PM  
Printed by: wet


Ident: CCV  
Analysis from: 6/13/2023 10:23:16 AM  
File: \_2023-06-13\_

Last save: 6/13/2023 10:50:16 AM

Method: AnionsIC2-052423.mtw  
Run operator: wet  
Analysis number: 34570

Last save: 5/25/2023 9:20:

SAMPLE:  
: IZ/MA  
Vial number: 15  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

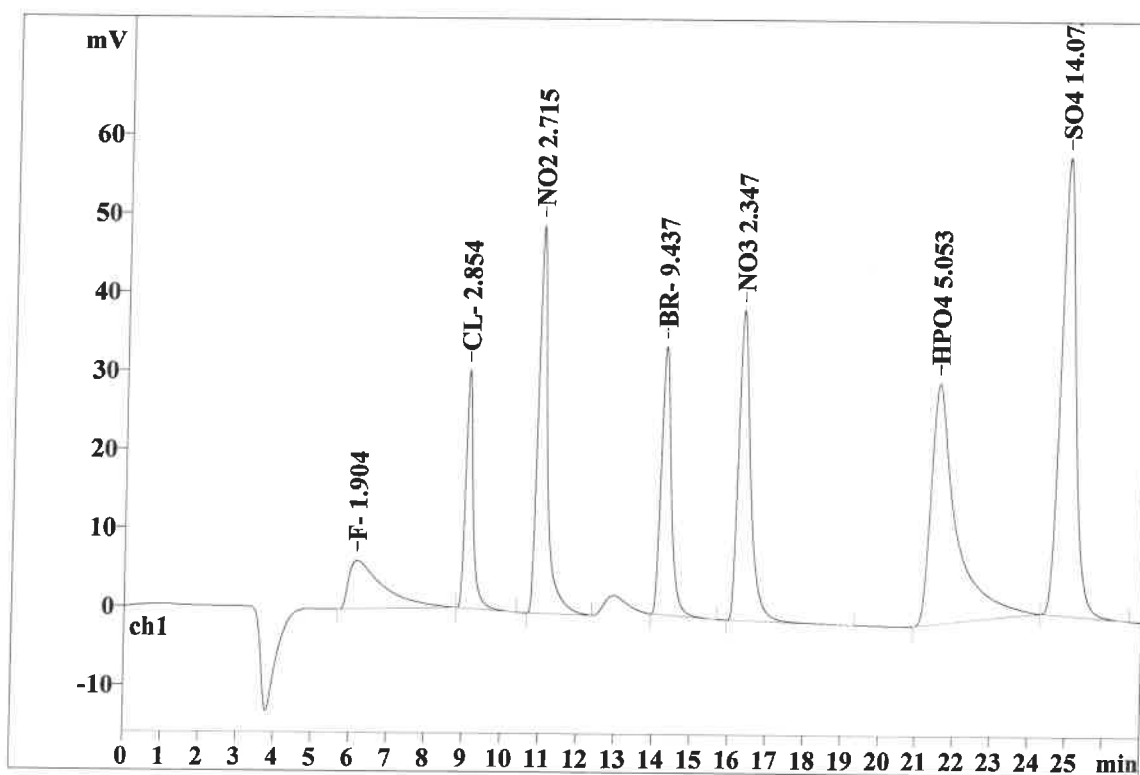

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 6.16             | 0.899          | 6.13         | 2.47        | 391.146        | 6.23      |
| 2  | 9.08             | 0.197          | 30.34        | 12.22       | 423.461        | 6.75      |
| 3  | 10.96            | 0.238          | 49.30        | 19.86       | 861.182        | 13.72     |
| 4  | 14.25            | 0.271          | 34.13        | 13.75       | 628.909        | 10.02     |
| 5  | 16.28            | 0.328          | 39.47        | 15.90       | 892.933        | 14.23     |
| 6  | 21.53            | 0.589          | 30.60        | 12.33       | 1450.203       | 23.11     |
| 7  | 24.92            | 0.418          | 58.27        | 23.47       | 1628.571       | 25.95     |
| 7  | 27.00            | 0.420          | 248.25       | 100.00      | 6276.404       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 6/14/2023 1:38:18 PM  
Printed by: wet


Ident: CCB  
Analysis from: 6/13/2023 10:53:14 AM  
File: \_2023-06-13\_

Last save: 6/13/2023 11:20:14 AM

Method: AnionsIC2-052423.mtw  
Run operator: wet  
Analysis number: 34571

Last save: 5/25/2023 9:20:

SAMPLE:  
: IZ/MA  
Vial number: 12  
Volume: 20.0  $\mu$ L  
Dilution: 1.00  
Amount: 1.0000

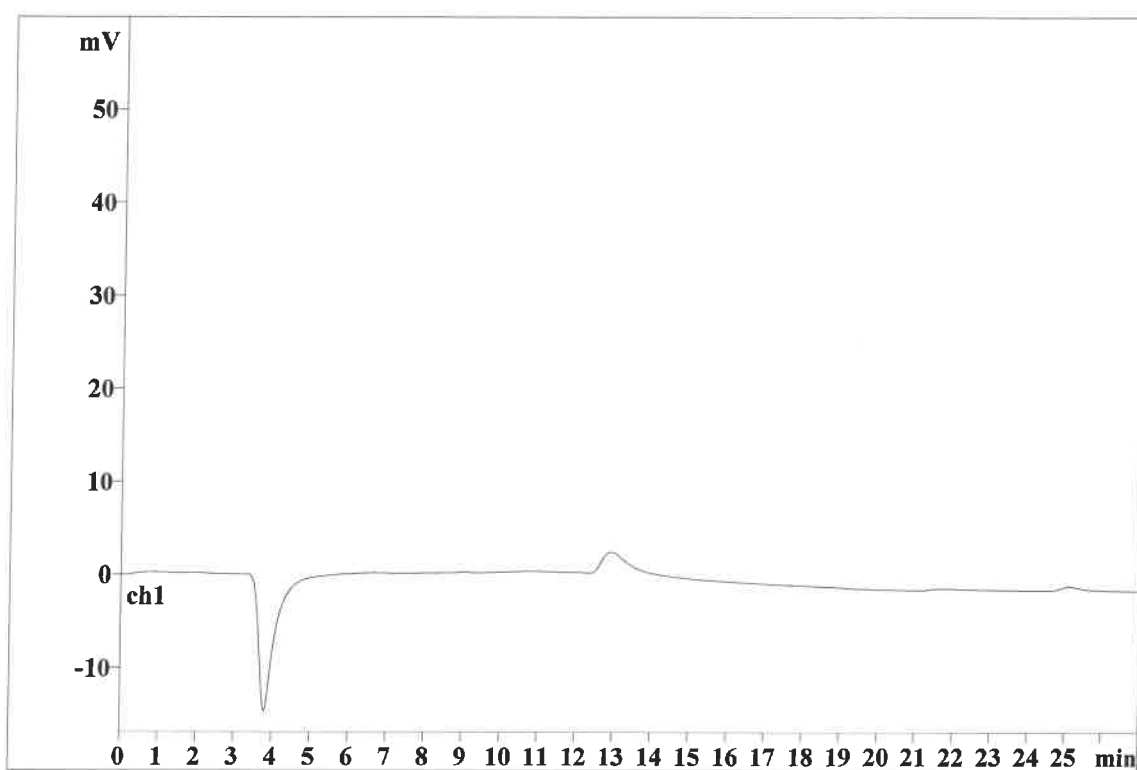

Quantitation method: Custom

No peaks

This report has been created by IC Net  
METROHM LTD

Report date: 6/14/2023 1:41:06 PM  
Printed by: wet


Ident: LB125948BLW  
Analysis from: 6/13/2023 11:22:52 AM  
File: \_2023-06-13\_

Last save: 6/14/2023 1:41:02 PM

Method: AnionsIC2-052423.mtw  
Run operator: wet  
Analysis number: 34572

Last save: 5/25/2023 9:20:

SAMPLE:  
: IZ/MA  
Vial number: 13  
Volume: 20.0  $\mu$ L  
Dilution: 1.00  
Amount: 1.0000

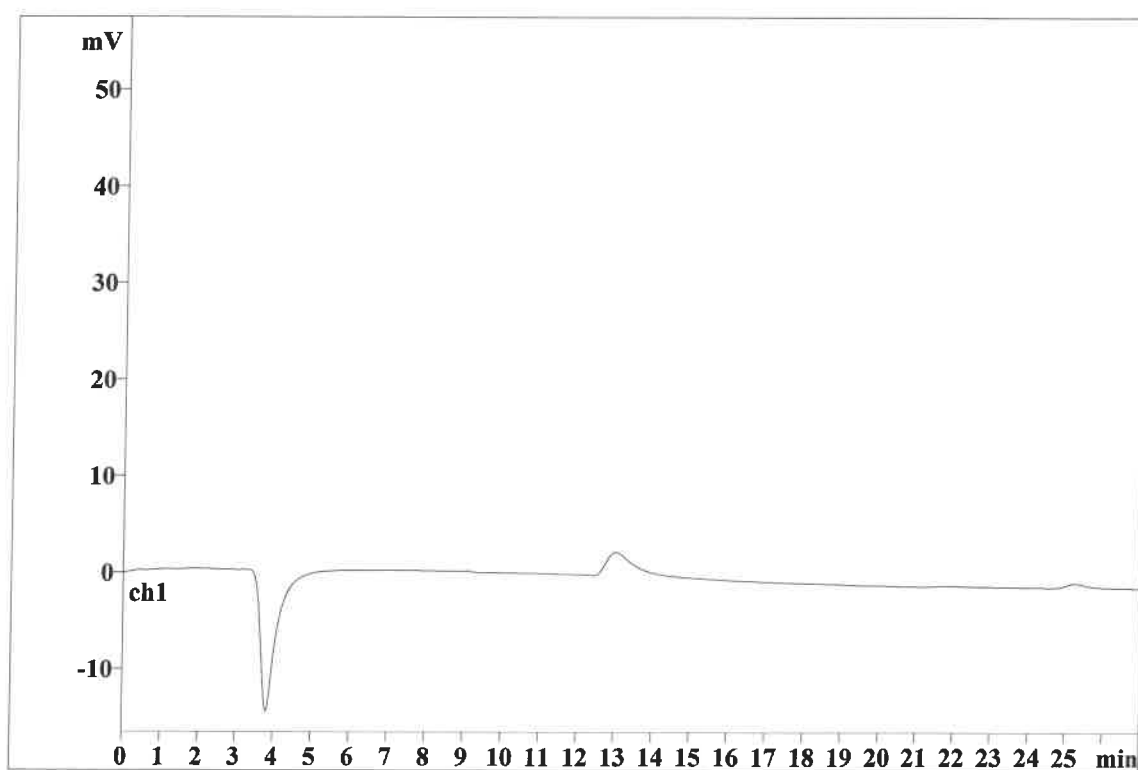

Quantitation method: Custom

No peaks

This report has been created by IC Net  
METROHM LTD

Report date: 6/14/2023 1:41:12 PM  
Printed by: wet


Ident: LB125948BSW  
Analysis from: 6/13/2023 11:52:29 AM  
File: \_2023-06-13\_

Last save: 6/14/2023 1:37:52 PM

Method: AnionsIC2-052423.mtw  
Run operator: wet  
Analysis number: 34573

Last save: 5/25/2023 9:20:

SAMPLE:  
: IZ/MA  
Vial number: 14  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

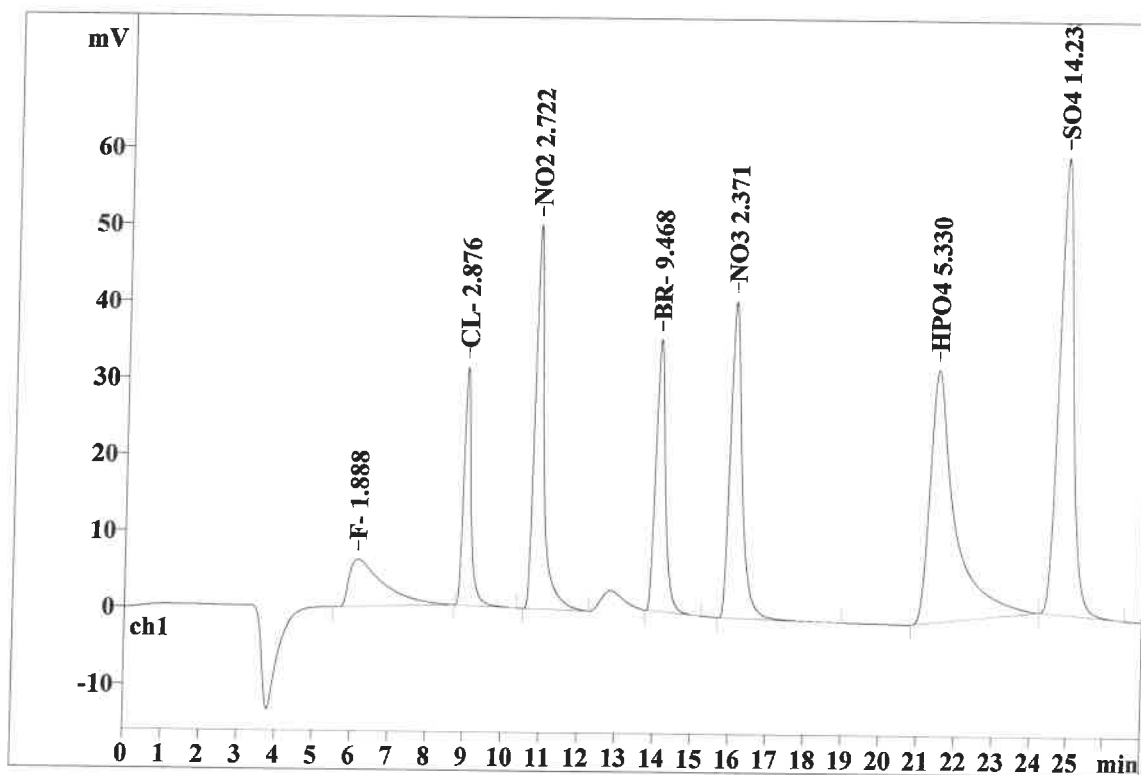

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 6.14             | 0.908          | 6.14         | 2.39        | 387.249        | 6.05      |
| 2  | 8.99             | 0.194          | 31.07        | 12.10       | 426.835        | 6.67      |
| 3  | 10.83            | 0.234          | 50.14        | 19.54       | 863.638        | 13.49     |
| 4  | 14.06            | 0.264          | 35.49        | 13.83       | 631.117        | 9.86      |
| 5  | 16.04            | 0.319          | 41.26        | 16.07       | 902.658        | 14.10     |
| 6  | 21.44            | 0.582          | 32.96        | 12.84       | 1540.027       | 24.06     |
| 7  | 24.81            | 0.414          | 59.62        | 23.23       | 1648.953       | 25.76     |
| 7  | 27.00            | 0.416          | 256.68       | 100.00      | 6400.477       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 6/14/2023 1:41:20 PM  
Printed by: wet


Ident: 03175-01  
Analysis from: 6/13/2023 12:27:02 PM  
File: \_2023-06-13\_

Last save: 6/13/2023 12:54:02 PM

Method: AnionsIC2-052423.mtw  
Run operator: wet  
Analysis number: 34574

Last save: 5/25/2023 9:20:

SAMPLE:  
: IZ/MA  
Vial number: 17  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

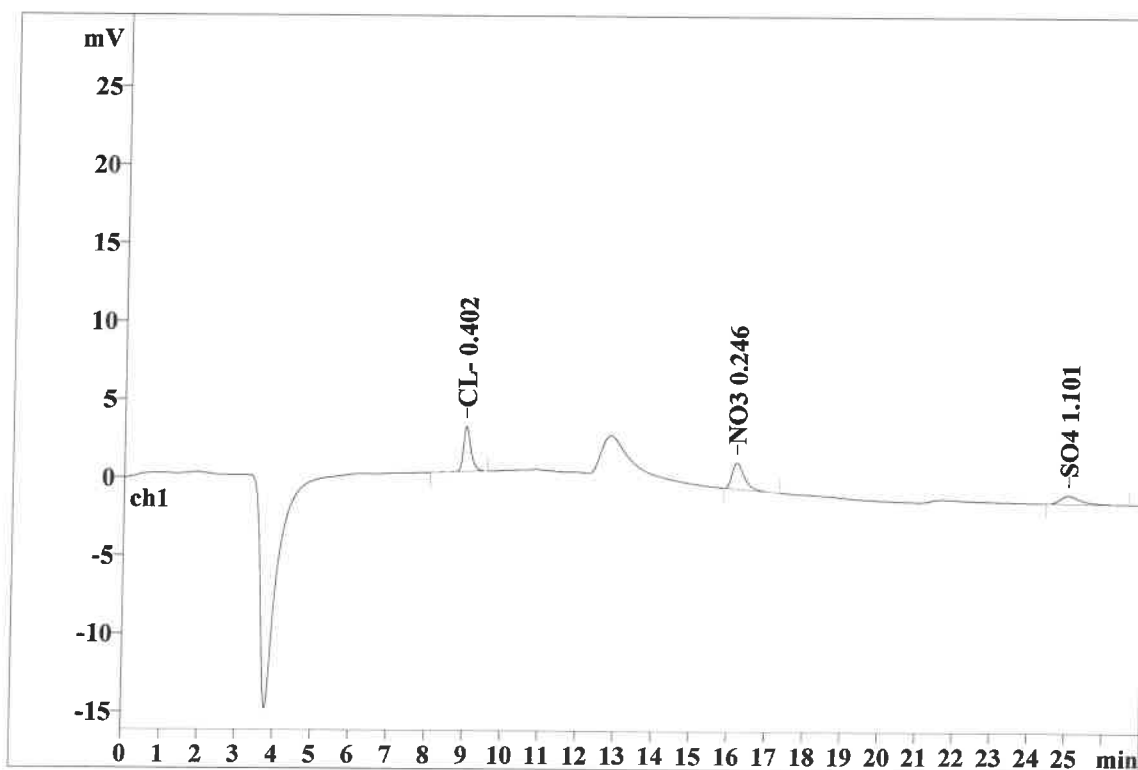

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 9.00             | 0.199          | 2.90         | 56.57       | 39.780         | 40.50     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 16.17            | 0.332          | 1.69         | 32.96       | 37.665         | 38.35     |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 25.01            | 0.572          | 0.53         | 10.38       | 20.777         | 21.15     |
| 7  | 27.00            | 0.158          | 5.12         | 99.91       | 98.222         | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 6/14/2023 1:41:27 PM  
Printed by: wet


Ident: O3175-02  
Analysis from: 6/13/2023 12:56:40 PM  
File: \_2023-06-13\_

Last save: 6/13/2023 1:23:40 PM

Method: AnionsIC2-052423.mtw  
Run operator: wet  
Analysis number: 34575

Last save: 5/25/2023 9:20:

SAMPLE:  
: IZ/MA  
Vial number: 18  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

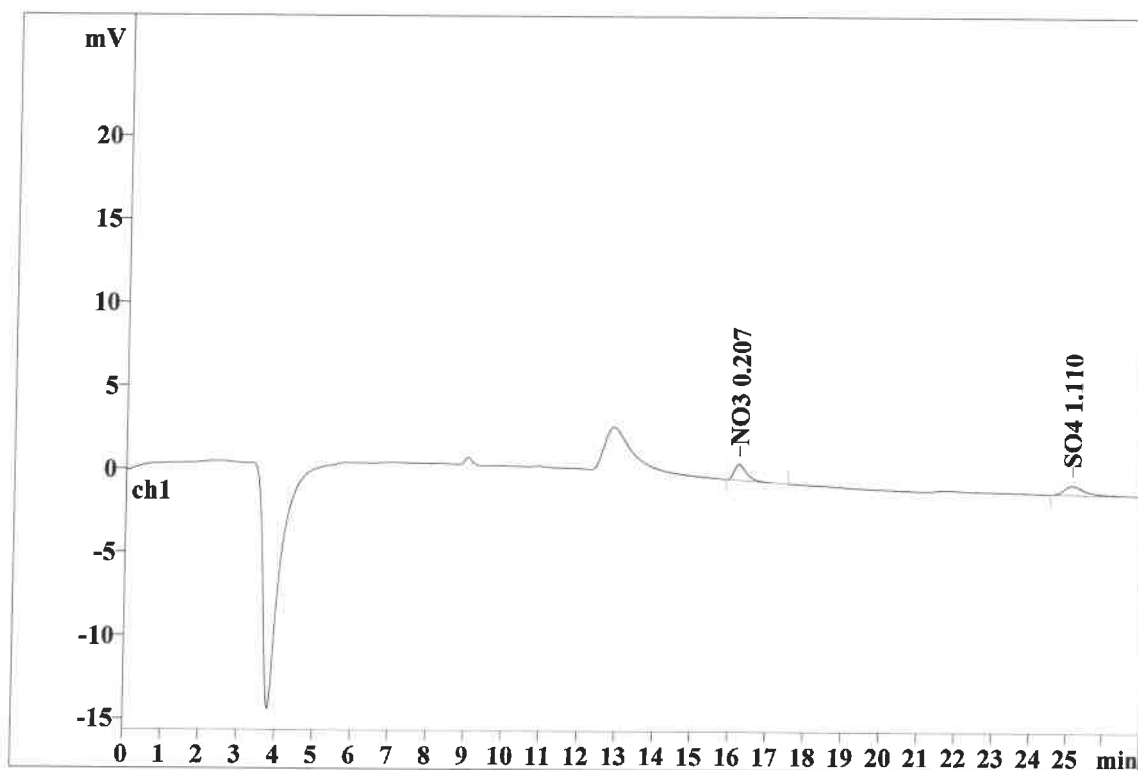

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 16.20            | 0.335          | 0.96         | 63.64       | 21.932         | 50.00     |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 25.08            | 0.580          | 0.55         | 36.13       | 21.930         | 50.00     |
| 7  | 27.00            | 0.131          | 1.51         | 99.77       | 43.862         | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 6/14/2023 1:41:35 PM  
Printed by: wet


Ident: O3175-03  
Analysis from: 6/13/2023 1:26:18 PM  
File: \_2023-06-13\_

Last save: 6/13/2023 1:53:18 PM

Method: AnionsIC2-052423.mtw  
Run operator: wet  
Analysis number: 34576

Last save: 5/25/2023 9:20:

SAMPLE:  
: IZ/MA  
Vial number: 19  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

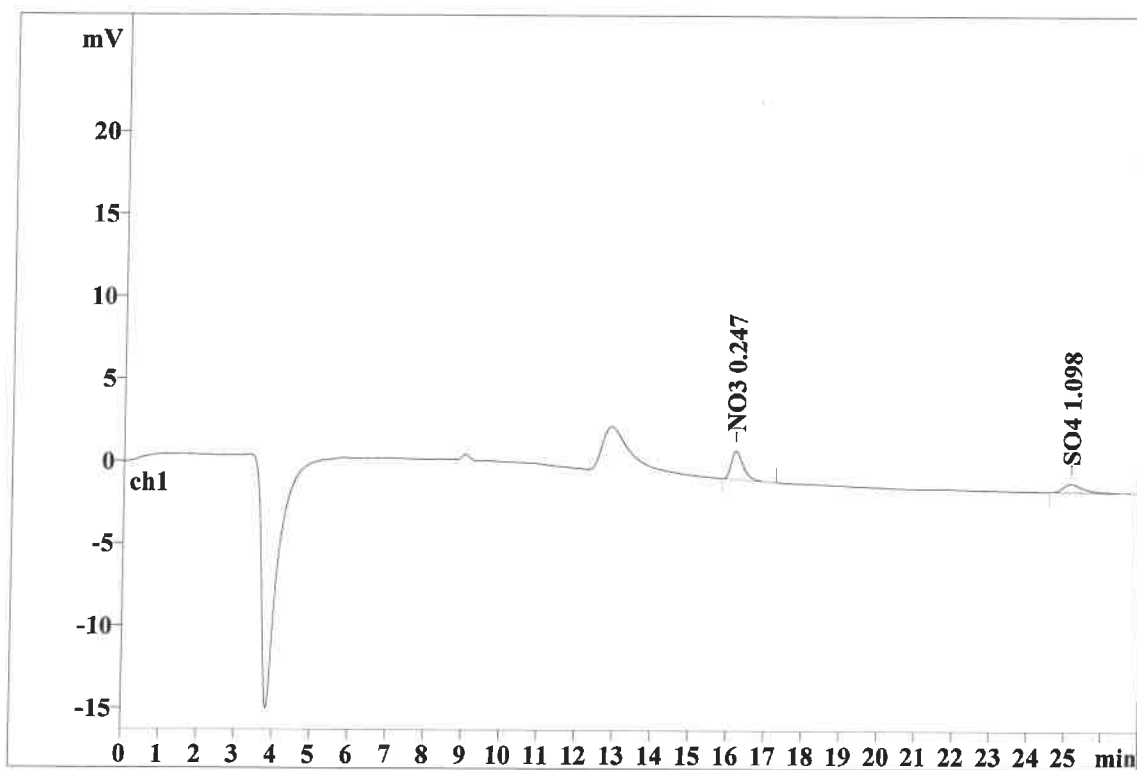

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 16.17            | 0.332          | 1.72         | 76.85       | 38.121         | 65.05     |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 25.11            | 0.573          | 0.51         | 23.00       | 20.485         | 34.95     |
| 7  | 27.00            | 0.129          | 2.23         | 99.86       | 58.605         | 100.00    |

This report has been created by IC Net  
METROHM LTD



Report date: 6/14/2023 1:41:42 PM  
Printed by: wet


Ident: 03176-01  
Analysis from: 6/13/2023 1:55:56 PM  
File: \_2023-06-13\_

Last save: 6/13/2023 2:22:56 PM

Method: AnionsIC2-052423.mtw  
Run operator: wet  
Analysis number: 34577

Last save: 5/25/2023 9:20:

SAMPLE:  
: IZ/MA  
Vial number: 20  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

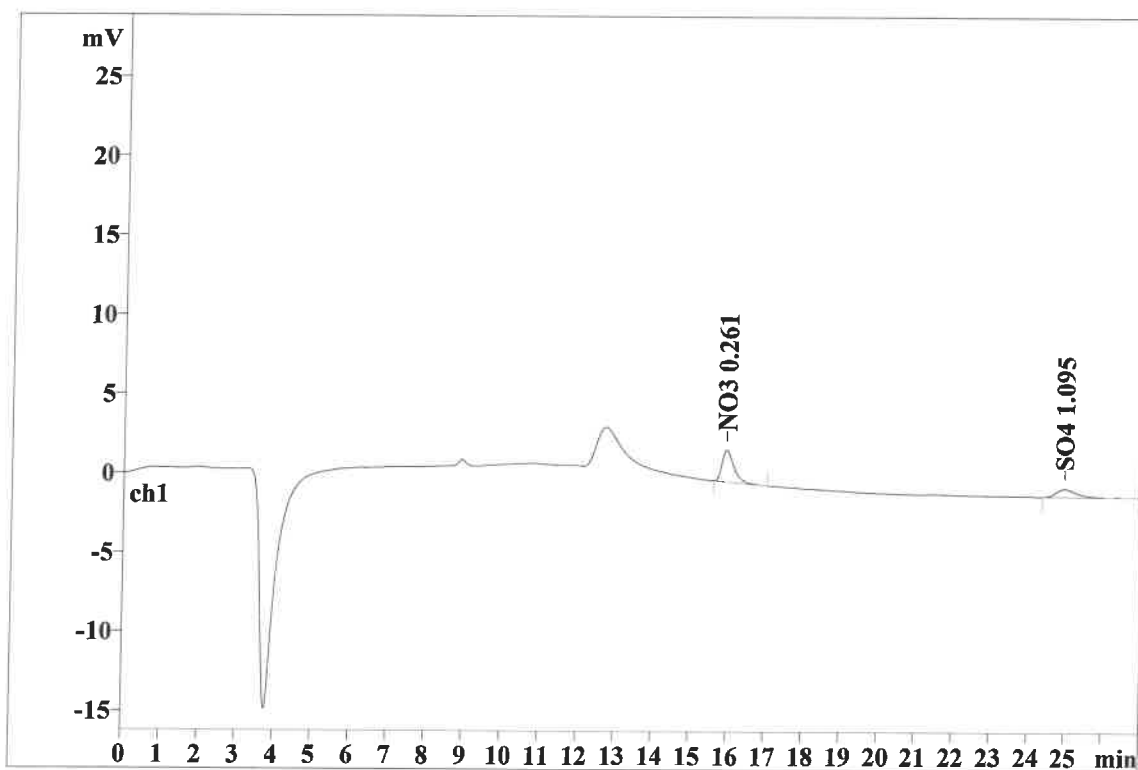

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 15.93            | 0.324          | 2.02         | 79.50       | 43.931         | 68.68     |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 24.93            | 0.567          | 0.52         | 20.34       | 20.035         | 31.32     |
| 7  | 27.00            | 0.127          | 2.53         | 99.84       | 63.966         | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 6/14/2023 1:41:49 PM  
Printed by: wet


Ident: O3176-01MS  
Analysis from: 6/13/2023 2:25:33 PM  
File: \_2023-06-13\_

Last save: 6/13/2023 2:52:33 PM

Method: AnionsIC2-052423.mtw  
Run operator: wet  
Analysis number: 34578

Last save: 5/25/2023 9:20:

SAMPLE:  
: IZ/MA  
Vial number: 21  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

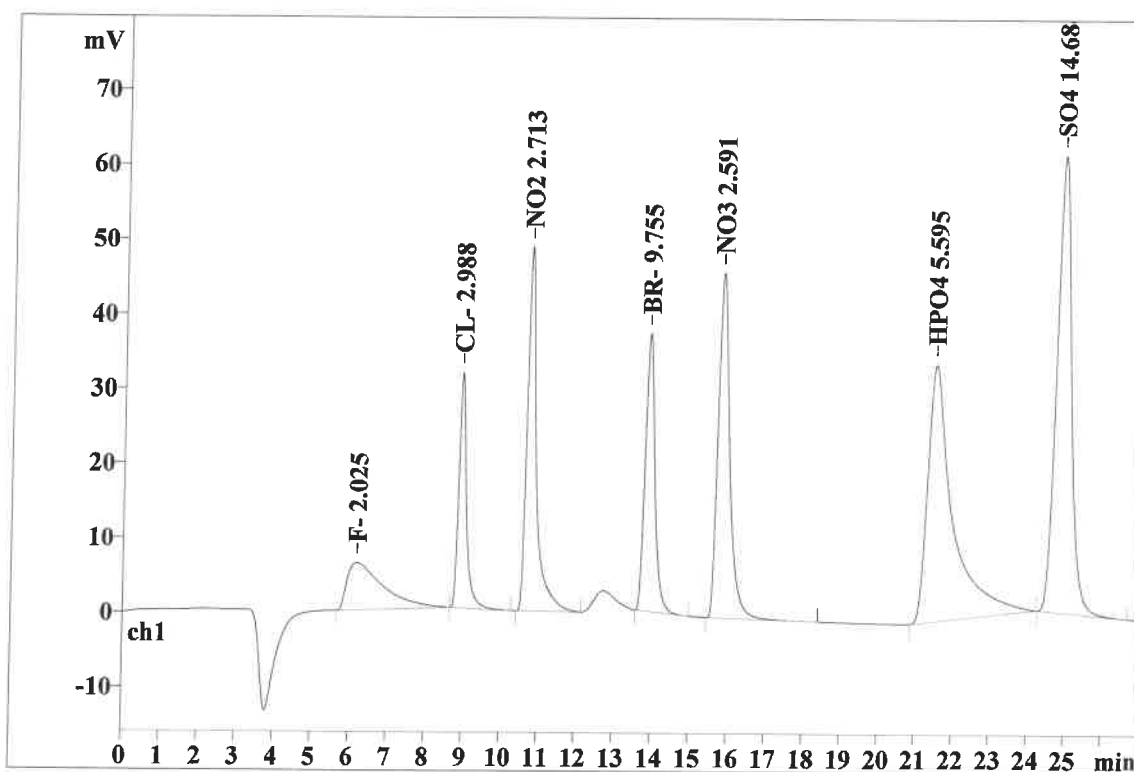

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 6.18             | 0.971          | 6.34         | 2.39        | 419.740        | 6.27      |
| 2  | 8.93             | 0.197          | 31.55        | 11.87       | 444.380        | 6.63      |
| 3  | 10.73            | 0.234          | 48.76        | 18.35       | 860.547        | 12.85     |
| 4  | 13.88            | 0.260          | 37.23        | 14.01       | 651.557        | 9.73      |
| 5  | 15.79            | 0.313          | 46.21        | 17.39       | 992.200        | 14.81     |
| 6  | 21.47            | 0.587          | 34.41        | 12.95       | 1625.665       | 24.27     |
| 7  | 24.86            | 0.417          | 61.20        | 23.03       | 1704.248       | 25.44     |
| 7  | 27.00            | 0.426          | 265.71       | 100.00      | 6698.337       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 6/14/2023 1:41:56 PM  
Printed by: wet


Ident: O3176-01MSD  
Analysis from: 6/13/2023 2:55:10 PM  
File: \_2023-06-13\_

Last save: 6/13/2023 3:22:10 PM

Method: AnionsIC2-052423.mtw  
Run operator: wet  
Analysis number: 34579

Last save: 5/25/2023 9:20:

SAMPLE:  
: IZ/MA  
Vial number: 22  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

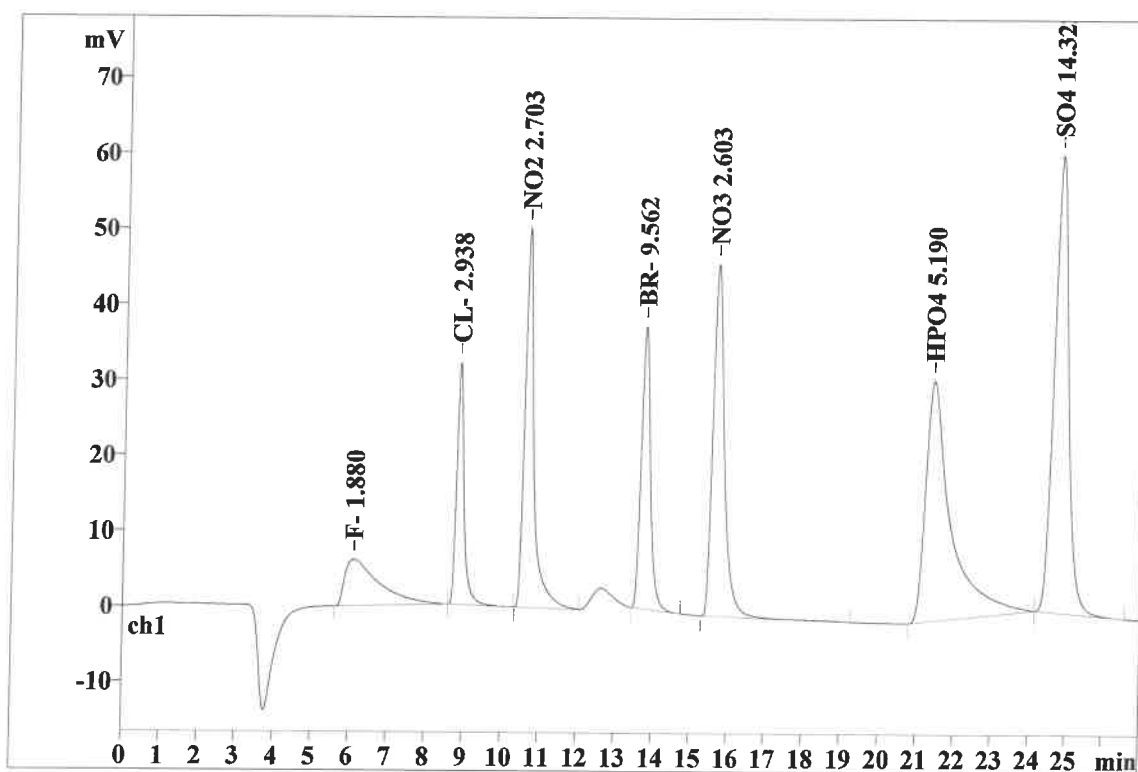

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 6.10             | 0.900          | 6.16         | 2.32        | 385.474        | 5.96      |
| 2  | 8.85             | 0.192          | 32.11        | 12.12       | 436.640        | 6.75      |
| 3  | 10.63            | 0.230          | 50.26        | 18.97       | 857.033        | 13.25     |
| 4  | 13.74            | 0.254          | 37.41        | 14.12       | 637.767        | 9.86      |
| 5  | 15.64            | 0.311          | 46.59        | 17.59       | 996.964        | 15.41     |
| 6  | 21.39            | 0.582          | 31.85        | 12.02       | 1494.626       | 23.11     |
| 7  | 24.76            | 0.410          | 60.55        | 22.86       | 1659.434       | 25.66     |
| 7  | 27.00            | 0.411          | 264.94       | 100.00      | 6467.938       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 6/14/2023 1:42:04 PM  
Printed by: wet


Ident: O3079-01X10  
Analysis from: 6/13/2023 3:24:49 PM  
File: \_2023-06-13\_

Last save: 6/13/2023 3:51:49 PM

Method: AnionsIC2-052423.mtw  
Run operator: wet  
Analysis number: 34580

Last save: 5/25/2023 9:20:

SAMPLE:  
: IZ/MA  
Vial number: 23  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

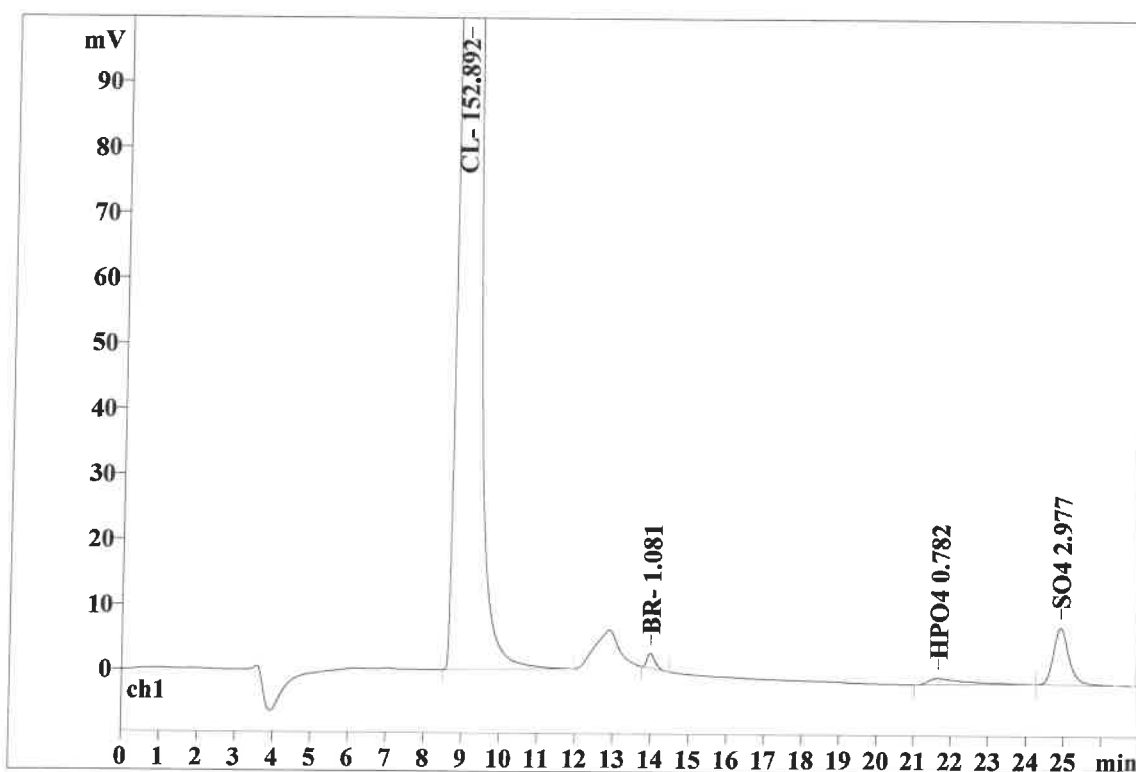

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 8.94             | 0.255          | 1343.13      | 99.12       | 23902.592      | 98.53     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 13.98            | 0.228          | 2.27         | 0.17        | 33.765         | 0.14      |
| 5  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 6  | 21.65            | 0.975          | 0.97         | 0.07        | 68.729         | 0.28      |
| 7  | 24.88            | 0.428          | 8.67         | 0.64        | 253.267        | 1.04      |
| 7  | 27.00            | 0.269          | 1355.05      | 100.00      | 24258.352      | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 6/14/2023 1:42:09 PM  
Printed by: wet


Ident: 03079-01DLX300  
Analysis from: 6/13/2023 3:54:26 PM  
File: \_2023-06-13\_

Last save: 6/13/2023 4:21:26 PM

Method: AnionsIC2-052423.mtw  
Run operator: wet  
Analysis number: 34581

Last save: 5/25/2023 9:20:

SAMPLE:  
: IZ/MA  
Vial number: 24  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

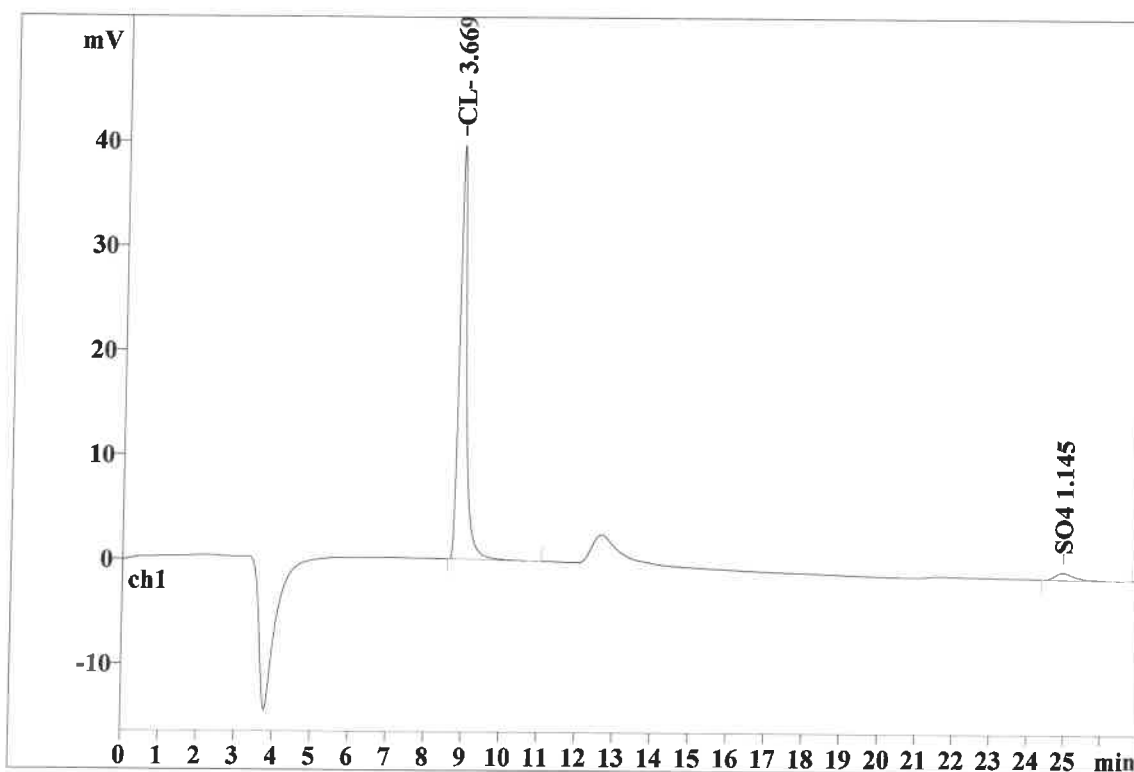

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 2  | 8.87             | 0.193          | 39.66        | 98.32       | 550.978        | 95.46     |
| 3  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 4  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 5  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 6  | 0.00             | 0.000          | 0.00         | 0.00        | 0.000          | 0.00      |
| 7  | 24.93            | 0.558          | 0.68         | 1.67        | 26.223         | 4.54      |
| 7  | 27.00            | 0.107          | 40.33        | 100.00      | 577.202        | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 6/14/2023 1:43:22 PM  
Printed by: wet


Ident: CCV  
Analysis from: 6/13/2023 4:24:14 PM  
File: \_2023-06-13\_

Last save: 6/13/2023 4:51:14 PM

Method: AnionsIC2-052423.mtw  
Run operator: wet  
Analysis number: 34582

Last save: 5/25/2023 9:20:

SAMPLE:  
: IZ/MA  
Vial number: 11  
Volume: 20.0 µL  
Dilution: 1.00  
Amount: 1.0000

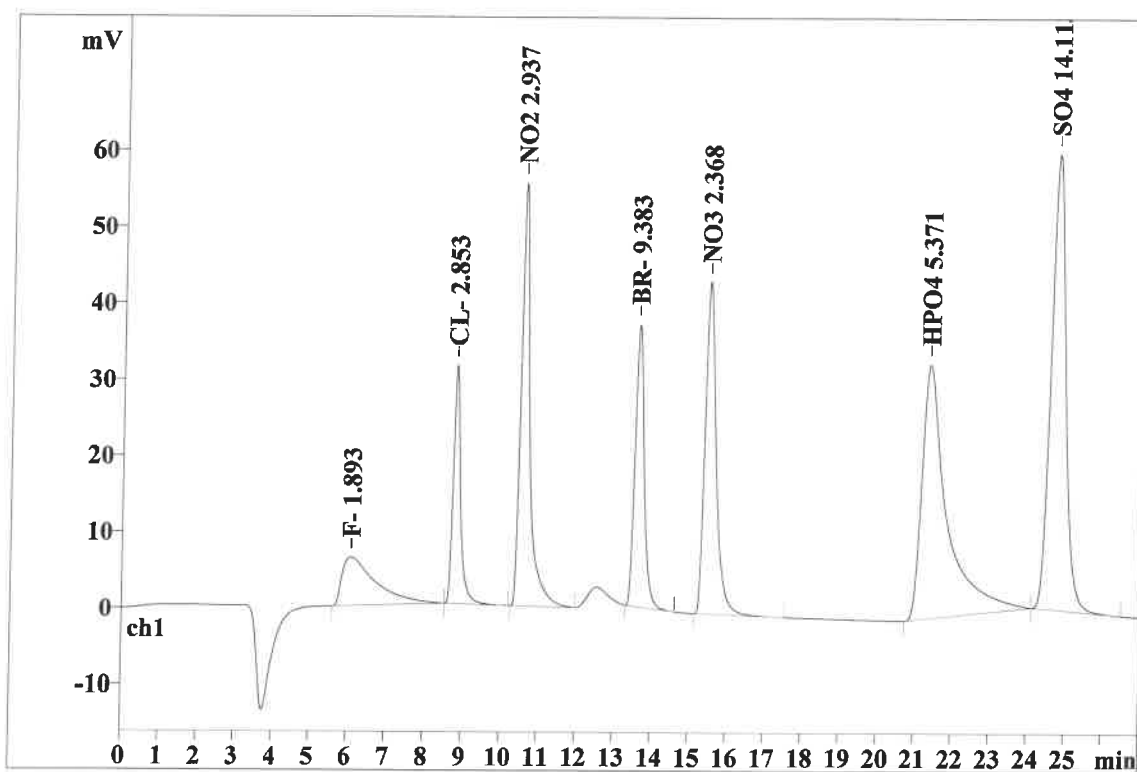

Quantitation method: Custom

| No | Retention<br>min | Width/2<br>min | Height<br>mV | Height<br>% | Area<br>mV*sec | Area<br>% |
|----|------------------|----------------|--------------|-------------|----------------|-----------|
| 1  | 6.08             | 0.879          | 6.36         | 2.39        | 388.531        | 6.01      |
| 2  | 8.80             | 0.190          | 31.28        | 11.74       | 423.229        | 6.55      |
| 3  | 10.56            | 0.228          | 55.41        | 20.79       | 937.148        | 14.50     |
| 4  | 13.61            | 0.253          | 36.96        | 13.87       | 625.043        | 9.67      |
| 5  | 15.47            | 0.303          | 43.55        | 16.34       | 901.547        | 13.95     |
| 6  | 21.35            | 0.579          | 33.25        | 12.48       | 1553.135       | 24.03     |
| 7  | 24.72            | 0.411          | 59.69        | 22.40       | 1633.520       | 25.28     |
| 7  | 27.00            | 0.406          | 266.50       | 100.00      | 6462.153       | 100.00    |

This report has been created by IC Net  
METROHM LTD

Report date: 6/14/2023 1:43:29 PM  
Printed by: wet


Ident: CCB  
Analysis from: 6/13/2023 5:00:04 PM  
File: \_2023-06-13\_

Last save: 6/13/2023 5:27:04 PM

Method: AnionsIC2-052423.mtw  
Run operator: wet  
Analysis number: 34583

Last save: 5/25/2023 9:20:

SAMPLE:  
: IZ/MA  
Vial number: 12  
Volume: 20.0  $\mu$ L  
Dilution: 1.00  
Amount: 1.0000

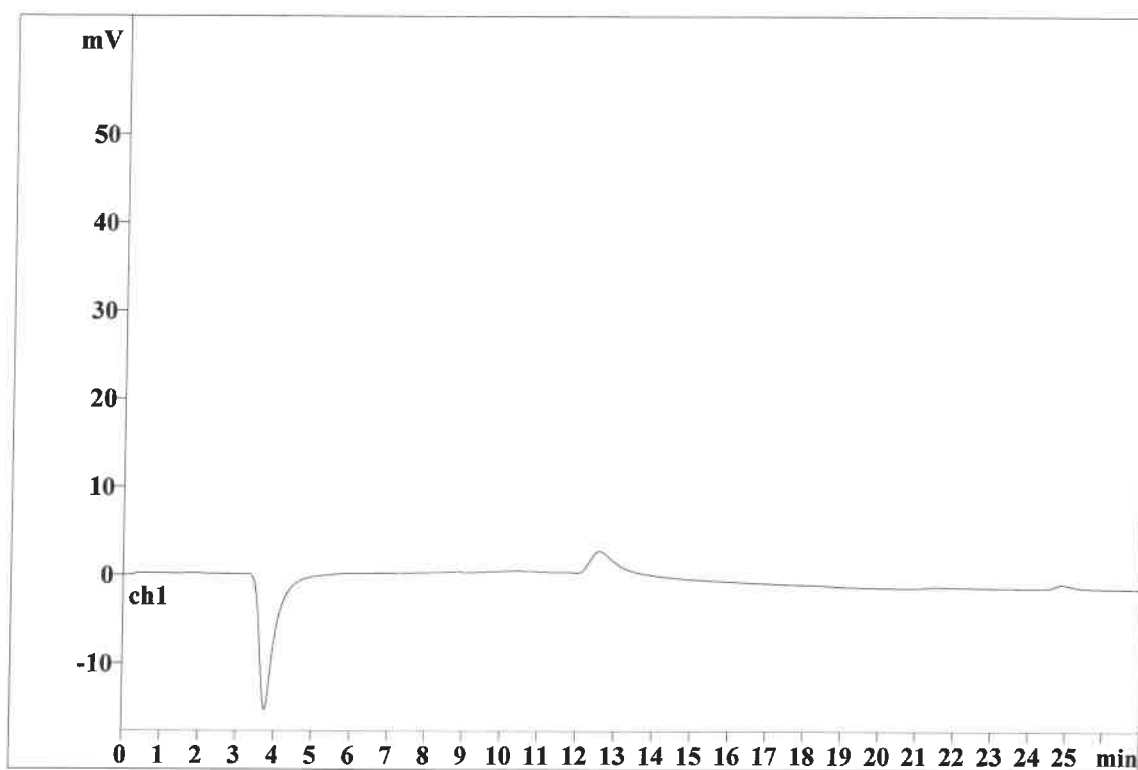

Quantitation method: Custom

No peaks

This report has been created by IC Net  
METROHM LTD