

LB126086


245.1

INSTRUMENT ID: EVZ

Linear

μ Abs.:

38847

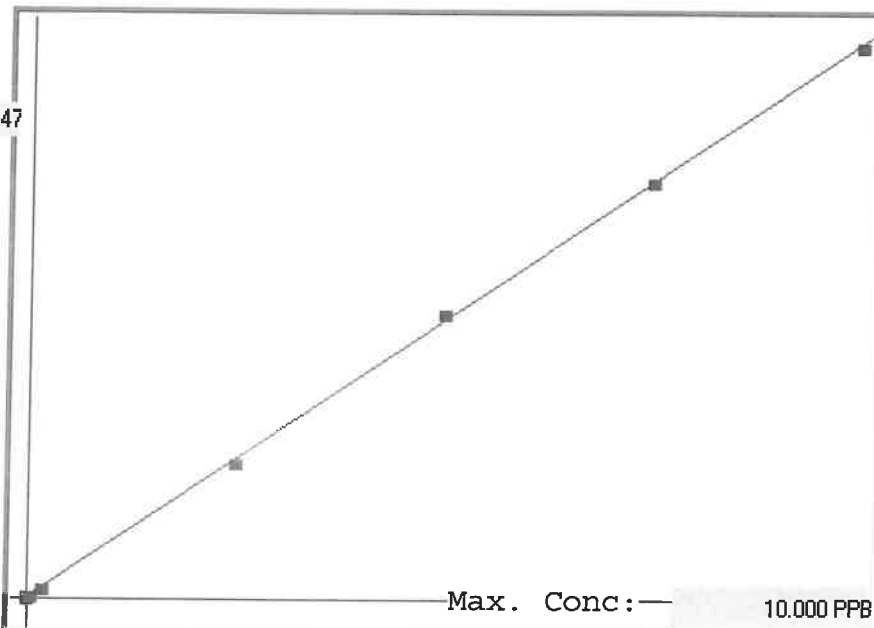

A= 0.0000e+000

B= 2.5623e-004

C= -1.8802e-002

Rho= 0.9998635

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.002	-0.002	67	0.000	67					-
0.05	0.050	0.036	-0.014	215	0.0 %	215	0				-28
0.2	0.200	0.177	-0.023	763	0.0 %	763					-12
2.5	2.500	2.459	-0.041	9672	0.0 %	9672					-2
5.0	5.000	5.140	0.140	20135	0.0 %	20135					3
7.5	7.500	7.504	0.004	29359	0.0 %	29359					0
10.0	10.000	9.935	-0.065	38847	0.0 %	38847					-1

L;B126086 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 21 Jun 2023 07:44:28

Sample ID	Extended ID	μ Abs	Conc	Stnd Conc	Method	Units	Date	Type	Type
0.0 - 1	50	67	-	0.0000	245.1	PPB	21 Jun 2023 08:00:45	S	Std
0.05 - 1	50.05	215	-	0.0500	245.1	PPB	21 Jun 2023 08:05:43	S	Std
0.2 - 1	50.2	763	-	0.2000	245.1	PPB	21 Jun 2023 08:08:01	S	Std
2.5 - 1	52.5	9672	-	2.5000	245.1	PPB	21 Jun 2023 08:10:18	S	Std
5.0 - 1	55	20135	-	5.0000	245.1	PPB	21 Jun 2023 08:12:35	S	Std
7.5 - 1	57.5	29359	-	7.5000	245.1	PPB	21 Jun 2023 08:14:51	S	Std
10.0 - 1	516	38847	-	10.0000	245.1	PPB	21 Jun 2023 08:17:09	S	Std
ICV31 - 1	ICV31	15022	3.8303	-245.1		PPB	21 Jun 2023 08:23:34	U	SMPL
ICB31 - 1	ICB31	-91	-0.0421	-245.1		PPB	21 Jun 2023 08:25:49	U	SMPL
CCV87 - 1	CCV87	19979	5.1004	-245.1		PPB	21 Jun 2023 08:28:07	U	SMPL
CCB87 - 1	CCB87	-151	-0.0575	-245.1		PPB	21 Jun 2023 08:30:22	U	SMPL
CRA - 1	CRA	232	0.0406	-245.1		PPB	21 Jun 2023 08:32:39	U	SMPL
HighStd - 1	HighStd	39058	9.9890	-245.1		PPB	21 Jun 2023 08:34:54	U	SMPL
ChkStd - 1	ChkStd	27179	6.9453	-245.1		PPB	21 Jun 2023 08:37:10	U	SMPL
PB153642BL - 1	PBW	116	0.0109	-245.1		PPB	21 Jun 2023 08:39:29	U	SMPL
PB153642BS - 1	LCSW	16344	4.1690	-245.1		PPB	21 Jun 2023 08:41:47	U	SMPL
O3251-01 - 1	MW-01	533	0.1178	-245.1		PPB	21 Jun 2023 08:48:42	U	SMPL
O3251-01DUP - 1	MW-01DUP	416	0.0878	-245.1		PPB	21 Jun 2023 08:50:58	U	SMPL
O3251-01MS - 1	MW-01MS	16140	4.1167	-245.1		PPB	21 Jun 2023 08:58:54	U	SMPL
O3251-01MSD - 1	MW-01MSD	16548	4.2213	-245.1		PPB	21 Jun 2023 09:01:11	U	SMPL
O3305-01 - 1	NEGATIVE-MH-BT-TRACK-89-90	144	0.0181	-245.1		PPB	21 Jun 2023 09:03:27	U	SMPL
CCV88 - 1	CCV88	19706	5.0305	-245.1		PPB	21 Jun 2023 09:05:42	U	SMPL
CCB88 - 1	CCB88	-24	-0.0250	-245.1		PPB	21 Jun 2023 09:07:59	U	SMPL
O3305-02 - 1	NEGATIVE-MH-BT-TRACK-89-90	491	0.1070	-245.1		PPB	21 Jun 2023 09:10:16	U	SMPL
O3251-01LX5 - 1		31	-0.0109	-245.1		PPB	21 Jun 2023 09:12:31	U	SMPL
O3251-01A - 1		16365	4.1744	-245.1		PPB	21 Jun 2023 09:14:48	U	SMPL
CCV89 - 1	CCV89	19497	4.9769	-245.1		PPB	21 Jun 2023 09:17:05	U	SMPL
CCB89 - 1	CCB89	-56	-0.0332	-245.1		PPB	21 Jun 2023 09:19:21	U	SMPL