

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

6/21/2023 12:03

Reviewed by : 12 Instrument ID : Konelab

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.006	0.0	0.091	
ICB1	0.004	0.0	0.010	
CCV1	1.010	0.0	0.091	
CCB1	0.013	0.0	0.011	
PB153631BL	-0.004	0.0	0.009	
PB153631BS	0.996	0.0	0.090	
O3251-01	0.004	0.0	0.010	
O3251-01DUP	0.002	0.0	0.010	
O3251-01MS	1.011	0.0	0.091	
O3251-01MSD	1.010	0.0	0.091	
CCV2	1.012	0.0	0.091	
CCB2	0.002	0.0	0.010	

N	12
Mean	0.505
SD	0.5245
CV%	103.77

Aquakem v. 7.2AQ1

Results from time period:

Wed Jun 21 10:04:51 2023

Wed Jun 21 11:52:09 2023

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0004	mg/l	6/21/2023 10:33:19	
0.05PPM	A	Phenolics-	P	0.0555	mg/l	6/21/2023 10:33:20	
0.1PPM	A	Phenolics-	P	0.0991	mg/l	6/21/2023 10:33:21	
0.25PPM	A	Phenolics-	P	0.2573	mg/l	6/21/2023 10:33:22	
0.50PPM	A	Phenolics-	P	0.5009	mg/l	6/21/2023 10:33:23	
1.0PPM	A	Phenolics-	P	0.976	mg/l	6/21/2023 10:33:24	
2.0PPM	A	Phenolics-	P	2.0107	mg/l	6/21/2023 10:33:25	
ICV1	S	Phenolics-	P	1.0055	mg/l	6/21/2023 11:41:56	
ICB1	S	Phenolics-	P	0.0044	mg/l	6/21/2023 11:41:59	
CCV1	S	Phenolics-	P	1.0097	mg/l	6/21/2023 11:42:00	
CCB1	S	Phenolics-	P	0.0131	mg/l	6/21/2023 11:42:02	
PB153631BL	S	Phenolics-	P	-0.0044	mg/l	6/21/2023 11:42:04	
PB153631BS	S	Phenolics-	P	0.9964	mg/l	6/21/2023 11:42:06	
O3251-01	S	Phenolics-	P	0.0035	mg/l	6/21/2023 11:51:59	
O3251-01DUP	S	Phenolics-	P	0.0018	mg/l	6/21/2023 11:52:01	
O3251-01MS	S	Phenolics-	P	1.0109	mg/l	6/21/2023 11:52:02	
O3251-01MSD	S	Phenolics-	P	1.0102	mg/l	6/21/2023 11:52:05	
CCV2	S	Phenolics-	P	1.0125	mg/l	6/21/2023 11:52:06	
CCB2	S	Phenolics-	P	0.0015	mg/l	6/21/2023 11:52:09	

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

6/21/2023 10:42

Reviewed by : 12

Instrument ID : Konelab

Test Phenolics-


Accepted 6/21/2023 10:42

Factor 12.37

Bias 0.009

Coeff. of det. 0.999754

Errors

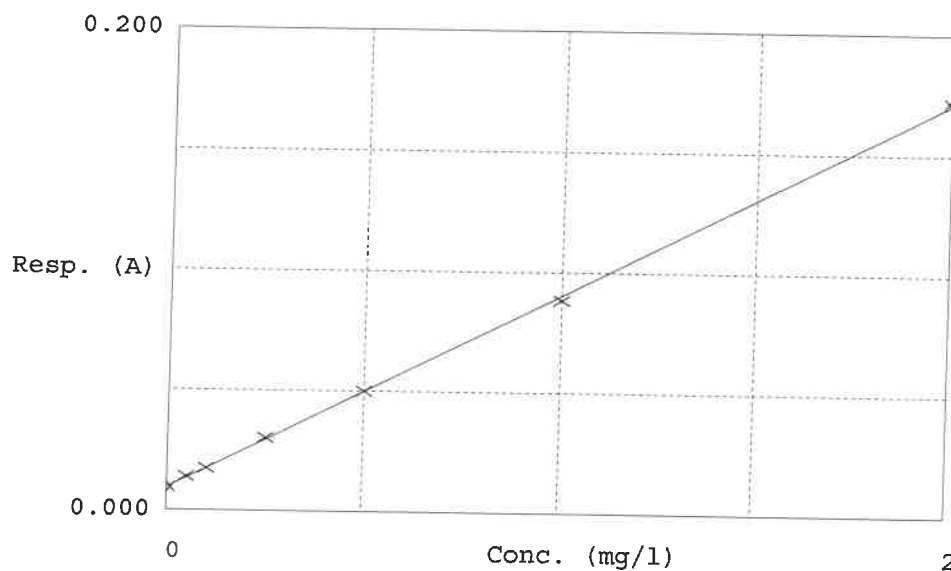

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.009	0.0004	0.0000	-
2	Phenol-2	0.014	0.0555	0.0500	11.0
3	Phenol-2	0.017	0.0991	0.1000	-0.9
4	Phenol-2	0.030	0.2573	0.2500	2.9
5	Phenol-2	0.050	0.5009	0.5000	0.2
6	Phenol-2	0.088	0.9760	1.0000	-2.4
7	Phenol-2	0.172	2.0107	2.0000	0.5

12
6/21/23