

LB126150


7470A

INSTRUMENT ID: EVL

Linear

 μ Abs.:

50086

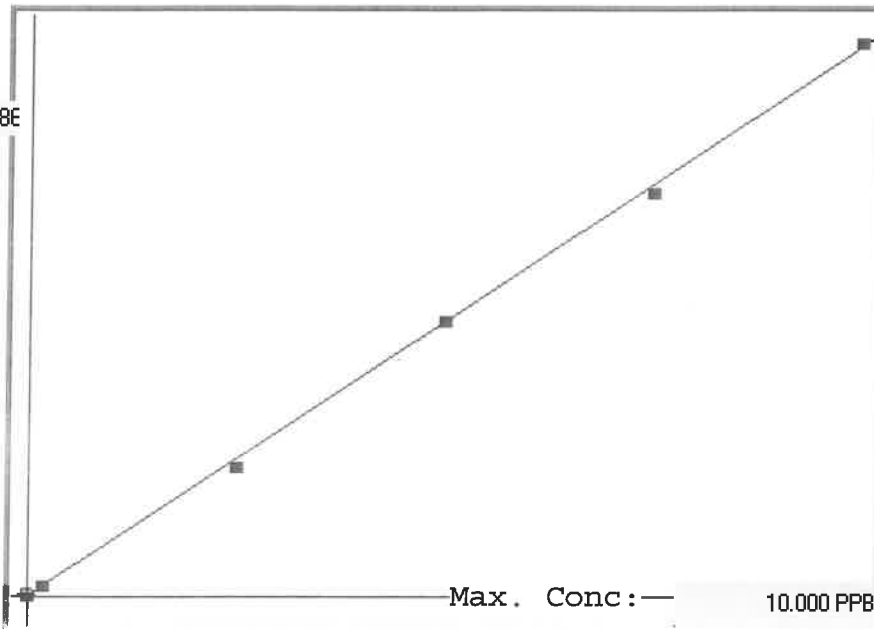

A= 0.0000e+000

B= 2.0150e-004

C= -3.3312e-003

Rho= 0.9997634

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	9/10
0.0	0.000	0.055	0.055	290	0.000	290	0				-
0.2	0.200	0.229	0.029	1151	0.0 %	1151					15
2.5	2.500	2.404	-0.096	11948	0.0 %	11948					-4
5.0	5.000	5.047	0.047	25065	0.0 %	25065					1
7.5	7.500	7.376	-0.124	36620	0.0 %	36620					-2
10.0	10.000	10.089	0.089	50086	0.0 %	50086					1

LB126150 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 23 Jun 2023 13:26:55

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	290	-	0.000	7470A	PPB	23 Jun 2023 13:27:04	S	Std
0.2 - 1	50.2	1151	-	0.200	7470A	PPB	23 Jun 2023 13:29:21	S	Std
2.5 - 1	52.5	11948	-	2.500	7470A	PPB	23 Jun 2023 13:31:38	S	Std
5.0 - 1	55	25065	-	5.000	7470A	PPB	23 Jun 2023 13:33:55	S	Std
7.5 - 1	57.5	36620	-	7.500	7470A	PPB	23 Jun 2023 13:36:14	S	Std
10.0 - 1	511	50086	-	10.000	7470A	PPB	23 Jun 2023 13:46:42	S	Std
ICV38 - 1	ICV38	18586	3.7418	-	7470A	PPB	23 Jun 2023 13:52:01	U	SMPL
ICB38 - 1	ICB38	112	0.0192	-	7470A	PPB	23 Jun 2023 13:54:16	U	SMPL
CCV17 - 1	CCV17	23825	4.7975	-	7470A	PPB	23 Jun 2023 14:11:07	U	SMPL
CCB17 - 1	CCB17	142	0.0253	-	7470A	PPB	23 Jun 2023 14:13:22	U	SMPL
CRA - 1	CRA	1004	0.1990	-	7470A	PPB	23 Jun 2023 14:15:38	U	SMPL
HighStd - 1	HighStd	47628	9.5938	-	7470A	PPB	23 Jun 2023 14:17:53	U	SMPL
ChkStd - 1	ChkStd	33493	6.7456	-	7470A	PPB	23 Jun 2023 14:22:46	U	SMPL
PB153709BL - 1	PBW	82	0.0132	-	7470A	PPB	23 Jun 2023 14:25:02	U	SMPL
PB153709BS - 1	LCSW	17125	3.4474	-	7470A	PPB	23 Jun 2023 14:32:37	U	SMPL
O3355-02 - 1	SB-01-COMP	159	0.0287	-	7470A	PPB	23 Jun 2023 14:34:52	U	SMPL
O3355-04 - 1	SB-02-COMP	271	0.0513	-	7470A	PPB	23 Jun 2023 14:37:10	U	SMPL
O3355-06 - 1	SB-03-COMP	306	0.0583	-	7470A	PPB	23 Jun 2023 14:39:27	U	SMPL
O3355-08 - 1	SB-04-COMP	415	0.0803	-	7470A	PPB	23 Jun 2023 14:41:44	U	SMPL
O3355-10 - 1	SB-05-COMP	331	0.0634	-	7470A	PPB	23 Jun 2023 14:43:59	U	SMPL
CCV18 - 1	CCV18	23525	4.7370	-	7470A	PPB	23 Jun 2023 14:46:15	U	SMPL
CCB18 - 1	CCB18	138	0.0245	-	7470A	PPB	23 Jun 2023 14:48:30	U	SMPL
O3355-12 - 1	SB-06-COMP	295	0.0561	-	7470A	PPB	23 Jun 2023 14:50:46	U	SMPL
O3355-14 - 1	SB-07-COMP	236	0.0442	-	7470A	PPB	23 Jun 2023 14:53:01	U	SMPL
O3357-02 - 1	WC-SCAN-01	272	0.0515	-	7470A	PPB	23 Jun 2023 14:55:17	U	SMPL
O3357-07 - 1	WC-SCAN-02	319	0.0609	-	7470A	PPB	23 Jun 2023 14:57:32	U	SMPL
O3357-12 - 1	WC-SCAN-03	302	0.0575	-	7470A	PPB	23 Jun 2023 14:59:48	U	SMPL
O3357-17 - 1	WC-SCAN-04	422	0.0817	-	7470A	PPB	23 Jun 2023 15:02:04	U	SMPL
O3360-04 - 1	CE-91-062023	297	0.0565	-	7470A	PPB	23 Jun 2023 15:04:20	U	SMPL
O3360-08 - 1	CE-88N-062023	279	0.0529	-	7470A	PPB	23 Jun 2023 15:06:37	U	SMPL
O3361-02 - 1	COMPOSIT-SB-28-29	314	0.0599	-	7470A	PPB	23 Jun 2023 15:08:53	U	SMPL
O3361-08 - 1	COMPOSIT-SB-31-36	301	0.0573	-	7470A	PPB	23 Jun 2023 15:11:09	U	SMPL
CCV19 - 1	CCV19	22767	4.5843	-	7470A	PPB	23 Jun 2023 15:13:25	U	SMPL
CCB19 - 1	CCB19	174	0.0317	-	7470A	PPB	23 Jun 2023 15:15:40	U	SMPL
O3361-14 - 1	COMPOSIT-SB-21-23	271	0.0513	-	7470A	PPB	23 Jun 2023 15:17:57	U	SMPL
O3361-20 - 1	COMPOSIT-SB-7-22	310	0.0591	-	7470A	PPB	23 Jun 2023 15:20:12	U	SMPL
O3366-02 - 1	WC37	299	0.0569	-	7470A	PPB	23 Jun 2023 15:22:27	U	SMPL
O3366-04 - 1	WC38	327	0.0626	-	7470A	PPB	23 Jun 2023 15:24:43	U	SMPL
O3366-04DUP - 1	WC38DUP	394	0.0761	-	7470A	PPB	23 Jun 2023 15:26:59	U	SMPL
O3366-04MS - 1	WC38MS	14059	2.8296	-	7470A	PPB	23 Jun 2023 15:29:15	U	SMPL
O3366-04MSD - 1	WC38MSD	13362	2.6891	-	7470A	PPB	23 Jun 2023 15:31:31	U	SMPL
PB153717BL - 1	PBW	234	0.0438	-	7470A	PPB	23 Jun 2023 15:33:48	U	SMPL
PB153717BS - 1	LCSW	21794	4.3882	-	7470A	PPB	23 Jun 2023 15:44:05	U	SMPL
O3366-05 - 1	FB02	193	0.0356	-	7470A	PPB	23 Jun 2023 15:46:24	U	SMPL
CCV20 - 1	CCV20	22933	4.6177	-	7470A	PPB	23 Jun 2023 15:48:41	U	SMPL
CCB20 - 1	CCB20	145	0.0259	-	7470A	PPB	23 Jun 2023 15:50:56	U	SMPL
O3375-09 - 1	FB-5-062123	325	0.0622	-	7470A	PPB	23 Jun 2023 15:53:13	U	SMPL
O3376-01 - 1	FB-GW-062123	370	0.0712	-	7470A	PPB	23 Jun 2023 15:55:29	U	SMPL
O3376-02 - 1	FB-GW-062123	138	0.0245	-	7470A	PPB	23 Jun 2023 15:57:44	U	SMPL
O3376-03 - 1	TW-1	1633	0.3257	-	7470A	PPB	23 Jun 2023 16:06:11	U	SMPL
O3376-03DUP - 1	TW-1DUP	1345	0.2677	-	7470A	PPB	23 Jun 2023 16:08:27	U	SMPL
O3376-04 - 1	TW-1	212	0.0394	-	7470A	PPB	23 Jun 2023 16:16:23	U	SMPL
O3376-05 - 1	O3376-03MS	17653	3.5538	-	7470A	PPB	23 Jun 2023 16:18:39	U	SMPL
O3376-06 - 1	O3376-03MSD	18069	3.6376	-	7470A	PPB	23 Jun 2023 16:20:55	U	SMPL
O3376-07 - 1	O3376-04MS	16502	3.3219	-	7470A	PPB	23 Jun 2023 16:23:13	U	SMPL
O3376-08 - 1	O3376-04MSD	16809	3.3837	-	7470A	PPB	23 Jun 2023 16:25:30	U	SMPL
CCV21 - 1	CCV21	26316	5.2994	-	7470A	PPB	23 Jun 2023 16:27:46	U	SMPL
CCB21 - 1	CCB21	242	0.0454	-	7470A	PPB	23 Jun 2023 16:30:01	U	SMPL
O3376-09 - 1	TW-2	631	0.1238	-	7470A	PPB	23 Jun 2023 16:32:18	U	SMPL
O3376-10 - 1	TW-2	310	0.0591	-	7470A	PPB	23 Jun 2023 16:34:34	U	SMPL
O3376-12 - 1	DUP-01	534	0.1043	-	7470A	PPB	23 Jun 2023 16:36:49	U	SMPL
O3376-13 - 1	DUP-01	317	0.0605	-	7470A	PPB	23 Jun 2023 16:39:04	U	SMPL
O3390-01 - 1	TW-3	725	0.1428	-	7470A	PPB	23 Jun 2023 16:41:20	U	SMPL
PB153702TB - 1	PB153702TB	304	0.0579	-	7470A	PPB	23 Jun 2023 16:43:35	U	SMPL
O3366-04LX5 - 1		85	0.0138	-	7470A	PPB	23 Jun 2023 16:45:52	U	SMPL
O3366-04A - 1		18002	3.6241	-	7470A	PPB	23 Jun 2023 16:50:37	U	SMPL
O3376-03LX5 - 1		183	0.0335	-	7470A	PPB	23 Jun 2023 16:52:55	U	SMPL
O3376-03A - 1		19585	3.9431	-	7470A	PPB	23 Jun 2023 16:55:12	U	SMPL
CCV22 - 1	CCV22	24750	4.9838	-	7470A	PPB	23 Jun 2023 16:57:28	U	SMPL
CCB22 - 1	CCB22	220	0.0410	-	7470A	PPB	23 Jun 2023 16:59:46	U	SMPL