

LB128181


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

45161

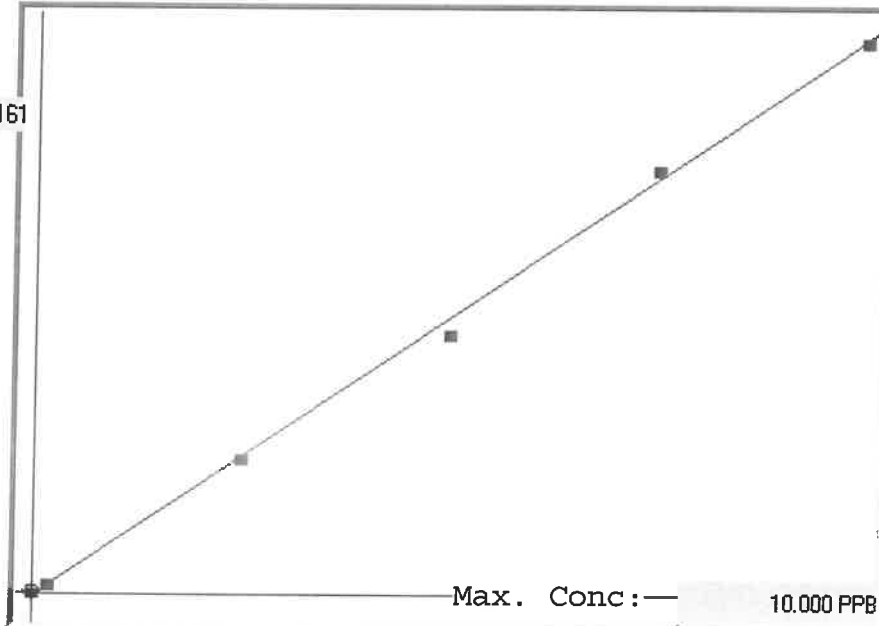

A= 0.0000e+000

B= 2.2020e-004

C= 3.0638e-002

Rho= 0.9993123

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.078	-0.078	213	0.000	213	0				
0.2	0.200	0.217	0.017	847	0.0 %	847					
2.5	2.500	2.499	-0.001	11211	0.0 %	11211					
5.0	5.000	4.739	-0.261	21381	0.0 %	21381					
7.5	7.500	7.693	0.193	34796	0.0 %	34796					
10.0	10.000	9.975	-0.025	45161	0.0 %	45161					

164081

LB126181 INSTRUMENT ID :CV1

Method: 7470A

Operator: Admin

Date of Analysis: 26 Jun 2023 10:07:38

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	213	-	0.0000	7470A	PPB	26 Jun 2023 10:14:21	S	Std
0.2 - 1	50.2	847	-	0.2000	7470A	PPB	26 Jun 2023 10:16:38	S	Std
2.5 - 1	52.5	11211	-	2.5000	7470A	PPB	26 Jun 2023 10:18:55	S	Std
5.0 - 1	55	21381	-	5.0000	7470A	PPB	26 Jun 2023 10:21:12	S	Std
7.5 - 1	57.5	34796	-	7.5000	7470A	PPB	26 Jun 2023 10:23:28	S	Std
10.0 - 1	510	45161	-	10.0000	7470A	PPB	26 Jun 2023 10:25:45	S	Std
ICV41 - 1	ICV41	18161	4.0296	-	7470A	PPB	26 Jun 2023 10:29:43	U	SMPL
ICB41 - 1	ICB41	22	0.0355	-	7470A	PPB	26 Jun 2023 10:31:58	U	SMPL
CCV30 - 1	CCV30	21347	4.7311	-	7470A	PPB	26 Jun 2023 10:34:14	U	SMPL
CCB30 - 1	CCB30	1	0.0309	-	7470A	PPB	26 Jun 2023 10:36:29	U	SMPL
CRA - 1	CRA	728	0.1909	-	7470A	PPB	26 Jun 2023 10:38:46	U	SMPL
HighStd - 1	HighStd	43605	9.6323	-	7470A	PPB	26 Jun 2023 10:41:00	U	SMPL
ChkStd - 1	ChkStd	30159	6.6715	-	7470A	PPB	26 Jun 2023 10:43:15	U	SMPL
PB153733BL - 1	PBW	-145	-0.0013	-	7470A	PPB	26 Jun 2023 10:45:33	U	SMPL
PB153733BS - 1	LCSW	16008	3.5555	-	7470A	PPB	26 Jun 2023 10:50:28	U	SMPL
O3362-02 - 1	COMPOSIT-SB-32-37	-59	0.0176	-	7470A	PPB	26 Jun 2023 10:52:45	U	SMPL
O3362-02DUP - 1	COMPOSIT-SB-32-37DUP	53	0.0423	-	7470A	PPB	26 Jun 2023 10:55:02	U	SMPL
O3362-02MS - 1	COMPOSIT-SB-32-37MS	14033	3.1206	-	7470A	PPB	26 Jun 2023 10:57:19	U	SMPL
O3362-02MSD - 1	COMPOSIT-SB-32-37MSD	14945	3.3215	-	7470A	PPB	26 Jun 2023 10:59:36	U	SMPL
O3362-09 - 1	COMPOSIT-SB-12-13	-24	0.0254	-	7470A	PPB	26 Jun 2023 11:01:53	U	SMPL
CCV31 - 1	CCV31	22996	5.0942	-	7470A	PPB	26 Jun 2023 11:06:48	U	SMPL
CCB31 - 1	CCB31	6	0.0320	-	7470A	PPB	26 Jun 2023 11:09:03	U	SMPL
O3362-15 - 1	COMPOSIT-SB-19-20	74	0.0469	-	7470A	PPB	26 Jun 2023 11:11:20	U	SMPL
O3362-21 - 1	COMPOSIT-SB-25	68	0.0456	-	7470A	PPB	26 Jun 2023 11:13:35	U	SMPL
O3363-04 - 1	CONCRETE-BLOCKING	79	0.0480	-	7470A	PPB	26 Jun 2023 11:15:51	U	SMPL
O3365-04 - 1	TP2	99	0.0524	-	7470A	PPB	26 Jun 2023 11:18:06	U	SMPL
O3365-14 - 1	TP4	181	0.0705	-	7470A	PPB	26 Jun 2023 11:20:22	U	SMPL
O3365-23 - 1	TP1	129	0.0590	-	7470A	PPB	26 Jun 2023 11:22:38	U	SMPL
O3365-34 - 1	TP3	131	0.0595	-	7470A	PPB	26 Jun 2023 11:24:54	U	SMPL
O3369-04 - 1	ORA-1650	184	0.0712	-	7470A	PPB	26 Jun 2023 11:27:12	U	SMPL
O3381-01 - 1	COMP1-0622	31	0.0375	-	7470A	PPB	26 Jun 2023 11:29:29	U	SMPL
O3381-02 - 1	COMP2-0622	102	0.0531	-	7470A	PPB	26 Jun 2023 11:31:44	U	SMPL
CCV32 - 1	CCV32	22606	5.0084	-	7470A	PPB	26 Jun 2023 11:36:34	U	SMPL
CCB32 - 1	CCB32	-28	0.0245	-	7470A	PPB	26 Jun 2023 11:38:48	U	SMPL
O3381-03 - 1	8352	106	0.0540	-	7470A	PPB	26 Jun 2023 11:41:06	U	SMPL
O3389-01 - 1	WC-DRUM	106	0.0540	-	7470A	PPB	26 Jun 2023 11:43:21	U	SMPL
O3394-02 - 1	ORA-1651	147	0.0630	-	7470A	PPB	26 Jun 2023 11:45:36	U	SMPL
PB153702TB - 1	PB153702TB	44	0.0403	-	7470A	PPB	26 Jun 2023 11:47:52	U	SMPL
O3362-02LX5 - 1		21	0.0353	-	7470A	PPB	26 Jun 2023 11:50:08	U	SMPL
O3362-02A - 1		14808	3.2913	-	7470A	PPB	26 Jun 2023 11:52:25	U	SMPL
CCV33 - 1	CCV33	21893	4.8514	-	7470A	PPB	26 Jun 2023 11:54:41	U	SMPL
CCB33 - 1	CCB33	0	0.0306	-	7470A	PPB	26 Jun 2023 11:56:59	U	SMPL