


LB126225

7470A

INSTRUMENT ID: CXL

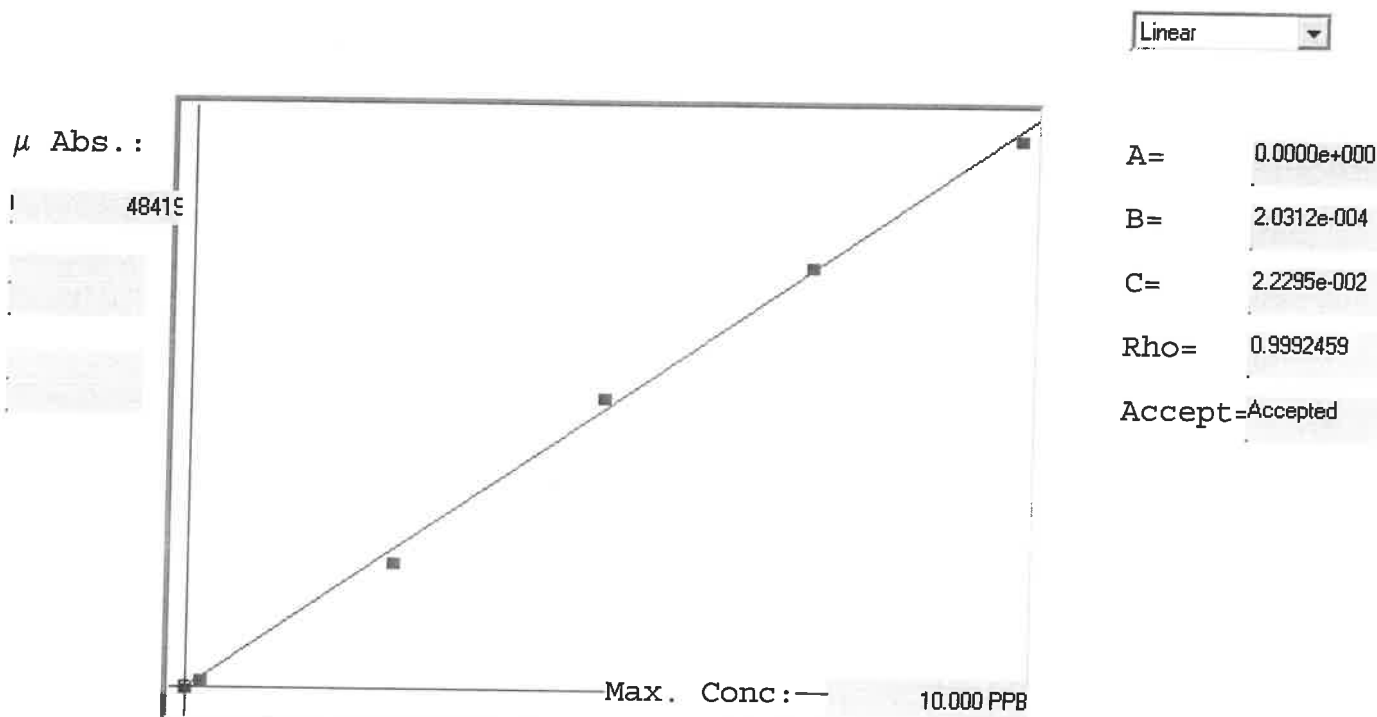

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.038	0.038	77	0.000	77	0				1
0.2	0.200	0.189	-0.011	820	0.0 %	820					6
2.5	2.500	2.298	-0.202	11204	0.0 %	11204					8
5.0	5.000	5.229	0.229	25634	0.0 %	25634					5
7.5	7.500	7.589	0.089	37253	0.0 %	37253					1
10.0	10.000	9.857	-0.143	48419	0.0 %	48419					1

LB126225 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 28 Jun 2023 12:53:53

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	56	77	-	0.0000	7470A	PPB	28 Jun 2023 13:30:39	S	Std
0.2 - 1	58.2	820	-	0.2000	7470A	PPB	28 Jun 2023 13:32:56	S	Std
2.5 - 1	52.5	11204	-	2.5000	7470A	PPB	28 Jun 2023 13:35:13	S	Std
5.0 - 1	57.5	25634	-	5.0000	7470A	PPB	28 Jun 2023 13:37:29	S	Std
7.5 - 1	57.5	37253	-	7.5000	7470A	PPB	28 Jun 2023 13:39:45	S	Std
10.0 - 1	51.8	48419	-	10.0000	7470A	PPB	28 Jun 2023 13:44:40	S	Std
ICV45 - 1	ICV45	20811	4.2494	-	7470A	PPB	28 Jun 2023 13:53:14	U	SMPL
ICB45 - 1	ICB45	-119	-0.0019	-	7470A	PPB	28 Jun 2023 13:55:29	U	SMPL
CCV43 - 1	CCV43	22641	4.6211	-	7470A	PPB	28 Jun 2023 13:57:45	U	SMPL
CCB43 - 1	CCB43	-150	-0.0082	-	7470A	PPB	28 Jun 2023 14:00:00	U	SMPL
CRA - 1	CRA	800	0.1848	-	7470A	PPB	28 Jun 2023 14:04:54	U	SMPL
HighStd - 1	HighStd	48509	9.8754	-	7470A	PPB	28 Jun 2023 14:07:08	U	SMPL
ChkStd - 1	ChkStd	33908	6.9096	-	7470A	PPB	28 Jun 2023 14:09:23	U	SMPL
PB153852BL - 1	PBW	-62	0.0097	-	7470A	PPB	28 Jun 2023 14:11:42	U	SMPL
PB153852BS - 1	LCSW	18488	3.7775	-	7470A	PPB	28 Jun 2023 14:13:59	U	SMPL
O3415-09 - 1	ESII-TP1	-8	0.0207	-	7470A	PPB	28 Jun 2023 14:16:15	U	SMPL
O3415-09DUP - 1	ESII-TP1DUP	106	0.0438	-	7470A	PPB	28 Jun 2023 14:18:33	U	SMPL
O3415-09MS - 1	ESII-TP1MS	16396	3.3526	-	7470A	PPB	28 Jun 2023 14:20:50	U	SMPL
O3415-09MSD - 1	ESII-TP1MSD	17259	3.5279	-	7470A	PPB	28 Jun 2023 14:23:06	U	SMPL
O3428-02 - 1	PNNL-APM-0621-1	291	0.0814	-	7470A	PPB	28 Jun 2023 14:25:22	U	SMPL
CCV44 - 1	CCV44	22484	4.5892	-	7470A	PPB	28 Jun 2023 14:27:39	U	SMPL
CCB44 - 1	CCB44	-73	0.0075	-	7470A	PPB	28 Jun 2023 14:29:54	U	SMPL
O3428-04 - 1	PNNL-APM-0621-2	343	0.0920	-	7470A	PPB	28 Jun 2023 14:32:10	U	SMPL
O3429-02 - 1	SB-COMP-0627	290	0.0812	-	7470A	PPB	28 Jun 2023 14:34:26	U	SMPL
O3441-02 - 1	KL-FM628-F06064	257	0.0745	-	7470A	PPB	28 Jun 2023 14:36:41	U	SMPL
PB153853BL - 1	PBW	194	0.0617	-	7470A	PPB	28 Jun 2023 14:38:56	U	SMPL
PB153853BS - 1	LCSW	19932	4.0709	-	7470A	PPB	28 Jun 2023 14:43:56	U	SMPL
O3381-04 - 1	8327	-93	0.0034	-	7470A	PPB	28 Jun 2023 14:46:12	U	SMPL
O3381-04DUP - 1	8327DUP	68	0.0361	-	7470A	PPB	28 Jun 2023 14:48:29	U	SMPL
O3381-04MS - 1	8327MS	21702	4.4304	-	7470A	PPB	28 Jun 2023 14:53:08	U	SMPL
O3381-04MSD - 1	8327MSD	18698	3.8202	-	7470A	PPB	28 Jun 2023 14:58:22	U	SMPL
PB153866BL - 1	PBW	-131	-0.0043	-	7470A	PPB	28 Jun 2023 15:00:37	U	SMPL
CCV45 - 1	CCV45	25662	5.2347	-	7470A	PPB	28 Jun 2023 15:02:54	U	SMPL
CCB45 - 1	CCB45	-105	0.0010	-	7470A	PPB	28 Jun 2023 15:05:09	U	SMPL
PB153866BS - 1	LCSW	17440	3.5647	-	7470A	PPB	28 Jun 2023 15:07:27	U	SMPL
O3430-01 - 1	1003	-38	0.0146	-	7470A	PPB	28 Jun 2023 15:09:42	U	SMPL
O3430-01DUP - 1	1003DUP	90	0.0406	-	7470A	PPB	28 Jun 2023 15:11:58	U	SMPL
O3430-01MS - 1	1003MS	17322	3.5407	-	7470A	PPB	28 Jun 2023 15:14:13	U	SMPL
O3430-01MSD - 1	1003MSD	16798	3.4343	-	7470A	PPB	28 Jun 2023 15:16:29	U	SMPL
O3430-03 - 1	1004	-79	0.0062	-	7470A	PPB	28 Jun 2023 15:18:46	U	SMPL
PB153852TB - 1		91	0.0408	-	7470A	PPB	28 Jun 2023 15:21:03	U	SMPL
PB153796TB - 1		33	0.0290	-	7470A	PPB	28 Jun 2023 15:23:20	U	SMPL
CCV46 - 1	CCV46	24755	5.0505	-	7470A	PPB	28 Jun 2023 15:25:37	U	SMPL
CCB46 - 1	CCB46	-130	-0.0041	-	7470A	PPB	28 Jun 2023 15:27:52	U	SMPL
O3415-09LX5 - 1		26	0.0276	-	7470A	PPB	28 Jun 2023 15:30:09	U	SMPL
O3415-09A - 1		17405	3.5576	-	7470A	PPB	28 Jun 2023 15:32:26	U	SMPL
O3381-04LX5 - 1		-104	0.0012	-	7470A	PPB	28 Jun 2023 15:34:41	U	SMPL
O3381-04A - 1		17632	3.6037	-	7470A	PPB	28 Jun 2023 15:36:57	U	SMPL
O3430-01LX5 - 1		27	0.0278	-	7470A	PPB	28 Jun 2023 15:43:01	U	SMPL
O3430-01A - 1		18205	3.7201	-	7470A	PPB	28 Jun 2023 15:45:15	U	SMPL
CCV47 - 1	CCV47	26129	5.3296	-	7470A	PPB	28 Jun 2023 15:47:31	U	SMPL
CCB47 - 1	CCB47	-135	-0.0051	-	7470A	PPB	28 Jun 2023 15:49:47	U	SMPL