


LB126529

7470A

INSTRUMENT ID: CV1

Linear

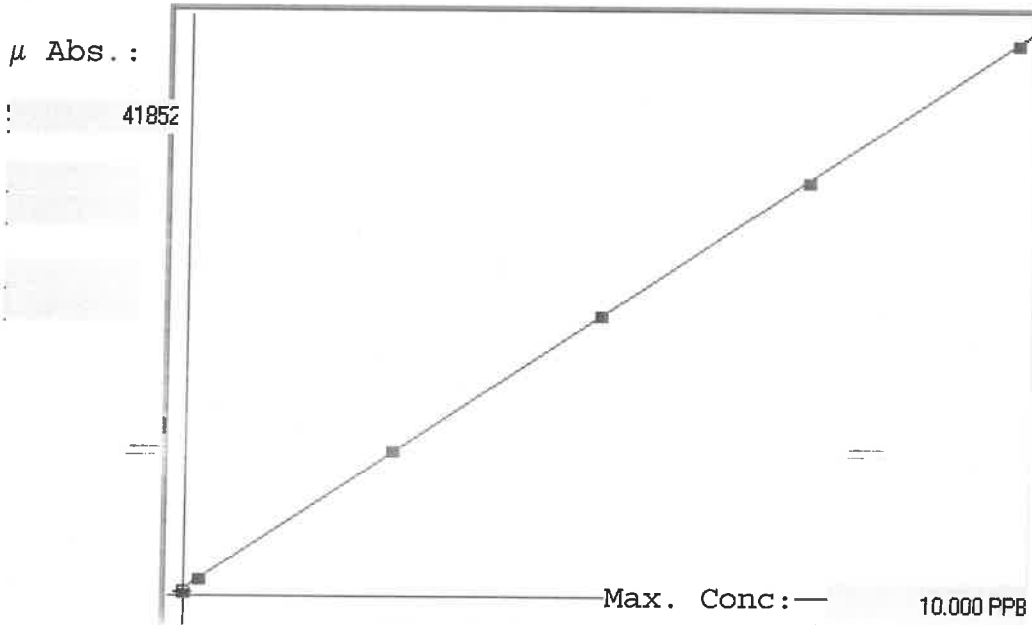

A= 0.0000e+000

B= 2.4156e-004

C= -1.2087e-001

Rho= 0.9999611

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.045	-0.045	314	0.000	314	0				1
0.2	0.200	0.202	0.002	1337	0.0 %	1337					2
2.5	2.500	2.538	0.038	11007	0.0 %	11007					1
5.0	5.000	5.044	0.044	21383	0.0 %	21383					0
7.5	7.500	7.472	-0.028	31432	0.0 %	31432					0
10.0	10.000	9.989	-0.011	41852	0.0 %	41852					0

LB126529 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 20 Jul 2023 12:19:38

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	314	-	0.0000	7470A	PPB	20 Jul 2023 12:34:00	S	Std
0.2 - 1	50.2	1337	-	0.2000	7470A	PPB	20 Jul 2023 12:39:02	S	Std
2.5 - 1	52.5	11007	-	2.5000	7470A	PPB	20 Jul 2023 12:41:18	S	Std
5.0 - 1	55	21383	-	5.0000	7470A	PPB	20 Jul 2023 12:43:35	S	Std
7.5 - 1	57.5	31432	-	7.5000	7470A	PPB	20 Jul 2023 12:48:24	S	Std
10.0 - 1	510	41852	-	10.0000	7470A	PPB	20 Jul 2023 13:01:14	S	Std
ICV78 - 1	ICV78	17813	4.1820	-	7470A	PPB	20 Jul 2023 13:06:33	U	SMPL
ICB78 - 1	ICB78	107	-0.0950	-	7470A	PPB	20 Jul 2023 13:08:47	U	SMPL
CCV67 - 1	CCV67	20753	4.8922	-	7470A	PPB	20 Jul 2023 13:11:02	U	SMPL
CCB67 - 1	CCB67	178	-0.0779	-	7470A	PPB	20 Jul 2023 13:13:17	U	SMPL
CRA - 1	CRA	1291	0.1910	-	7470A	PPB	20 Jul 2023 13:15:32	U	SMPL
HighStd - 1	HighStd	41463	9.8948	-	7470A	PPB	20 Jul 2023 13:17:46	U	SMPL
ChkStd - 1	ChkStd	28402	6.7399	-	7470A	PPB	20 Jul 2023 13:20:01	U	SMPL
O3646-02 - 1	GATE-1	32	-0.1131	-	7470A	PPB	20 Jul 2023 13:26:50	U	SMPL
O3646-05 - 1	YARD-1	95	-0.0979	-	7470A	PPB	20 Jul 2023 13:29:06	U	SMPL
O3652-02 - 1	TP19	115	-0.0931	-	7470A	PPB	20 Jul 2023 13:31:23	U	SMPL
O3652-12 - 1	TP18	197	-0.0733	-	7470A	PPB	20 Jul 2023 13:33:40	U	SMPL
O3652-22 - 1	TP17	99	-0.0970	-	7470A	PPB	20 Jul 2023 13:35:56	U	SMPL
PB154289BL - 1	PBW	319	-0.0438	-	7470A	PPB	20 Jul 2023 13:38:28	U	SMPL
PB154289BS - 1	LCSW	18382	4.3195	-	7470A	PPB	20 Jul 2023 13:40:43	U	SMPL
CCV68 - 1	CCV68	22540	5.3238	-	7470A	PPB	20 Jul 2023 13:43:20	U	SMPL
CCB68 - 1	CCB68	245	-0.0617	-	7470A	PPB	20 Jul 2023 13:45:34	U	SMPL
O3653-02 - 1	TP20	69	-0.1042	-	7470A	PPB	20 Jul 2023 13:47:49	U	SMPL
O3653-12 - 1	TP21	140	-0.0870	-	7470A	PPB	20 Jul 2023 13:50:04	U	SMPL
O3653-22 - 1	TP22	175	-0.0786	-	7470A	PPB	20 Jul 2023 13:52:19	U	SMPL
O3654-02 - 1	72-12016	248	-0.0610	-	7470A	PPB	20 Jul 2023 13:54:35	U	SMPL
O3654-02DUP - 1	72-12016DUP	125	-0.0907	-	7470A	PPB	20 Jul 2023 13:56:51	U	SMPL
O3654-02MS - 1	72-12016MS	16563	3.8801	-	7470A	PPB	20 Jul 2023 14:03:57	U	SMPL
O3654-02MSD - 1	72-12016MSD	18035	4.2356	-	7470A	PPB	20 Jul 2023 14:06:15	U	SMPL
O3654-02LX5 - 1		22	-0.1156	-	7470A	PPB	20 Jul 2023 14:10:49	U	SMPL
O3654-02A - 1		18787	4.4173	-	7470A	PPB	20 Jul 2023 14:13:04	U	SMPL
PB154272TB - 1	PB154272TB	496	-0.0011	-	7470A	PPB	20 Jul 2023 14:30:20	U	SMPL
CCV69 - 1	CCV69	23228	5.4900	-	7470A	PPB	20 Jul 2023 14:32:53	U	SMPL
CCB69 - 1	CCB69	333	-0.0404	-	7470A	PPB	20 Jul 2023 14:35:08	U	SMPL