


L3126548

7470A

INSTRUMENT 1A: CV1

Linear

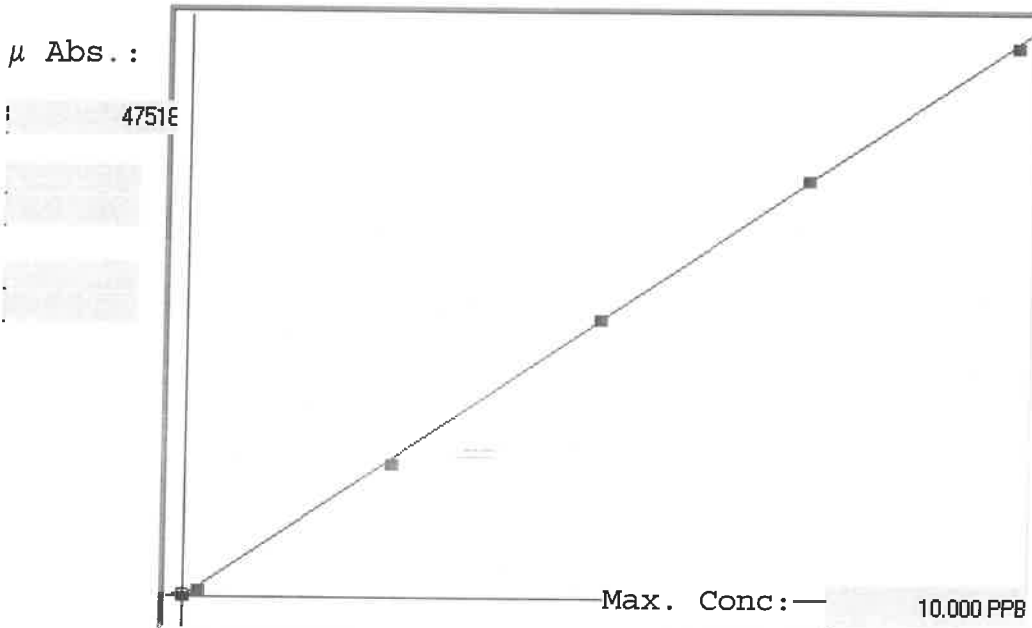

A= 0.0000e+000

B= 2.0919e-004

C= 1.3360e-002

Rho= 0.9999013

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.053	0.053	189	0.000	189	0				0/00
0.2	0.200	0.163	-0.037	716	0.0 %	716					-19
2.5	2.500	2.430	-0.070	11554	0.0 %	11554					-3
5.0	5.000	5.048	0.048	24069	0.0 %	24069					1
7.5	7.500	7.551	0.051	36034	0.0 %	36034					1
10.0	10.000	9.954	-0.046	47518	0.0 %	47518					0

LB126548 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 21 Jul 2023 11:48:33

Sample ID	Extended ID	μ Abs.	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	189	-	0.0000	7470A	PPB	21 Jul 2023 11:51:22	S	Std
0.2 - 1	50.2	716	-	0.2000	7470A	PPB	21 Jul 2023 11:53:39	S	Std
2.5 - 1	52.5	11554	-	2.5000	7470A	PPB	21 Jul 2023 11:55:55	S	Std
5.0 - 1	55	24069	-	5.0000	7470A	PPB	21 Jul 2023 12:03:20	S	Std
7.5 - 1	57.5	36034	-	7.5000	7470A	PPB	21 Jul 2023 12:05:35	S	Std
10.0 - 1	510	47518	-	10.0000	7470A	PPB	21 Jul 2023 12:18:19	S	Std
ICV80 - 1	ICV80	20345	4.2694	-	7470A	PPB	21 Jul 2023 12:23:39	U	SMPL
ICB80 - 1	ICB80	87	0.0316	-	7470A	PPB	21 Jul 2023 12:25:54	U	SMPL
CCV76 - 1	CCV76	23841	5.0007	-	7470A	PPB	21 Jul 2023 12:28:09	U	SMPL
CCB76 - 1	CCB76	86	0.0314	-	7470A	PPB	21 Jul 2023 12:30:23	U	SMPL
CRA - 1	CRA	975	0.2173	-	7470A	PPB	21 Jul 2023 12:35:07	U	SMPL
HighStd - 1	HighStd	46842	9.8124	-	7470A	PPB	21 Jul 2023 12:37:22	U	SMPL
ChkStd - 1	ChkStd	33707	7.0646	-	7470A	PPB	21 Jul 2023 12:39:37	U	SMPL
PB154355BL - 1	PBW	-23	0.0085	-	7470A	PPB	21 Jul 2023 12:41:52	U	SMPL
PB154355BS - 1	LCSW	18594	3.9031	-	7470A	PPB	21 Jul 2023 12:46:53	U	SMPL
O3664-03 - 1	AUD-1007	148	0.0443	-	7470A	PPB	21 Jul 2023 12:53:35	U	SMPL
O3664-03DUP - 1	AUD-1007DUP	94	0.0330	-	7470A	PPB	21 Jul 2023 12:55:50	U	SMPL
O3664-03MS - 1	AUD-1007MS	17585	3.6920	-	7470A	PPB	21 Jul 2023 12:58:07	U	SMPL
O3664-03MSD - 1	AUD-1007MSD	17764	3.7295	-	7470A	PPB	21 Jul 2023 13:03:09	U	SMPL
O3664-04 - 1	AUD-1013	63	0.0265	-	7470A	PPB	21 Jul 2023 13:05:23	U	SMPL
CCV77 - 1	CCV77	23733	4.9781	-	7470A	PPB	21 Jul 2023 13:07:39	U	SMPL
CCB77 - 1	CCB77	128	0.0401	-	7470A	PPB	21 Jul 2023 13:09:54	U	SMPL
O3664-05 - 1	AUD-1012	7425	1.5666	-	7470A	PPB	21 Jul 2023 13:12:09	U	SMPL
O3664-06 - 1	AUD-1022	1413	0.3089	-	7470A	PPB	21 Jul 2023 13:14:25	U	SMPL
O3664-07 - 1	A462	6523	1.3779	-	7470A	PPB	21 Jul 2023 13:16:40	U	SMPL
O3668-05 - 1	N48719	38	0.0213	-	7470A	PPB	21 Jul 2023 13:18:57	U	SMPL
O3670-01 - 1	N48909	352	0.0870	-	7470A	PPB	21 Jul 2023 13:21:12	U	SMPL
O3683-01 - 1	NORTH-TURNPIKE	84163	17.6196	-	7470A	PPB	21 Jul 2023 13:23:28	U	SMPL
O3688-01 - 1	FMI-123	39	0.0215	-	7470A	PPB	21 Jul 2023 13:25:45	U	SMPL
O3706-10 - 1	FB02	43	0.0224	-	7470A	PPB	21 Jul 2023 13:28:03	U	SMPL
O3664-03LX5 - 1		-36	0.0058	-	7470A	PPB	21 Jul 2023 13:30:19	U	SMPL
O3664-03A - 1		17919	3.7619	-	7470A	PPB	21 Jul 2023 13:32:35	U	SMPL
CCV78 - 1	CCV78	23808	4.9938	-	7470A	PPB	21 Jul 2023 13:34:50	U	SMPL
CCB78 - 1	CCB78	67	0.0274	-	7470A	PPB	21 Jul 2023 13:37:05	U	SMPL
O3683-01DLX5 - 1		19401	4.0719	-	7470A	PPB	21 Jul 2023 13:39:21	U	SMPL
CCV79 - 1	CCV79	23838	5.0001	-	7470A	PPB	21 Jul 2023 13:41:37	U	SMPL
CCB79 - 1	CCB79	152	0.0452	-	7470A	PPB	21 Jul 2023 13:43:52	U	SMPL